

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
 Data File : VU057820.D
 Acq On : 06 Feb 2024 14:16
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Feb 07 03:00:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 06 02:05:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.107	96	41964	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	13527	0.878	ug/l	0.00
Spiked Amount 1.000			Recovery	=	88.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	11683	0.858	ug/l	0.00
Spiked Amount 1.000			Recovery	=	86.000%	
Target Compounds						
15) Methylene Chloride	3.036	84	14599	1.126	ug/l	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057820.D
Acq On : 06 Feb 2024 14:16
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Feb 07 03:00:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 06 02:05:40 2024
Response via : Initial Calibration




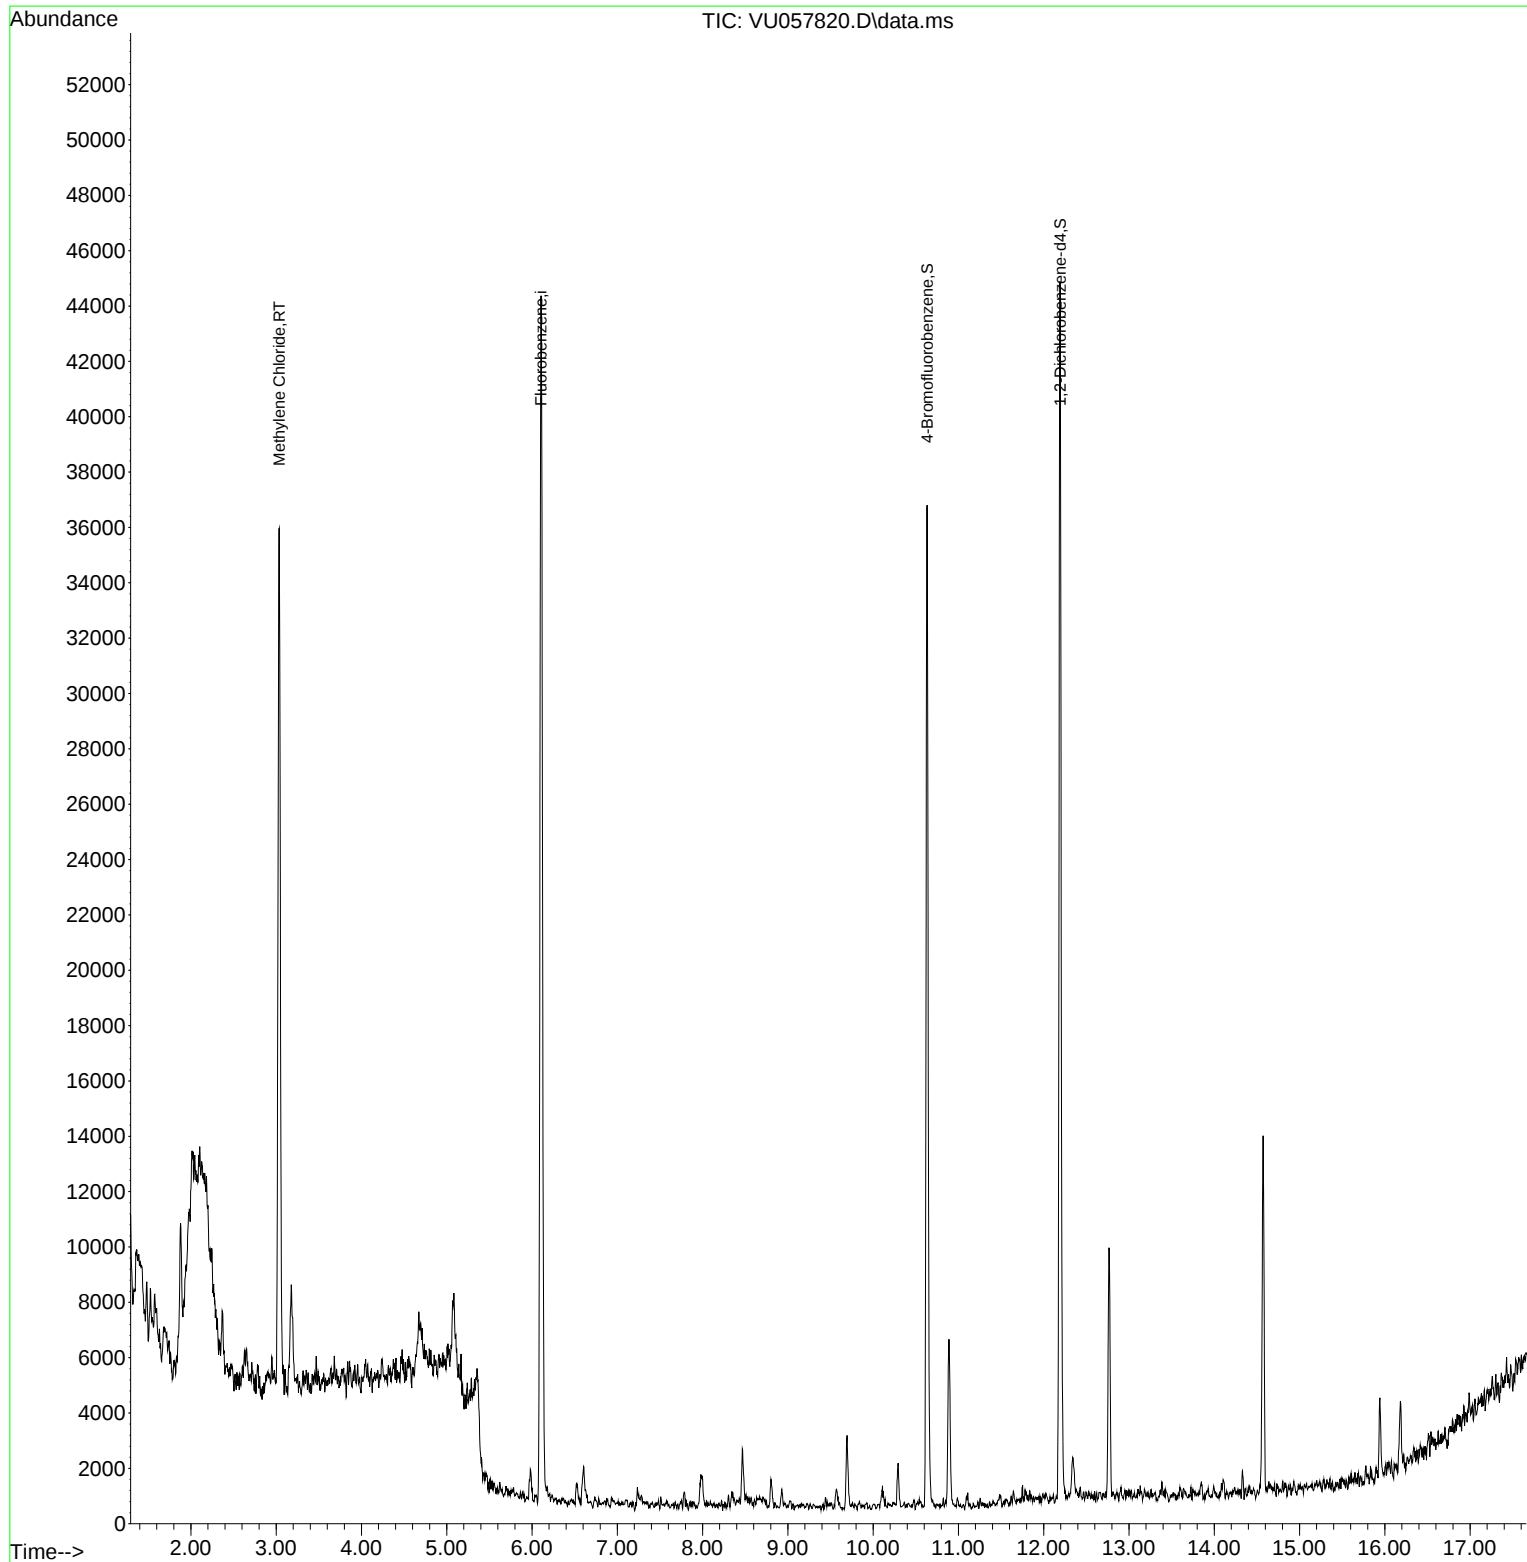


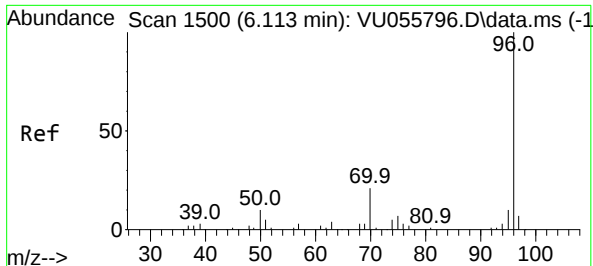

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 14
Delta R.T. 0.004 min
Lab File: VU057820.D
Acq: 06 Feb 2024 14:16




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion: 96	Resp: 41964
Ion Ratio	Lower Upper
96 100	
70 21.6	16.5 24.7
95 8.3	7.4 11.0
97 6.7	0.0 0.0

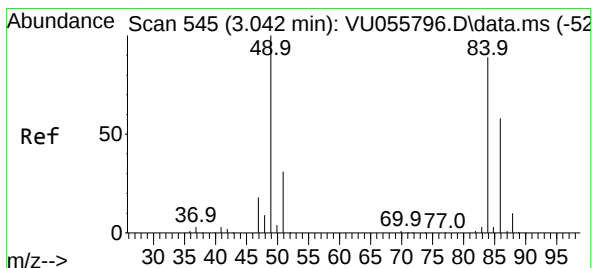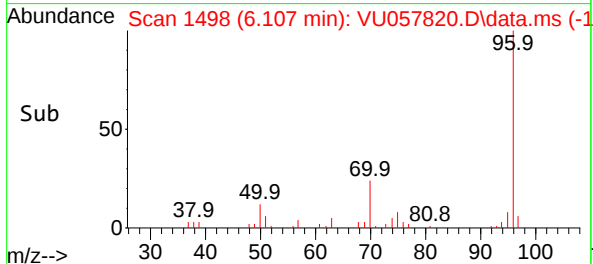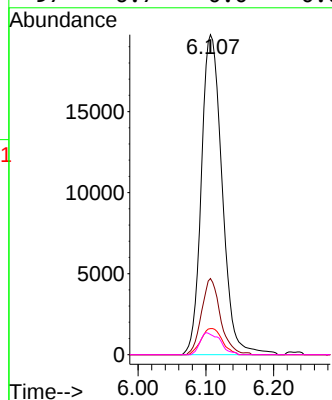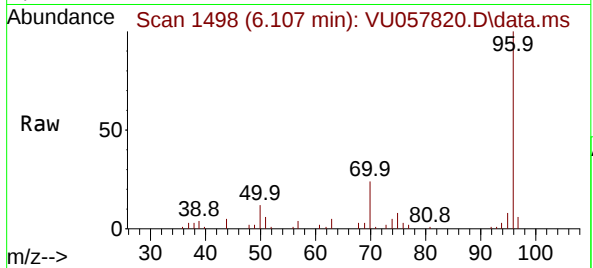

#15
Methylene Chloride
Concen: 1.126 ug/l
RT: 3.036 min Scan# 543
Delta R.T. 0.010 min
Lab File: VU057820.D
Acq: 06 Feb 2024 14:16

Tgt Ion: 84	Resp: 14599
Ion Ratio	Lower Upper
84 100	
49 126.8	98.9 148.3
51 39.4	0.0 75.4
86 66.8	51.3 76.9


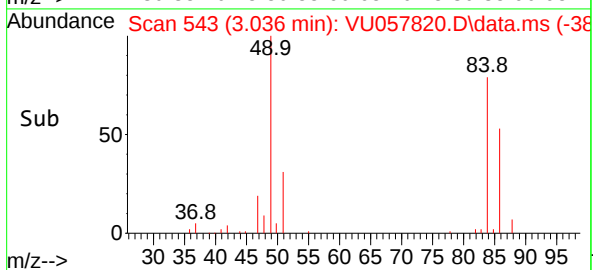
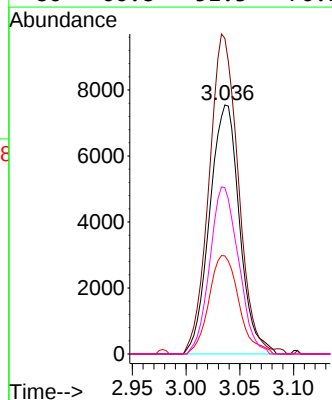
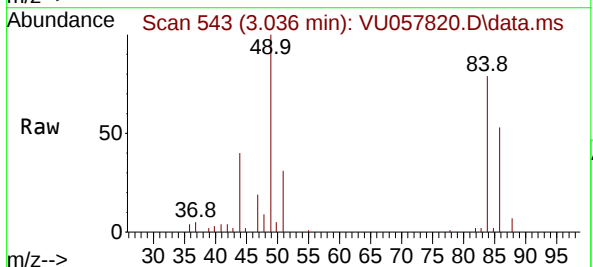


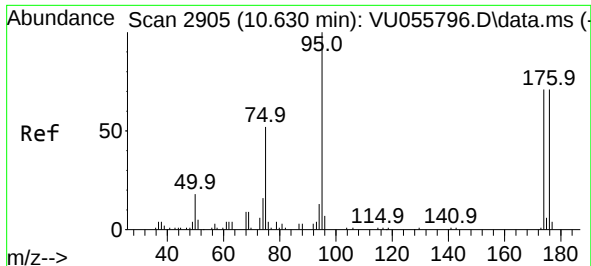

#57
4-Bromofluorobenzene
Concen: 0.878 ug/l
RT: 10.634 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU057820.D
Acq: 06 Feb 2024 14:16

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Tgt Ion: 95 Resp: 13527
Ion Ratio Lower Upper
95 100
174 70.7 63.3 94.9
176 69.0 59.3 88.9

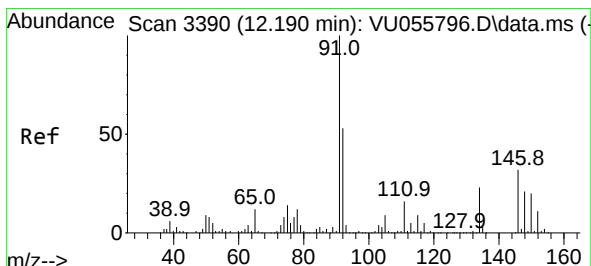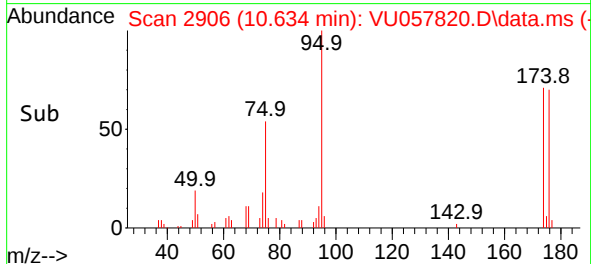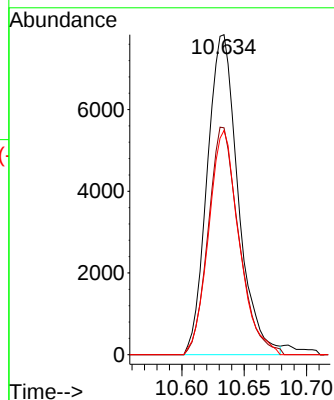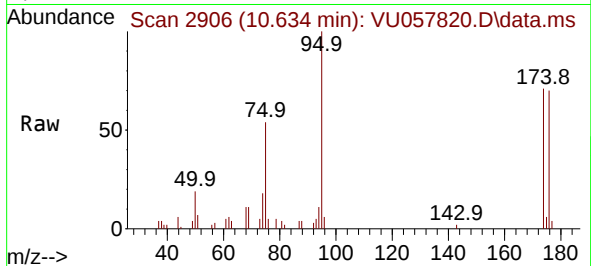

#68
1,2-Dichlorobenzene-d4
Concen: 0.858 ug/l
RT: 12.193 min Scan# 3391
Delta R.T. 0.000 min
Lab File: VU057820.D
Acq: 06 Feb 2024 14:16

Tgt Ion: 152 Resp: 11683
Ion Ratio Lower Upper
152 100
115 69.8 0.0 308.8
150 165.3 0.0 635.0

