

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
 Data File : VU057825.D
 Acq On : 06 Feb 2024 17:11
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Feb 07 03:02:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 06 02:05:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.107	96	40602	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	13202	0.886	ug/l	0.00
Spiked Amount	1.000		Recovery	=	89.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	12004	0.911	ug/l	0.00
Spiked Amount	1.000		Recovery	=	91.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057825.D
Acq On : 06 Feb 2024 17:11
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Feb 07 03:02:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 06 02:05:40 2024
Response via : Initial Calibration




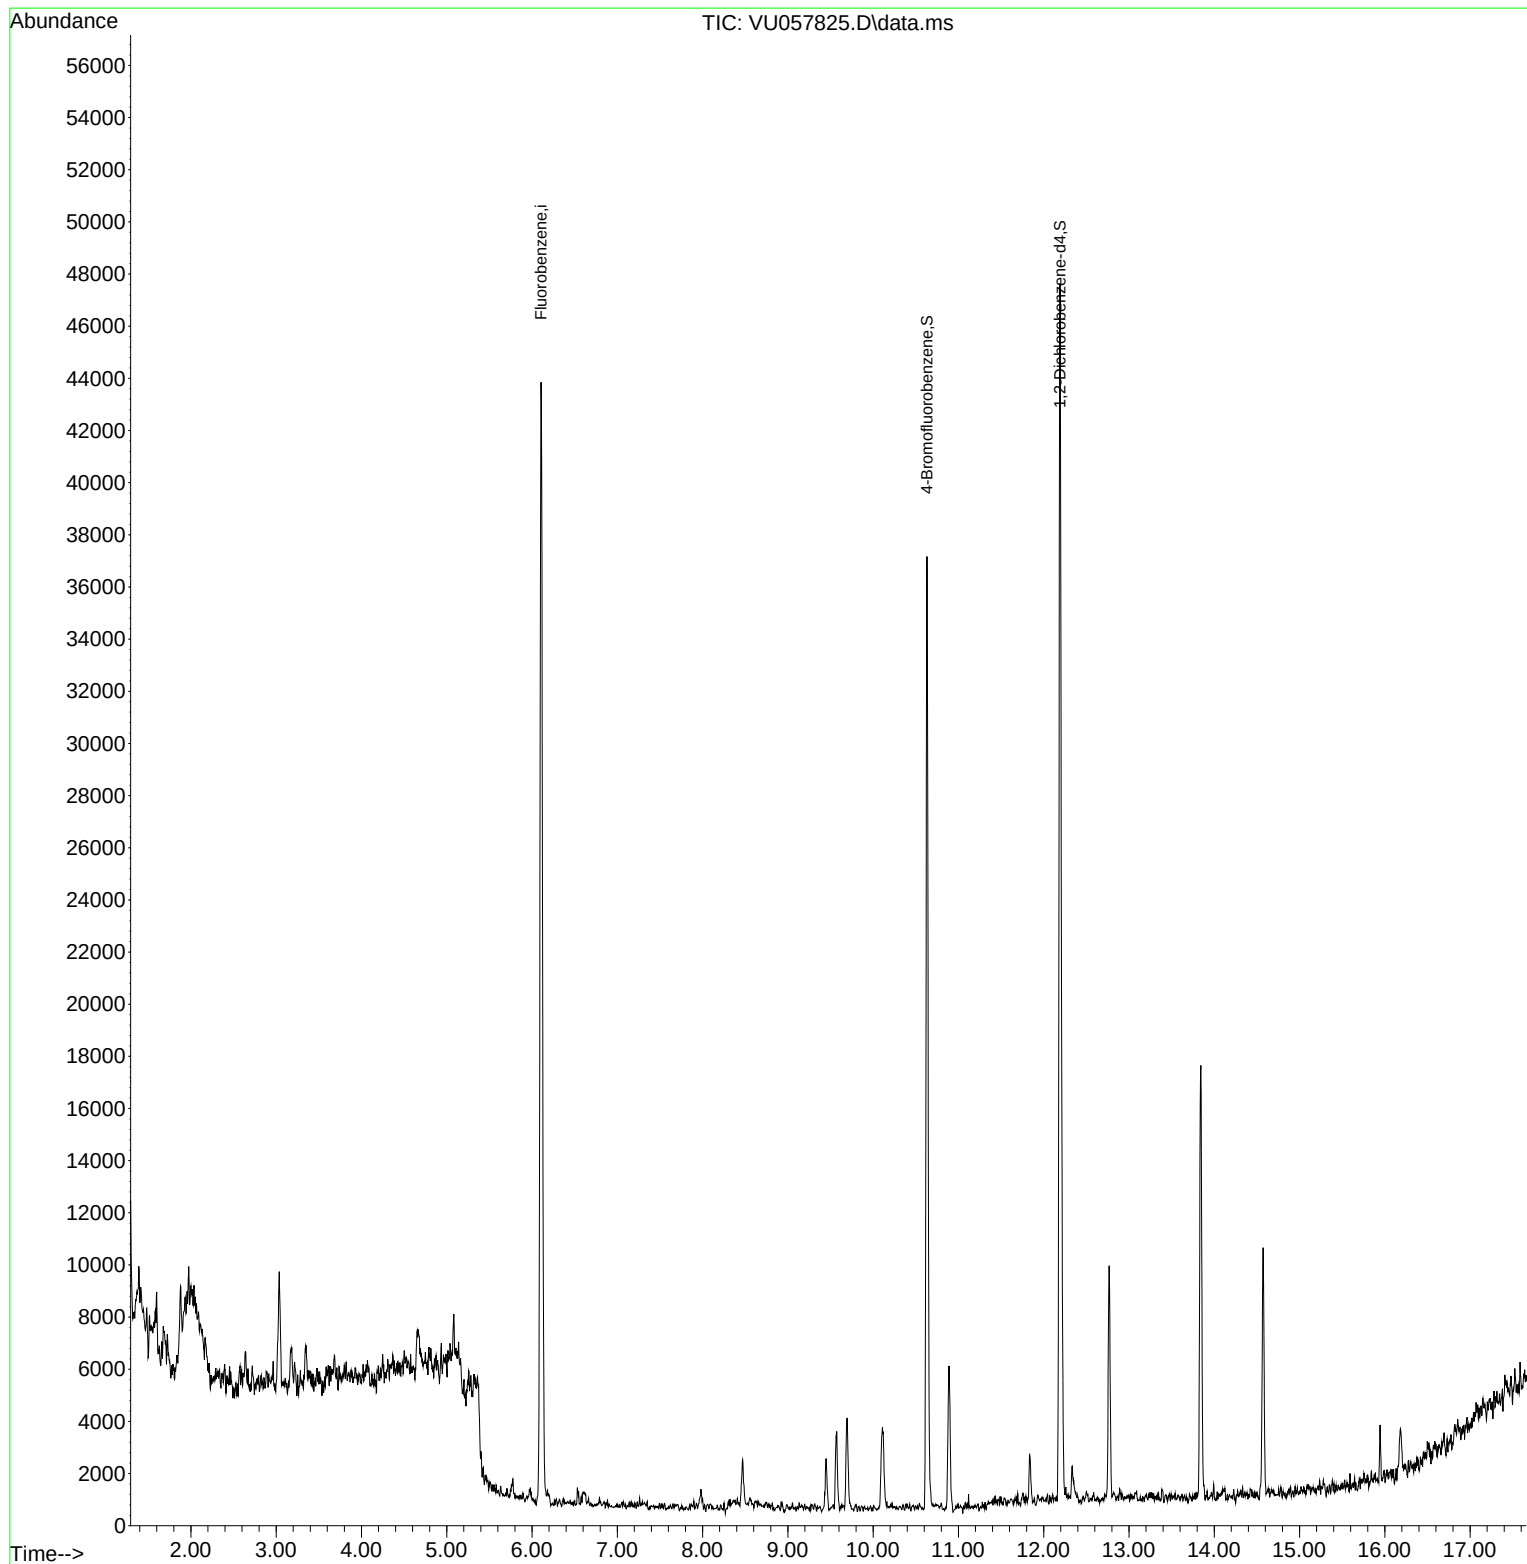


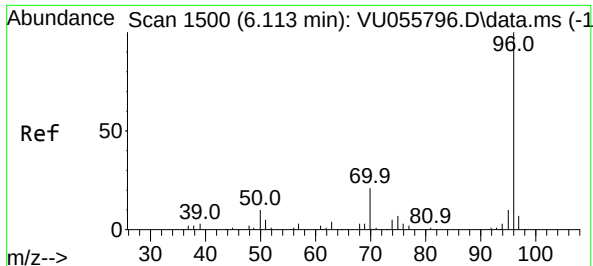

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 1498
Delta R.T. 0.004 min
Lab File: VU057825.D
Acq: 06 Feb 2024 17:11




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion: 96	Resp: 40602
Ion Ratio	Lower Upper
96 100	
70 21.2	16.5 24.7
95 8.4	7.4 11.0
97 6.6	0.0 0.0

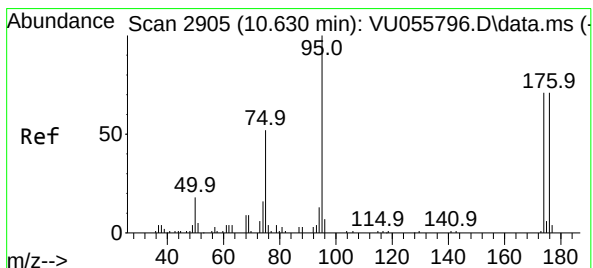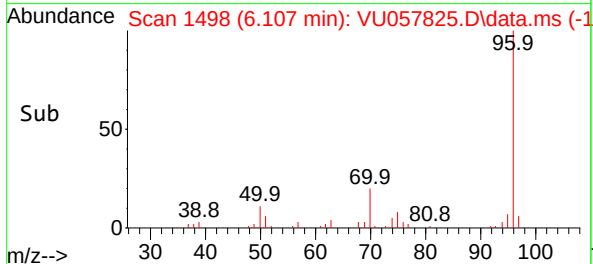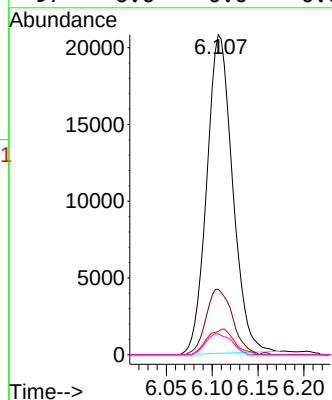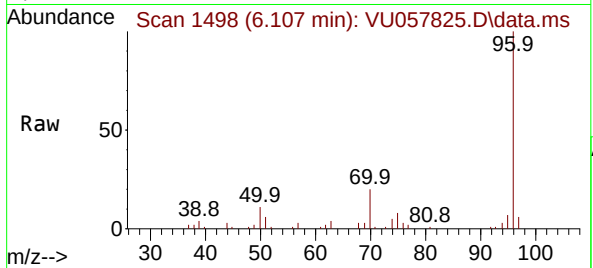

#57
4-Bromofluorobenzene
Concen: 0.886 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.000 min
Lab File: VU057825.D
Acq: 06 Feb 2024 17:11


Tgt Ion: 95	Resp: 13202
Ion Ratio	Lower Upper
95 100	
174 70.1	63.3 94.9
176 72.2	59.3 88.9

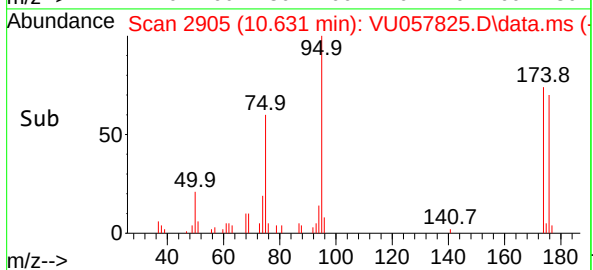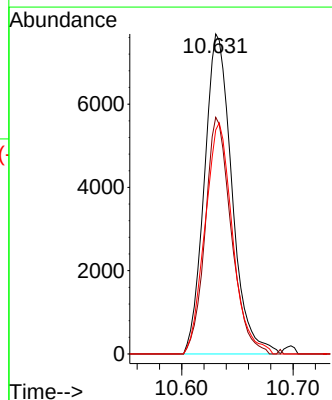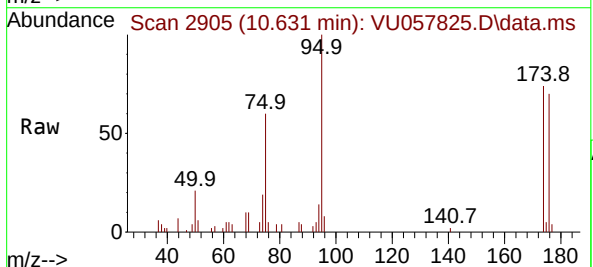

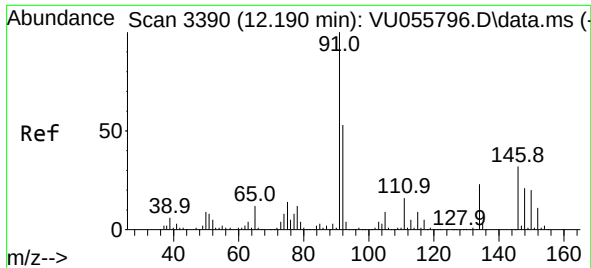

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.911 ug/l
 RT: 12.190 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VU057825.D
 Acq: 06 Feb 2024 17:11

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

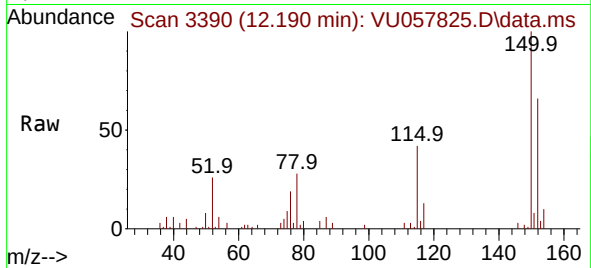

Tgt Ion:	152	Resp:	12004
Ion Ratio	Lower	Upper	
152	100		
115	65.7	0.0	308.8
150	158.7	0.0	635.0

