

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
 Data File : VU057813.D
 Acq On : 06 Feb 2024 10:11
 Operator : MD/SY
 Sample : VU0206WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0206WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU057813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	265	268	273	rBV3	1430	1596	1.72%	0.507%
2	3.036	536	543	549	rBV5	1753	3110	3.36%	0.988%
3	6.110	1486	1499	1520	rBV	46753	92531	100.00%	29.382%
4	8.466	2222	2232	2239	rBV4	1822	2925	3.16%	0.929%
5	9.698	2607	2615	2624	rBV3	1364	2403	2.60%	0.763%
6	10.630	2894	2905	2926	rVB2	38615	63509	68.64%	20.167%
7	10.888	2976	2985	2996	rBV3	5598	9802	10.59%	3.113%
8	11.646	3208	3221	3226	rBV3	714	1255	1.36%	0.399%
9	11.788	3260	3265	3273	rVV2	841	1066	1.15%	0.338%
10	11.839	3273	3281	3290	rVB4	1611	2169	2.34%	0.689%
11	12.190	3378	3390	3410	rBV	43491	78683	85.03%	24.985%
12	12.335	3426	3435	3443	rBV5	2439	4751	5.13%	1.509%
13	12.769	3556	3570	3579	rBV2	8243	13506	14.60%	4.289%
14	13.842	3896	3904	3916	rBV6	2807	4592	4.96%	1.458%
15	14.097	3975	3983	3985	rBV	2159	2592	2.80%	0.823%
16	14.331	4049	4056	4067	rVB5	2915	4560	4.93%	1.448%
17	14.572	4119	4131	4142	rBV	9694	15262	16.49%	4.846%
18	15.939	4549	4556	4567	rVV9	6646	10608	11.46%	3.368%




Sum of corrected areas: 314920

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057813.D
Acq On : 06 Feb 2024 10:11
Operator : MD/SY
Sample : VU0206WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0206WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

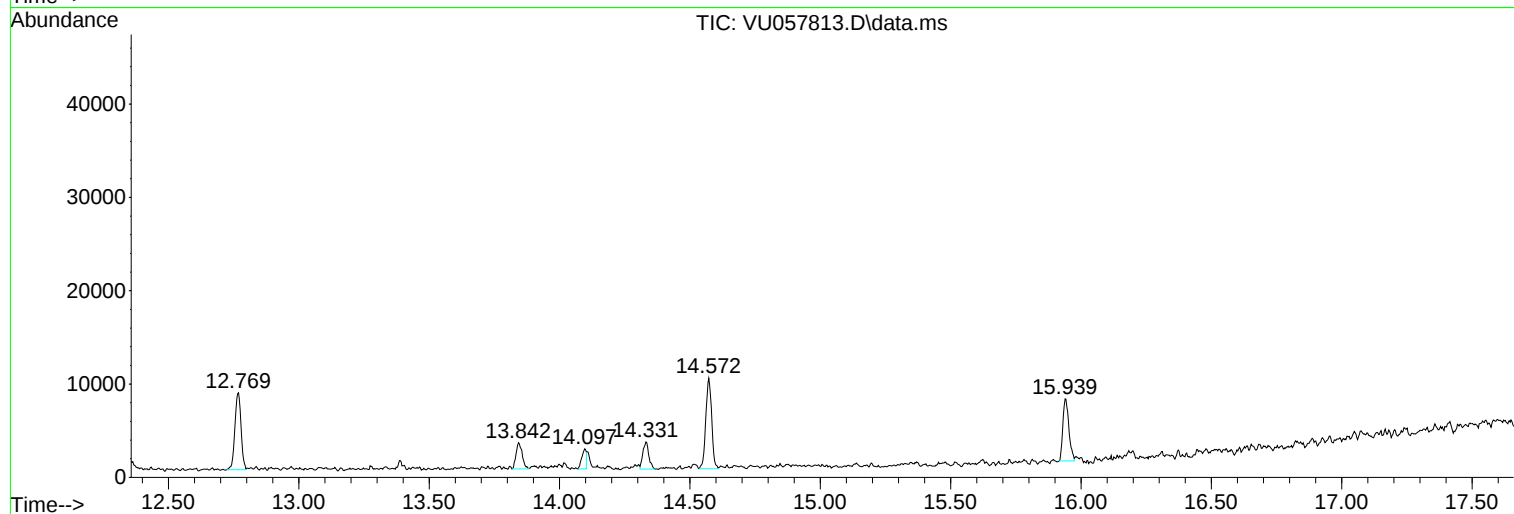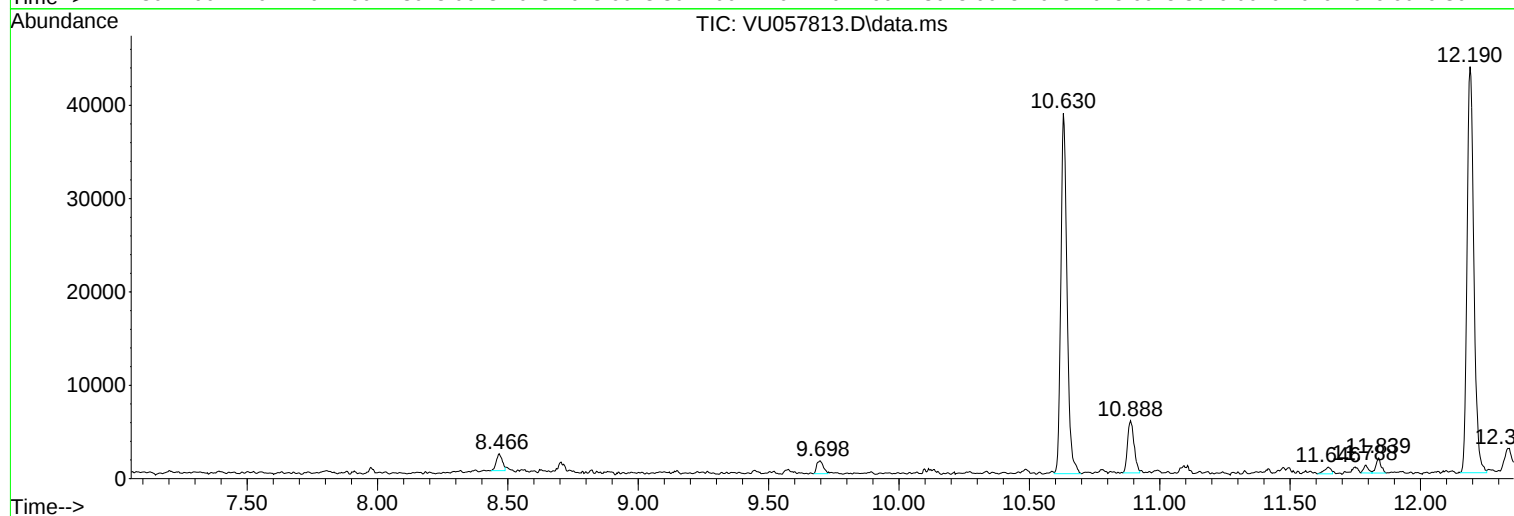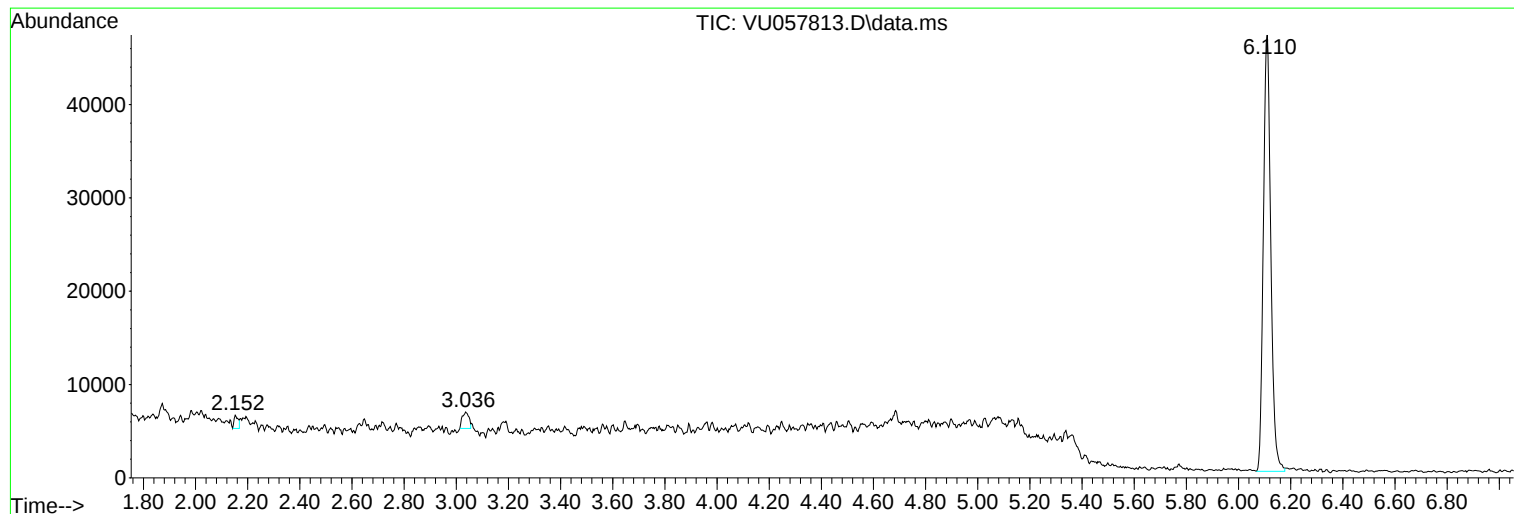

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057813.D
Acq On : 06 Feb 2024 10:11
Operator : MD/SY
Sample : VU0206WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0206WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057813.D
Acq On : 06 Feb 2024 10:11
Operator : MD/SY
Sample : VU0206WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0206WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------