

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057819.D
Acq On : 06 Feb 2024 13:46
Operator : MD/SY
Sample : P1174-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU057819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.033	532	542	554	rBV2	22895	41128	1.35%	0.647%
2	5.078	1161	1178	1213	rBV	1409280	3051879	100.00%	48.003%
3	6.107	1485	1498	1517	rBV	46105	90161	2.95%	1.418%
4	7.100	1793	1807	1827	rBV	259288	476558	15.62%	7.496%
5	8.804	2320	2337	2369	rBV	799628	1368132	44.83%	21.519%
6	10.287	2784	2798	2835	rBV	693939	1182875	38.76%	18.606%
7	10.631	2893	2905	2922	rBV2	38590	64459	2.11%	1.014%
8	12.193	3380	3391	3406	rBV	47091	82467	2.70%	1.297%




Sum of corrected areas: 6357659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057819.D
Acq On : 06 Feb 2024 13:46
Operator : MD/SY
Sample : P1174-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

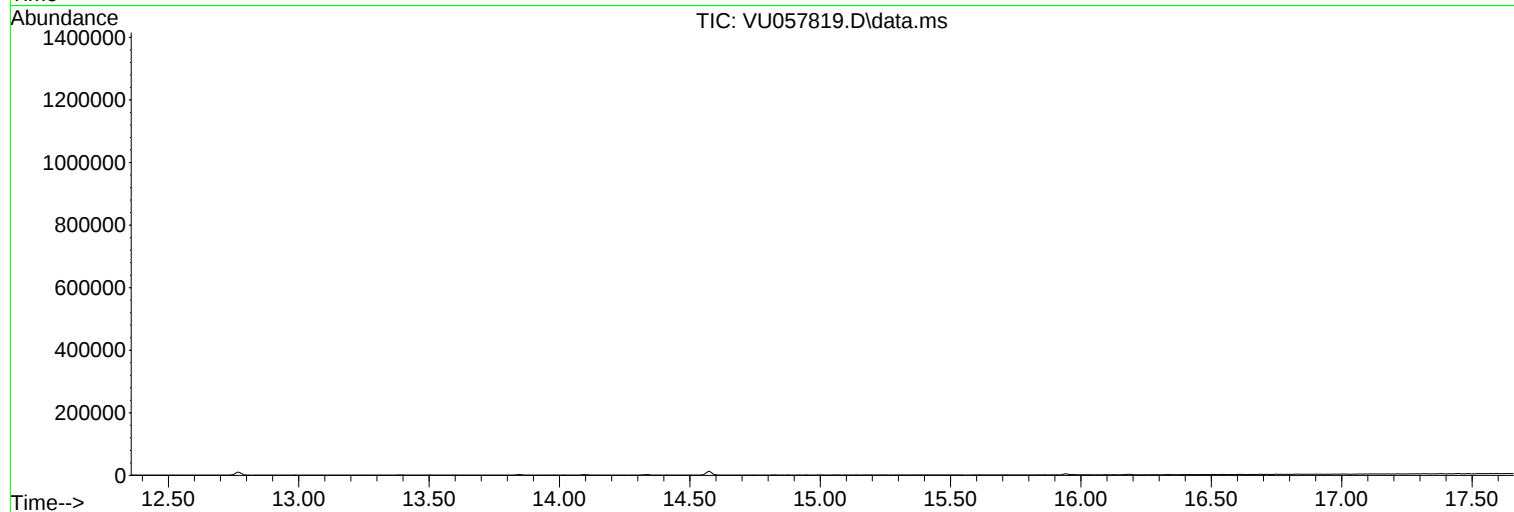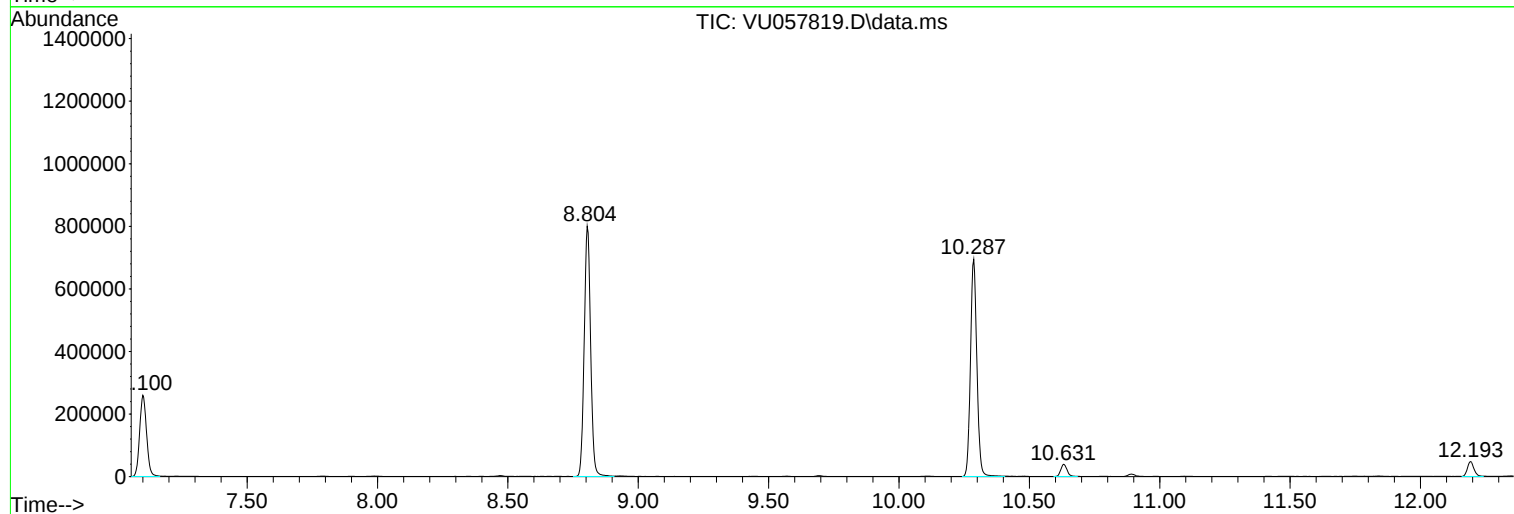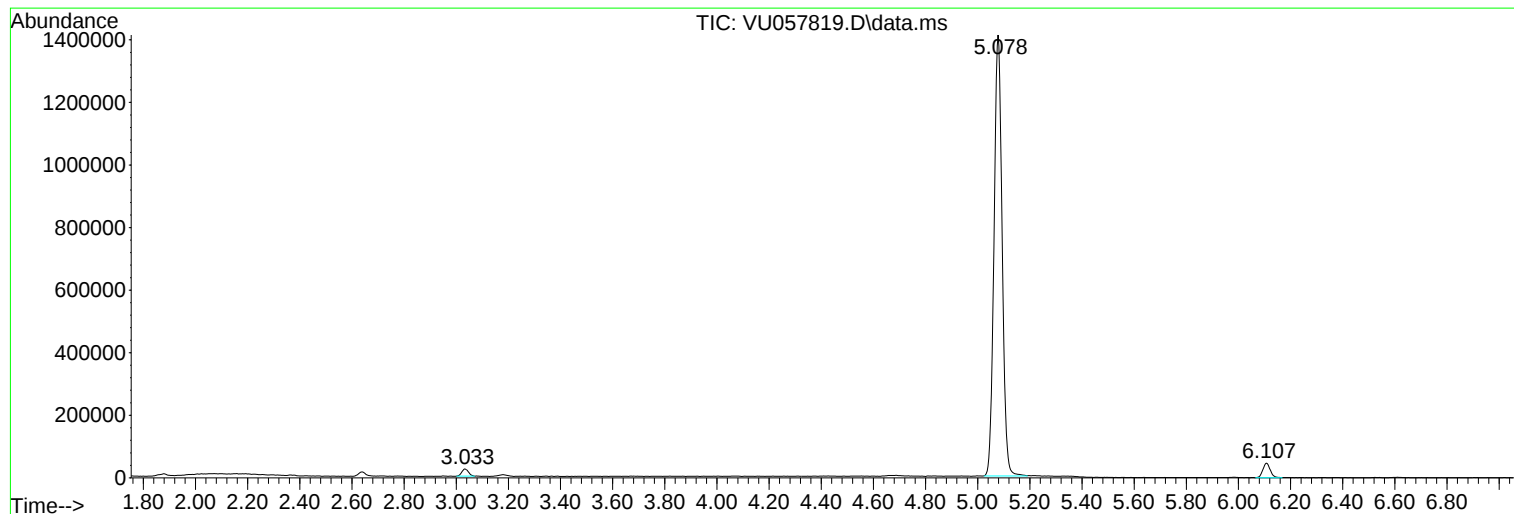

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057819.D
Acq On : 06 Feb 2024 13:46
Operator : MD/SY
Sample : P1174-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057819.D
Acq On : 06 Feb 2024 13:46
Operator : MD/SY
Sample : P1174-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------