

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
 Data File : VU057824.D
 Acq On : 06 Feb 2024 16:41
 Operator : MD/SY
 Sample : P1174-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU057824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.573	386	399	416	rBV	517887	841641	24.47%	4.009%
2	3.036	529	543	565	rBV	300046	562734	16.36%	2.681%
3	3.341	624	638	660	rBV	407669	801131	23.29%	3.816%
4	4.656	1032	1047	1068	rBV	280362	636821	18.52%	3.033%
5	5.303	1232	1248	1277	rVB	413653	939444	27.32%	4.475%
6	5.512	1295	1313	1335	rVB	308756	668125	19.43%	3.183%
7	5.763	1375	1391	1424	rBV	495896	1104556	32.12%	5.262%
8	6.107	1484	1498	1516	rBV2	51627	101963	2.96%	0.486%
9	6.534	1617	1631	1651	rBV	327142	614088	17.86%	2.925%
10	6.785	1694	1709	1733	rBV	562227	1068913	31.08%	5.092%
11	7.965	2062	2076	2102	rBV	222617	385722	11.22%	1.837%
12	8.396	2197	2210	2227	rBV	282563	487718	14.18%	2.323%
13	8.547	2246	2257	2275	rVB	114069	194055	5.64%	0.924%
14	9.441	2520	2535	2561	rBV	744774	1230672	35.78%	5.862%
15	9.563	2561	2573	2598	rVV	1580019	2544534	73.98%	12.121%
16	9.688	2599	2612	2646	rVB	1337365	2212683	64.34%	10.540%
17	10.097	2725	2739	2779	rBV4	1779210	3439276	100.00%	16.383%
18	10.630	2895	2905	2924	rVB3	47129	75271	2.19%	0.359%
19	11.830	3267	3278	3293	rBV	193374	309229	8.99%	1.473%
20	12.206	3378	3395	3428	rBV	987069	1656191	48.16%	7.889%
21	13.836	3889	3902	3924	rBV	690710	1118407	32.52%	5.327%




Sum of corrected areas: 20993174

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057824.D
Acq On : 06 Feb 2024 16:41
Operator : MD/SY
Sample : P1174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

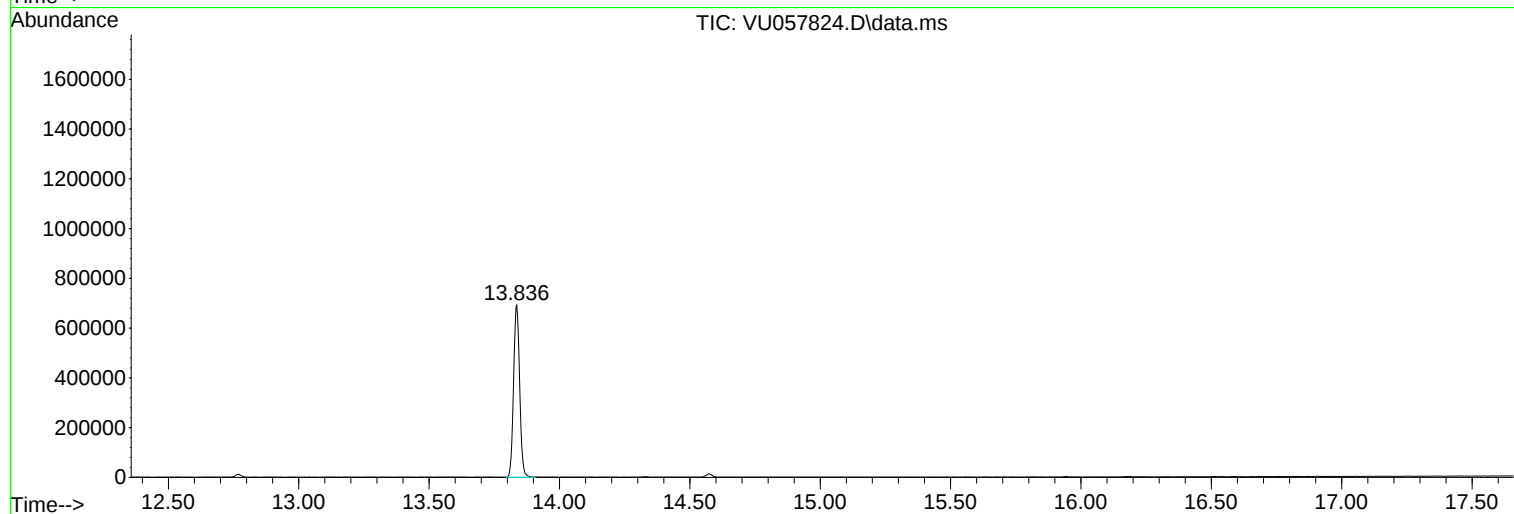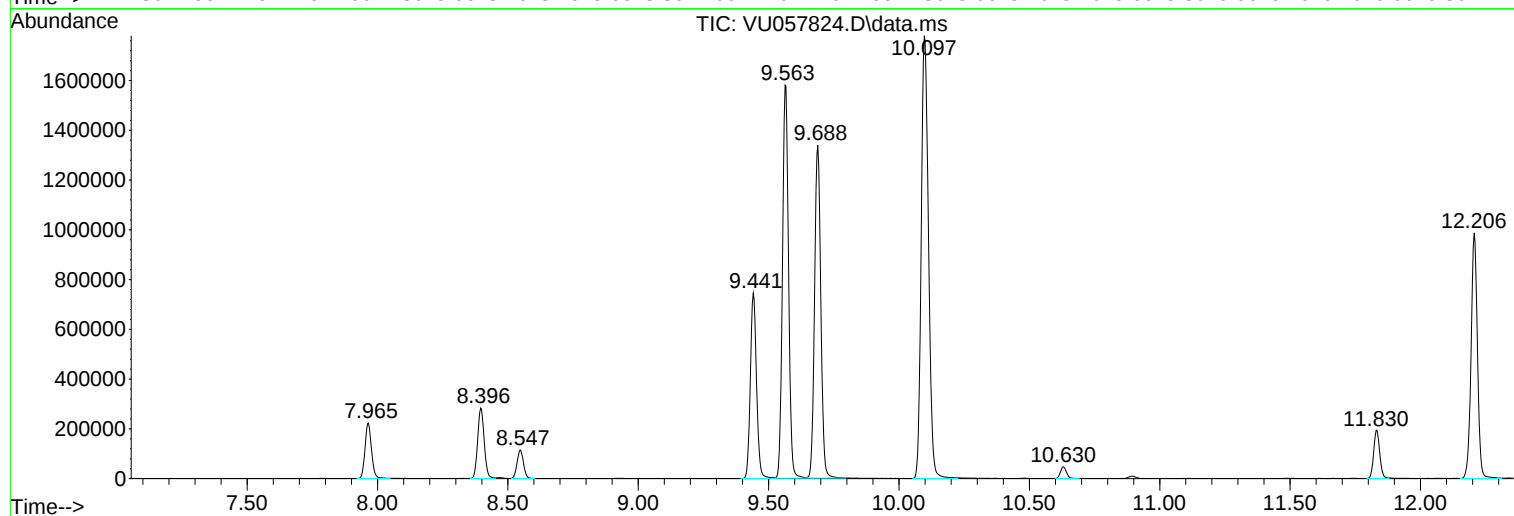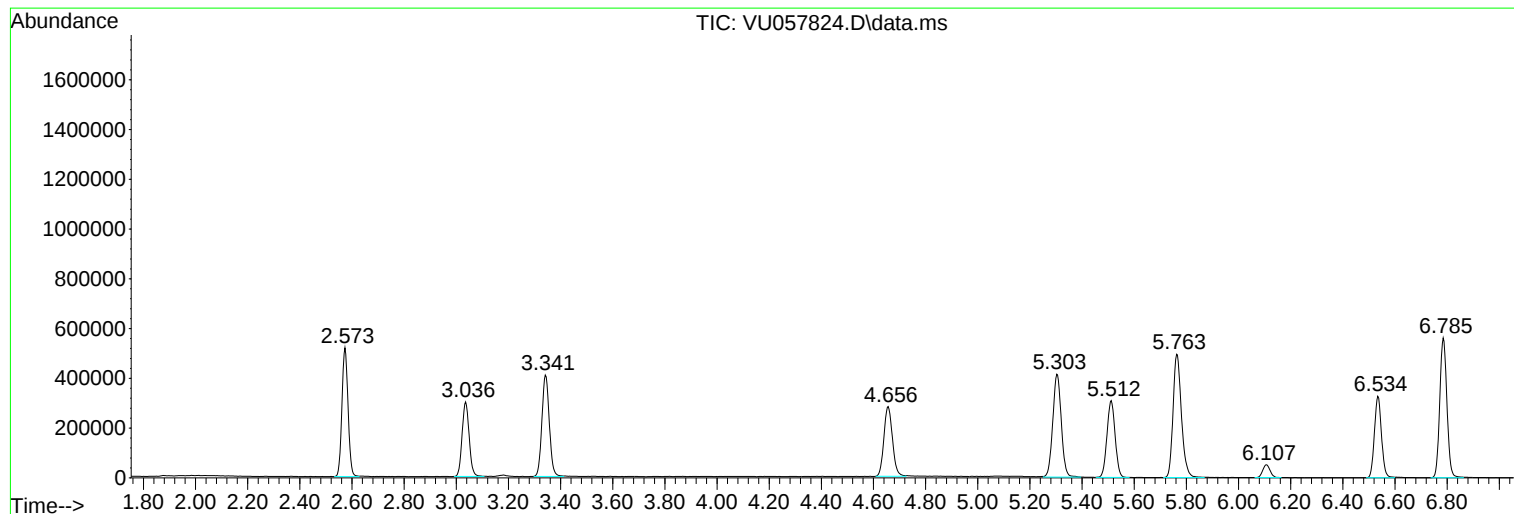

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057824.D
Acq On : 06 Feb 2024 16:41
Operator : MD/SY
Sample : P1174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057824.D
Acq On : 06 Feb 2024 16:41
Operator : MD/SY
Sample : P1174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------