

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
 Data File : VU057826.D
 Acq On : 06 Feb 2024 17:42
 Operator : MD/SY
 Sample : P1174-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU057826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.853	166	175	193	rBV	259415	355758	12.04%	1.082%
2	2.133	250	262	283	rBV	1517952	2211643	74.87%	6.729%
3	3.358	625	643	677	rBV	1244717	2882365	97.57%	8.770%
4	3.859	782	799	820	rVB	348373	818534	27.71%	2.491%
5	4.653	1029	1046	1068	rBV	200029	495413	16.77%	1.507%
6	4.965	1127	1143	1167	rBV	246205	536022	18.15%	1.631%
7	5.515	1298	1314	1334	rBV	164452	335083	11.34%	1.020%
8	6.107	1482	1498	1517	rBV	44627	87279	2.95%	0.266%
9	6.914	1737	1749	1779	rBV	188414	356557	12.07%	1.085%
10	7.602	1950	1963	1993	rBV	500964	877505	29.71%	2.670%
11	8.206	2138	2151	2182	rBV	230711	404485	13.69%	1.231%
12	8.570	2250	2264	2286	rBV	210962	372747	12.62%	1.134%
13	9.528	2549	2562	2584	rBV	324964	544660	18.44%	1.657%
14	10.479	2845	2858	2877	rBV	600354	933291	31.59%	2.840%
15	10.631	2895	2905	2925	rVB	43231	69216	2.34%	0.211%
16	10.775	2938	2950	2960	rBV	382897	648185	21.94%	1.972%
17	10.901	2976	2989	3003	rBV	1646807	2531334	85.69%	7.702%
18	10.981	3003	3014	3031	rVV	363379	577334	19.54%	1.757%
19	11.084	3033	3046	3068	rVV2	1819948	2866481	97.04%	8.722%
20	11.412	3135	3148	3155	rBV	277202	440674	14.92%	1.341%
21	11.463	3155	3164	3189	rVB	1605797	2463033	83.38%	7.494%
22	11.637	3203	3218	3234	rBV	693251	1065400	36.07%	3.242%
23	11.740	3238	3250	3257	rBV	546909	870825	29.48%	2.650%
24	11.788	3257	3265	3287	rVB	1964465	2954012	100.00%	8.988%
25	12.203	3378	3394	3423	rBV	1859200	2817235	95.37%	8.572%
26	14.016	3945	3958	3968	rBV	1275186	1975147	66.86%	6.010%
27	14.081	3968	3978	4003	rVB	813059	1292652	43.76%	3.933%
28	14.325	4040	4054	4072	rBV	664559	1082518	36.65%	3.294%




Sum of corrected areas: 32865388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057826.D
Acq On : 06 Feb 2024 17:42
Operator : MD/SY
Sample : P1174-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

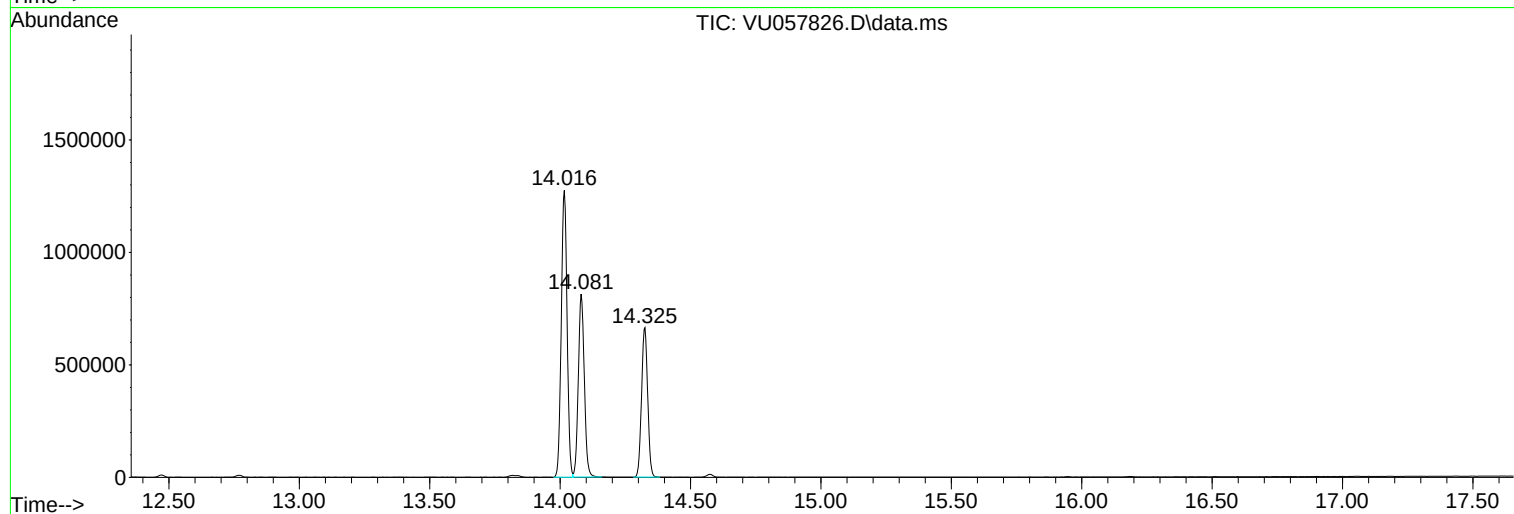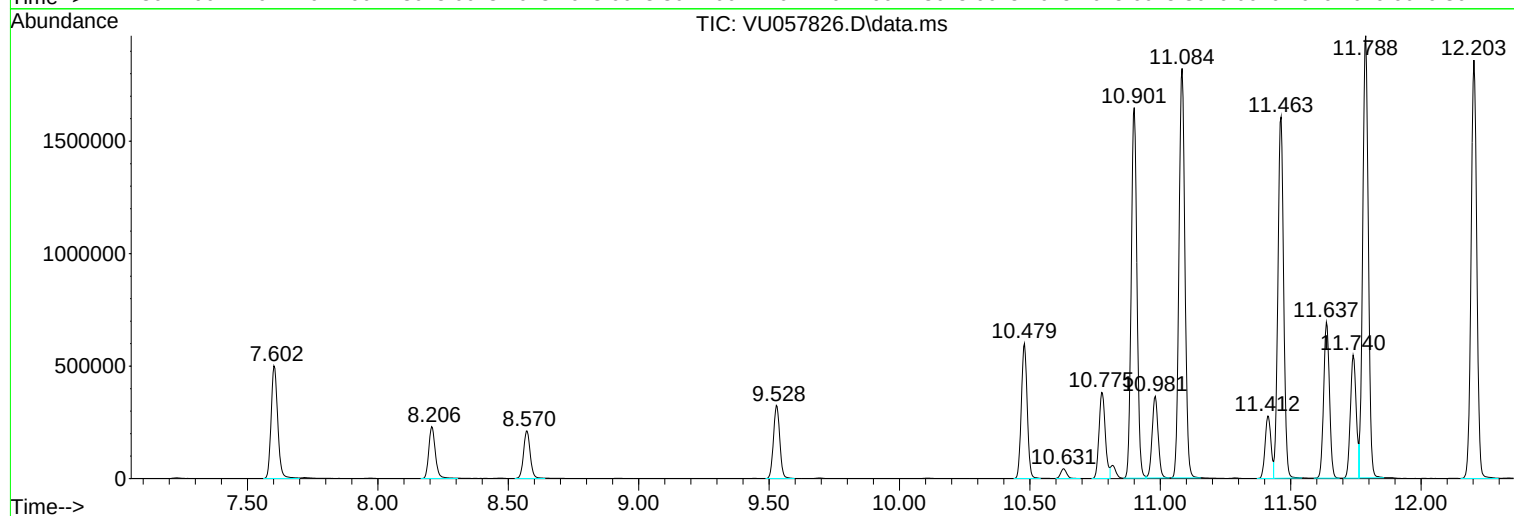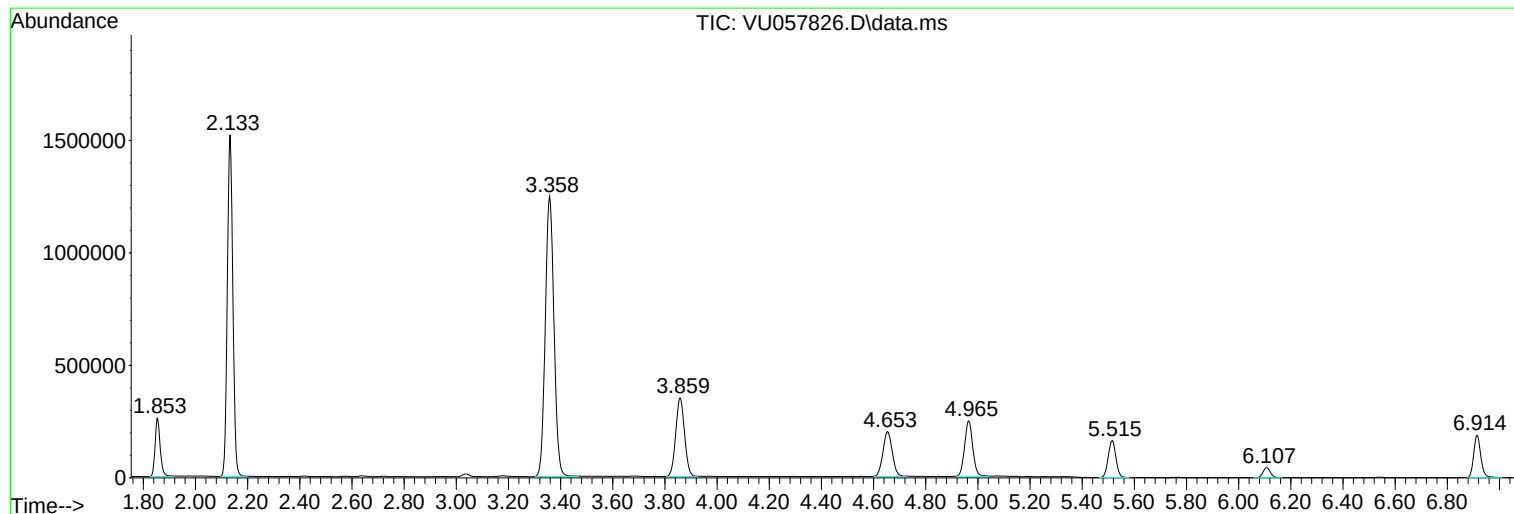

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057826.D
Acq On : 06 Feb 2024 17:42
Operator : MD/SY
Sample : P1174-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057826.D
Acq On : 06 Feb 2024 17:42
Operator : MD/SY
Sample : P1174-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------