


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU020624\  
Data File : VU057811.D  
Acq On : 06 Feb 2024 08:32  
Operator : MD/SY  
Sample : BFB  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\524U020524DW.M  
Title : METHOD 524.2 VOLATILES DRINKING WATER  
Last Update : Wed Feb 07 04:06:29 2024

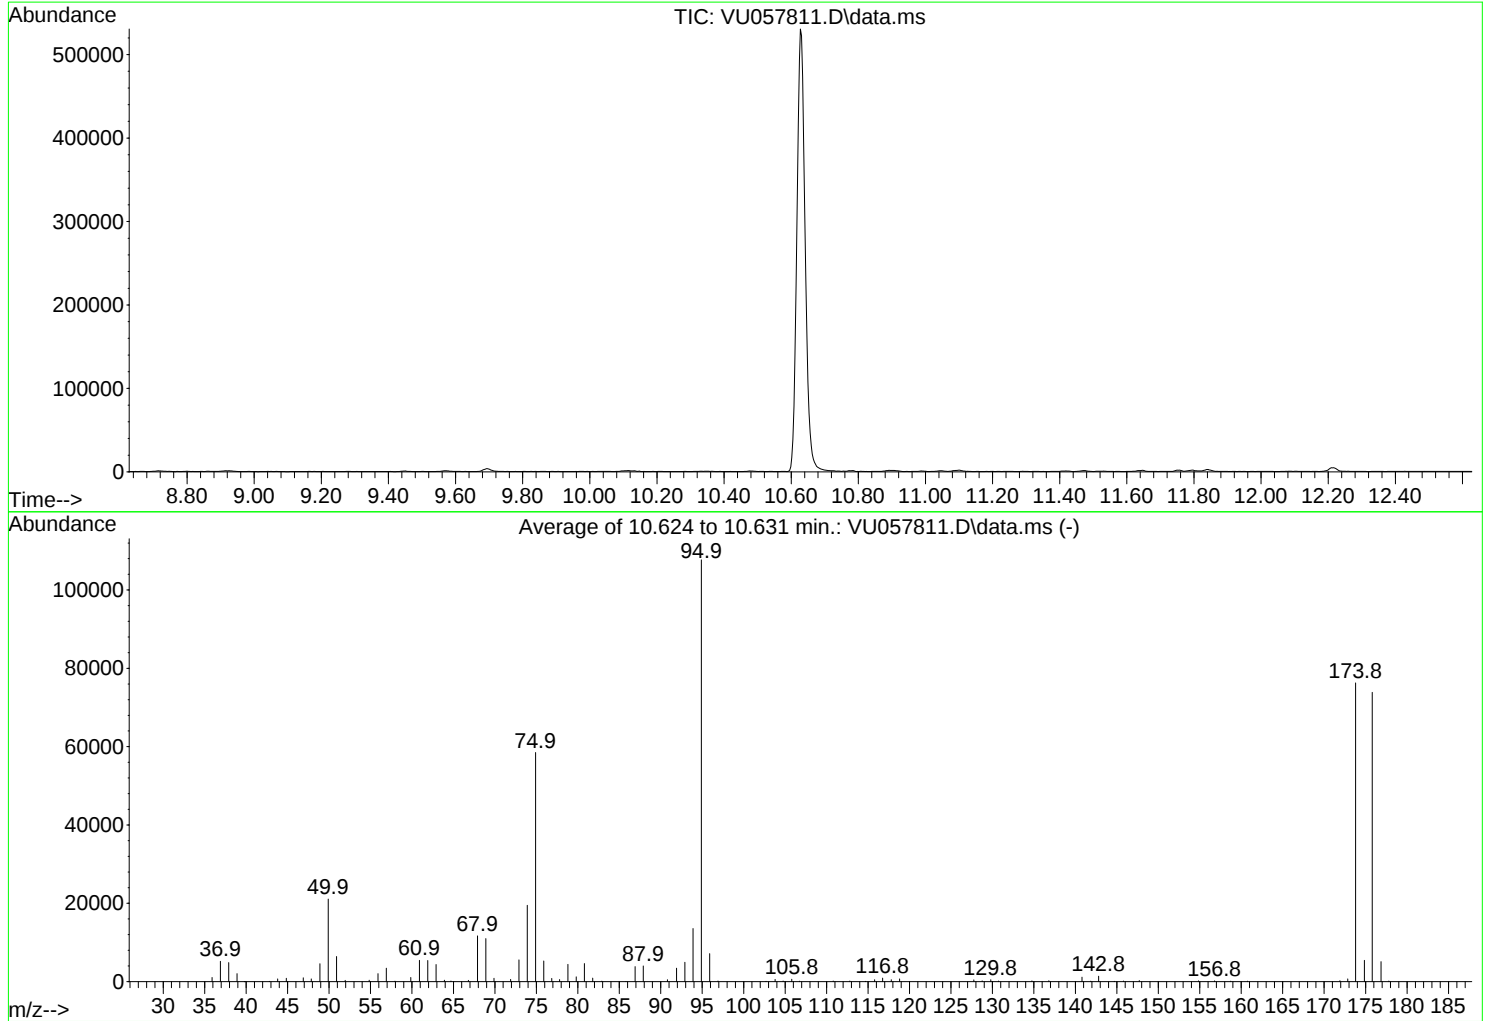

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.6         | 21096      | PASS                |
| 75             | 95              | 30              | 60              | 54.3         | 58523      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 107701     | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 7148       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 679        | PASS                |
| 174            | 95              | 50              | 100             | 70.8         | 76291      | PASS                |
| 175            | 174             | 5               | 9               | 7.1          | 5424       | PASS                |
| 176            | 174             | 95              | 101             | 96.8         | 73867      | PASS                |
| 177            | 176             | 5               | 9               | 6.9          | 5131       | PASS                |