


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020719\
Data File : VU029363.D
Acq On : 07 Feb 2019 09:19
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U020519DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Feb 08 10:52:46 2019

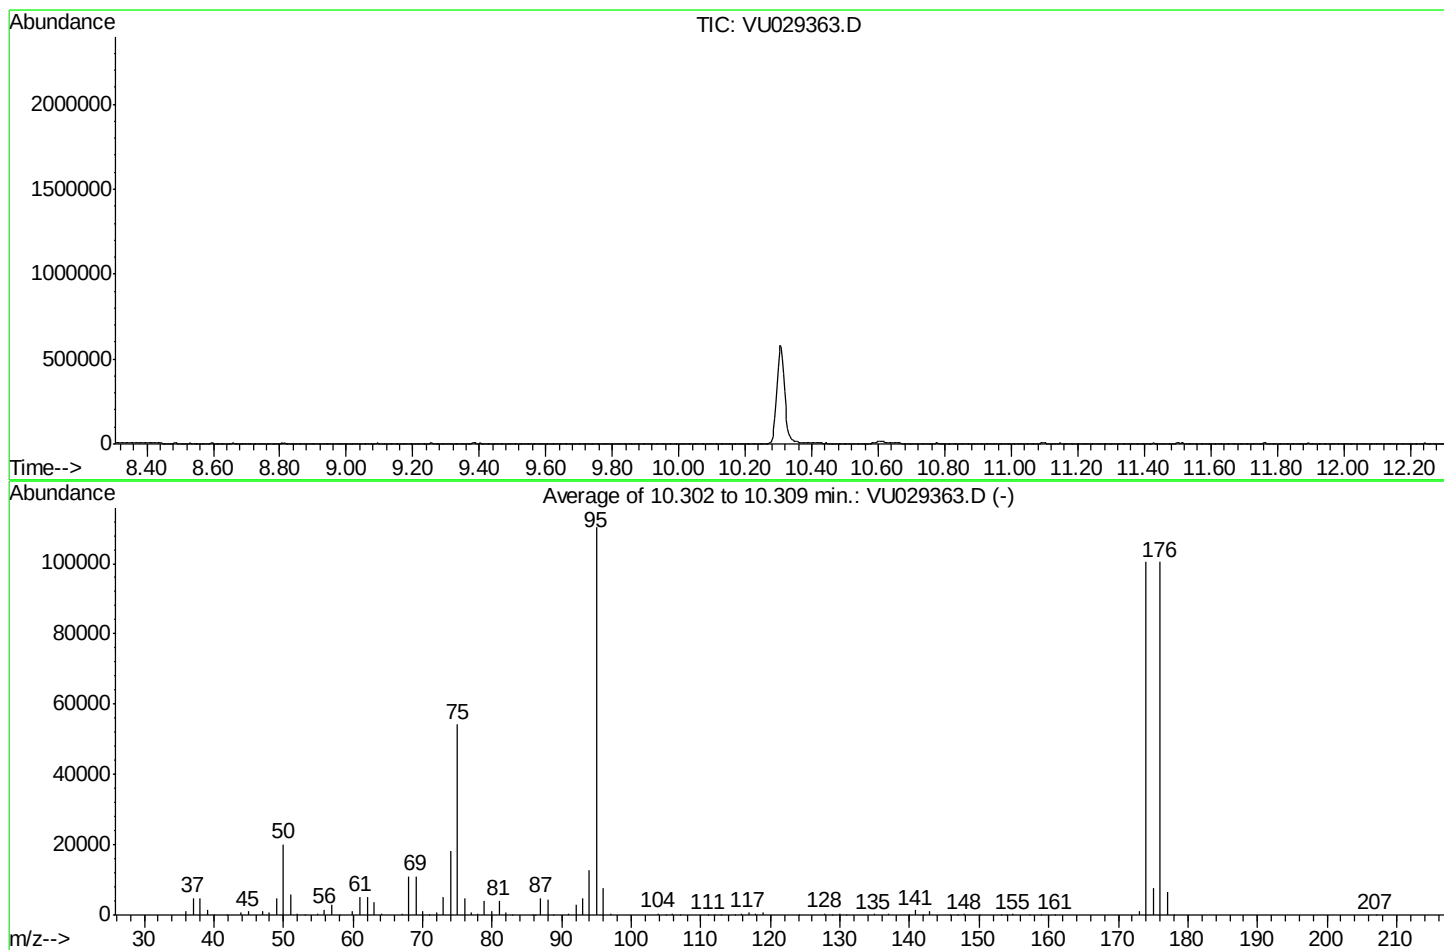

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	20189	PASS
75	95	30	60	49.2	54256	PASS
95	95	100	100	100.0	110320	PASS
96	95	5	9	6.8	7506	PASS
173	174	0.00	2	1.1	1076	PASS
174	95	50	100	91.0	100424	PASS
175	174	5	9	7.5	7576	PASS
176	174	95	101	100.0	100464	PASS
177	176	5	9	6.6	6639	PASS