
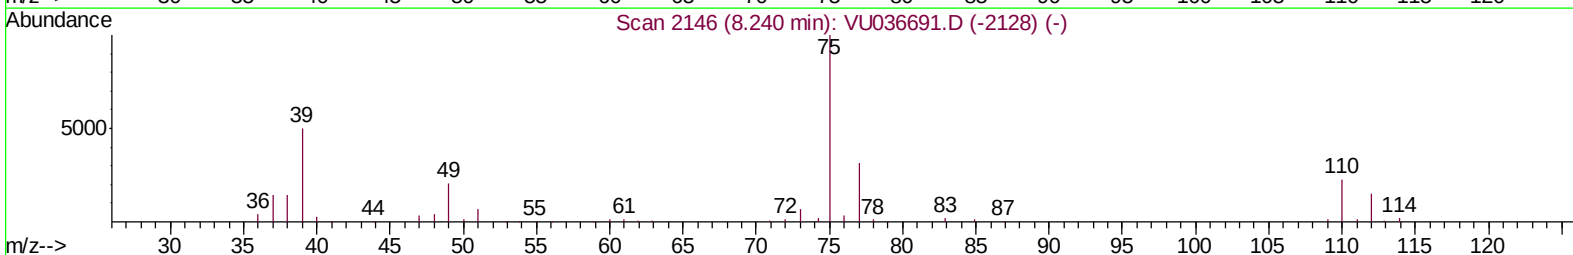
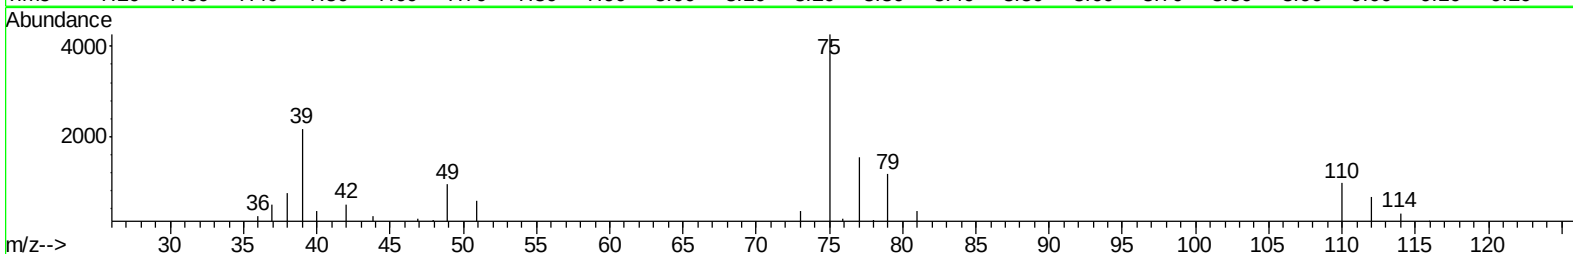


Data File : VU036696.D
Acq On : 07 Feb 2020 12:27
Operator : JC/MD
Sample : MDL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 07 23:16:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 07 22:36:50 2020
Response via : Initial Calibration

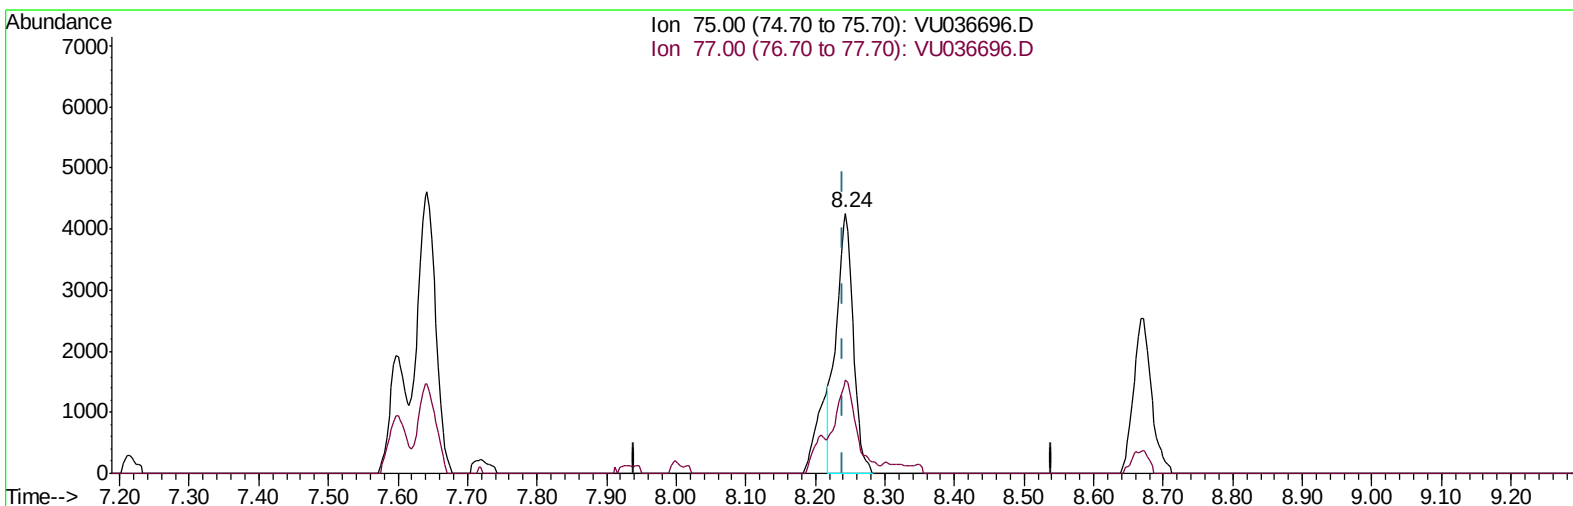

TIC: VU036696.D

(44) trans-1,3-Dichloropropene (T)

8.243min (+0.003) 2.58ug/L m

response 7219

Ion	Exp%	Act%
75.00	100	100
77.00	32.30	35.93
0.00	0.00	0.00
0.00	0.00	0.00