

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036693.D
 Acq On : 07 Feb 2020 11:11
 Operator : JC/MD
 Sample : VU0207MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Quant Time: Feb 07 22:49:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 07 22:36:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	255663	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	238513	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.83	152	101156	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	82777	48.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.10%
7) Chloroethane-d5	1.93	69	78824	49.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.72%
11) 1,1-Dichloroethene-d2	2.59	63	115295	35.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.64%
21) 2-Butanone-d5	4.68	46	168312	115.70	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	115.70%
24) Chloroform-d	5.11	84	151247	49.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.02%
26) 1,2-Dichloroethane-d4	5.75	65	107442	50.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.82%
32) Benzene-d6	5.77	84	322426	51.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.84%
36) 1,2-Dichloropropane-d6	6.73	67	108421	52.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.16%
41) Toluene-d8	7.93	98	289163	50.36	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.72%
43) trans-1,3-Dichloropropene-	8.21	79	49748	49.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.82%
47) 2-Hexanone-d5	8.67	63	131301	110.52	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.52%
56) 1,1,2,2-Tetrachloroethane-	10.78	84	158892	51.80	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.60%
66) 1,2-Dichlorobenzene-d4	12.21	152	96465	52.49	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.98%


Target Compounds					Ovalue
13) Acetone	2.66	43	2441	1.580 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020720\
Data File : VU036693.D
Acq On : 07 Feb 2020 11:11
Operator : JC/MD
Sample : VU0207MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Time: Feb 07 22:49:56 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 07 22:36:50 2020
Response via : Initial Calibration

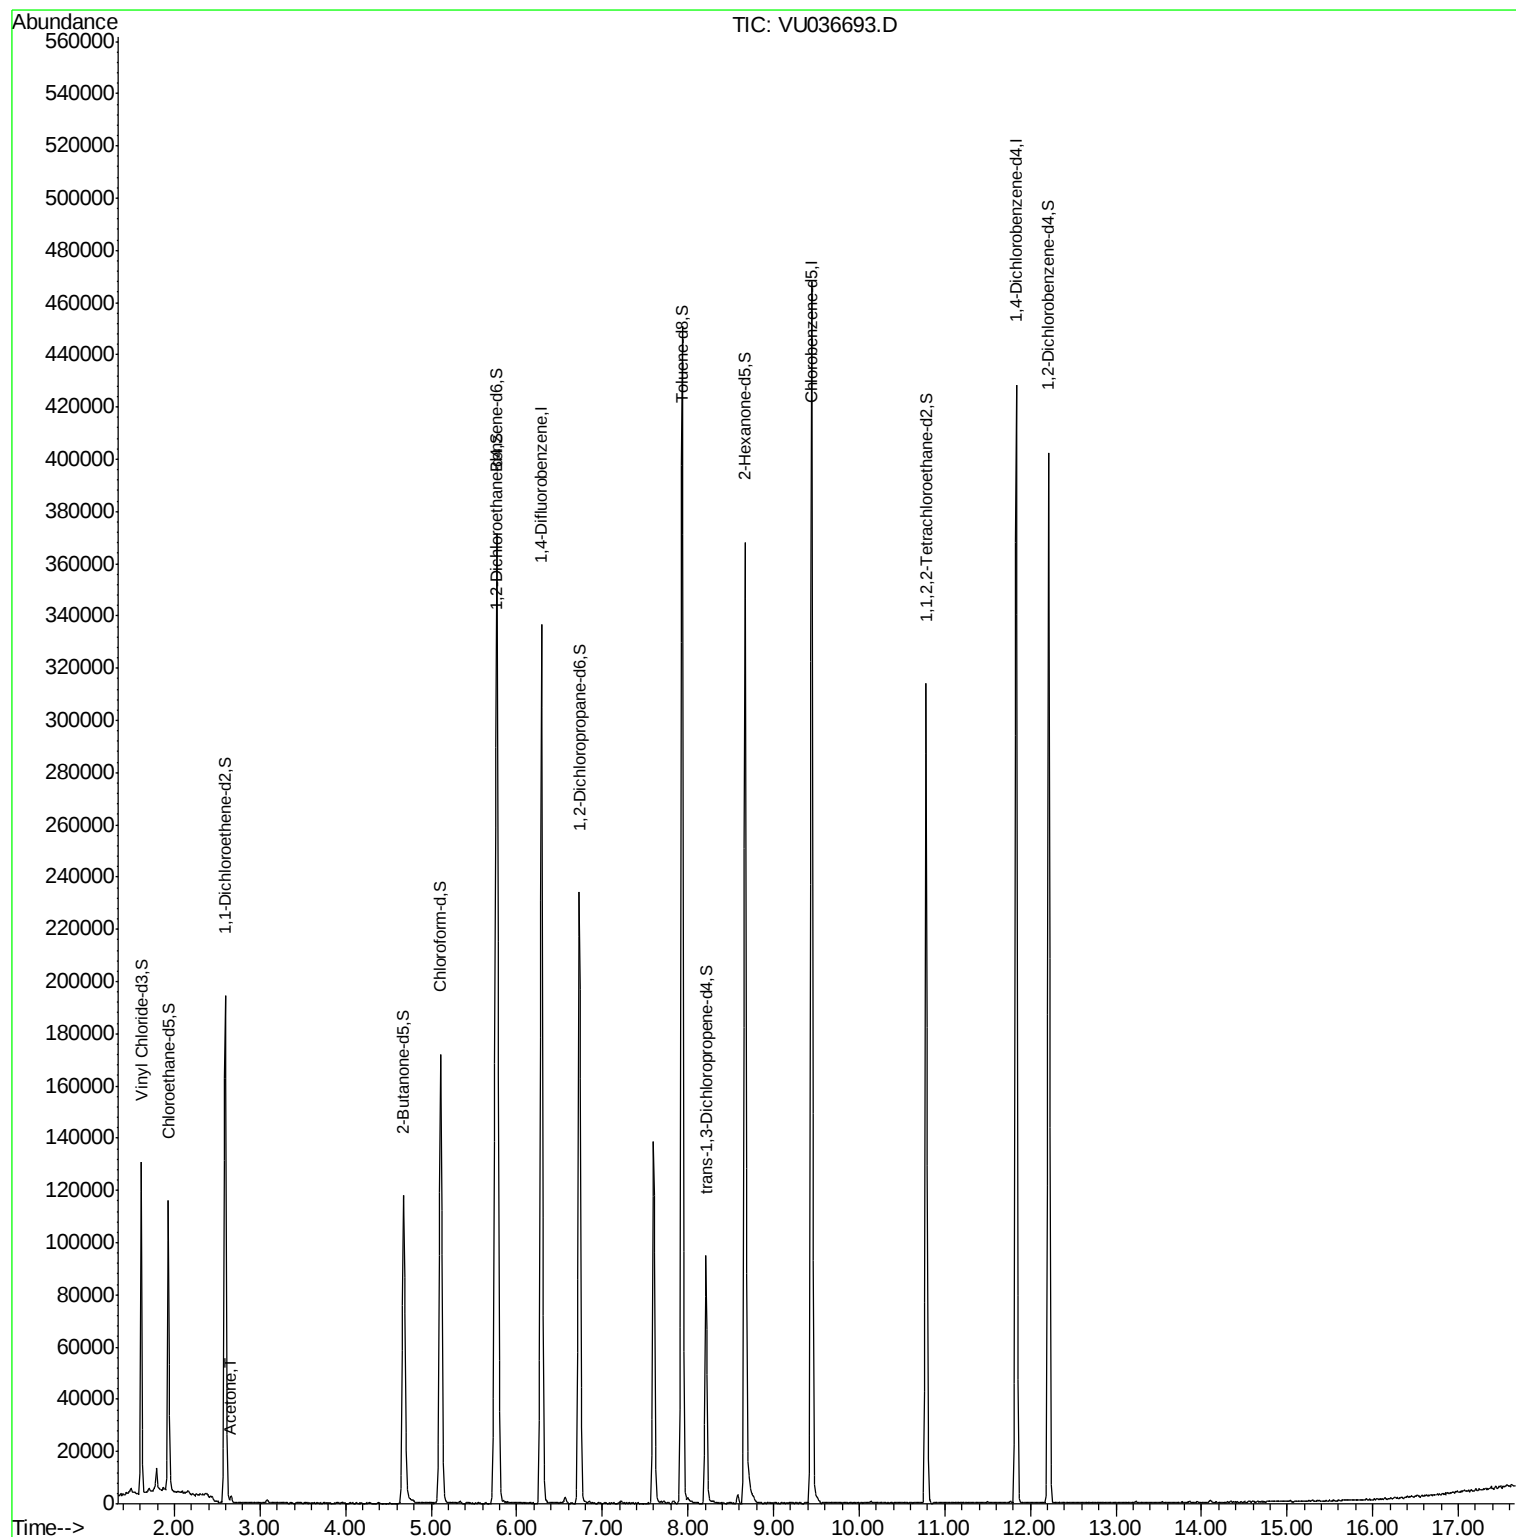

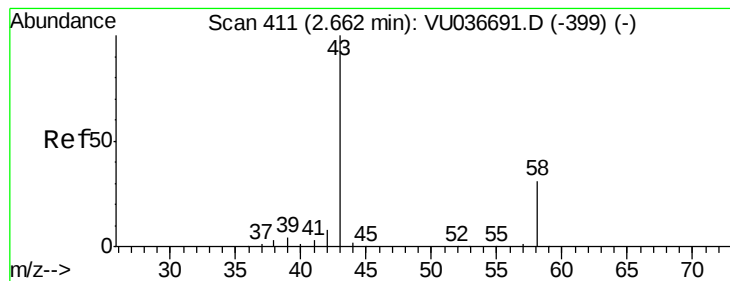

#13

Acetone

Concen: 1.580 ug/L

RT: 2.66 min Scan# 410

Delta R.T. -0.00 min

Lab File: VU036693.D

Acq: 07 Feb 2020 11:11

Instrument :

MSVOA_U

ClientSampleId :

VBLK104

Tot Ion: 43 Resp: 2441

Ion Ratio Lower Upper

43 100

58 28.4 0.0 64.0

