

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036693.D
 Acq On : 07 Feb 2020 11:11
 Operator : JC/MD
 Sample : VU0207MBL01
 Misc : 5.00µL/5.0mL/100µL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	98	rBV	126907	135525	13.91%	1.751%
2	1.928	176	183	200	rVB	111352	147758	15.17%	1.909%
3	2.594	378	390	405	rBV	193900	318841	32.73%	4.120%
4	2.925	491	493	496	rBV	151	69	0.01%	0.001%
5	3.086	536	543	552	rVB3	1214	1808	0.19%	0.023%
6	3.131	552	557	562	rBV	225	258	0.03%	0.003%
7	3.221	581	585	586	rBV	341	215	0.02%	0.003%
8	3.353	619	626	628	rBV	145	143	0.01%	0.002%
9	3.510	674	675	678	rBV	131	63	0.01%	0.001%
10	3.533	680	682	685	rBV	115	86	0.01%	0.001%
11	3.613	705	707	709	rVB	151	43	0.00%	0.001%
12	3.633	709	713	715	rBV2	263	169	0.02%	0.002%
13	3.790	760	762	765	rBV	196	99	0.01%	0.001%
14	3.867	785	786	788	rVB	115	24	0.00%	0.000%
15	3.948	809	811	813	rBV	120	70	0.01%	0.001%
16	3.961	813	815	817	rVB	226	99	0.01%	0.001%
17	4.047	840	842	844	rBV	110	56	0.01%	0.001%
18	4.073	846	850	854	rVV	133	119	0.01%	0.002%
19	4.189	882	886	891	rBV	134	136	0.01%	0.002%
20	4.234	896	900	901	rBV	103	66	0.01%	0.001%
21	4.337	930	932	935	rVB	70	33	0.00%	0.000%
22	4.356	935	938	940	rBV	91	62	0.01%	0.001%
23	4.379	943	945	948	rVV	199	117	0.01%	0.002%
24	4.395	948	950	954	rVB2	226	157	0.02%	0.002%
25	4.430	957	961	968	rBV	78	106	0.01%	0.001%
26	4.533	991	993	995	rBV	53	25	0.00%	0.000%
27	4.562	999	1002	1004	rBV	137	96	0.01%	0.001%
28	4.678	1023	1038	1060	rBV2	117858	273060	28.03%	3.529%
29	5.041	1149	1151	1154	rBV	217	116	0.01%	0.001%
30	5.112	1156	1173	1198	rVV	171874	373617	38.35%	4.828%
31	5.288	1225	1228	1233	rVB2	478	342	0.04%	0.004%
32	5.337	1233	1243	1250	rBV2	772	1274	0.13%	0.016%
33	5.375	1252	1255	1256	rBV	46	27	0.00%	0.000%
34	5.427	1262	1271	1275	rBV2	503	685	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036693.D
 Acq On : 07 Feb 2020 11:11
 Operator : JC/MD
 Sample : VU0207MBL01
 Misc : 5.00µL/5.0mL/100µL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

35	5.459	1279	1281	1285	rBV	143	79	0.01%	0.001%
36	5.517	1298	1299	1302	rVB	169	68	0.01%	0.001%
37	5.549	1302	1309	1313	rBV	171	244	0.03%	0.003%
38	5.629	1333	1334	1337	rBV	112	84	0.01%	0.001%
39	5.768	1355	1377	1399	rBV2	371408	974281	100.00%	12.590%
40	6.073	1469	1472	1473	rBV2	250	123	0.01%	0.002%
41	6.083	1473	1475	1478	rVB	339	208	0.02%	0.003%
42	6.144	1492	1494	1497	rBV	100	93	0.01%	0.001%
43	6.173	1501	1503	1505	rVV	134	60	0.01%	0.001%
44	6.189	1505	1508	1512	rVB2	252	192	0.02%	0.002%
45	6.288	1523	1539	1556	rBV	336514	621323	63.77%	8.029%
46	6.497	1602	1604	1605	rBV	116	48	0.00%	0.001%
47	6.565	1617	1625	1633	rVB4	2074	3383	0.35%	0.044%
48	6.632	1645	1646	1647	rBV4	86	19	0.00%	0.000%
49	6.732	1662	1677	1695	rBV	233932	454481	46.65%	5.873%
50	6.841	1705	1711	1715	rBV3	786	975	0.10%	0.013%
51	6.906	1729	1731	1734	rBV	129	75	0.01%	0.001%
52	6.980	1753	1754	1756	rVB	136	27	0.00%	0.000%
53	6.993	1756	1758	1761	rBV	51	35	0.00%	0.000%
54	7.067	1779	1781	1783	rBV	91	50	0.01%	0.001%
55	7.079	1783	1785	1788	rBV	117	88	0.01%	0.001%
56	7.105	1792	1793	1794	rVV	103	22	0.00%	0.000%
57	7.131	1799	1801	1802	rBV	104	43	0.00%	0.001%
58	7.182	1816	1817	1818	rBV	96	24	0.00%	0.000%
59	7.195	1818	1821	1822	rVV	153	95	0.01%	0.001%
60	7.214	1822	1827	1836	rVB2	959	1126	0.12%	0.015%
61	7.253	1836	1839	1841	rBV	118	78	0.01%	0.001%
62	7.285	1844	1849	1852	rBV	157	167	0.02%	0.002%
63	7.388	1879	1881	1884	rBV	84	48	0.00%	0.001%
64	7.481	1906	1910	1912	rBV	91	63	0.01%	0.001%
65	7.536	1924	1927	1928	rBV	151	65	0.01%	0.001%
66	7.600	1933	1947	1968	rBV	138322	239127	24.54%	3.090%
67	7.751	1992	1994	1995	rBV	106	40	0.00%	0.001%
68	7.832	2009	2019	2026	rBV3	910	1446	0.15%	0.019%
69	7.931	2035	2050	2067	rBV	450570	768972	78.93%	9.937%
70	8.211	2124	2137	2155	rBV	94914	159367	16.36%	2.059%
71	8.337	2173	2176	2181	rVB2	328	296	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036693.D
 Acq On : 07 Feb 2020 11:11
 Operator : JC/MD
 Sample : VU0207MBL01
 Misc : 5.00µL/5.0mL/100µL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

72	8.356	2181	2182	2184	rBV	227	105	0.01%	0.001%
73	8.385	2187	2191	2193	rVB	169	107	0.01%	0.001%
74	8.407	2196	2198	2200	rBV	152	53	0.01%	0.001%
75	8.456	2211	2213	2215	rBB	139	35	0.00%	0.000%
76	8.530	2234	2236	2239	rBV	142	40	0.00%	0.001%
77	8.581	2246	2252	2263	rVB5	3264	4853	0.50%	0.063%
78	8.668	2265	2279	2307	rBV	368053	634407	65.12%	8.198%
79	8.861	2336	2339	2342	rVB2	221	138	0.01%	0.002%
80	8.931	2356	2361	2366	rBV2	268	316	0.03%	0.004%
81	9.121	2417	2420	2426	rBV	120	119	0.01%	0.002%
82	9.198	2441	2444	2446	rBV	158	88	0.01%	0.001%
83	9.446	2507	2521	2554	rVB	467867	767913	78.82%	9.924%
84	9.677	2591	2593	2595	rBV	119	49	0.01%	0.001%
85	9.713	2601	2604	2606	rBV	377	263	0.03%	0.003%
86	10.166	2742	2745	2746	rBV	145	68	0.01%	0.001%
87	10.410	2815	2821	2826	rBV	161	252	0.03%	0.003%
88	10.504	2847	2850	2852	rBV2	216	167	0.02%	0.002%
89	10.780	2924	2936	2954	rVB	313992	510590	52.41%	6.598%
90	11.764	3239	3242	3245	rBV	465	371	0.04%	0.005%
91	11.835	3251	3264	3284	rVB	428210	682203	70.02%	8.816%
92	12.073	3336	3338	3339	rBV	239	90	0.01%	0.001%
93	12.214	3369	3382	3399	rVB	402140	652094	66.93%	8.427%
94	13.301	3717	3720	3721	rBV	278	163	0.02%	0.002%
95	13.848	3887	3890	3891	rBV	326	172	0.02%	0.002%
96	14.102	3962	3969	3977	rBV	762	1301	0.13%	0.017%


Sum of corrected areas: 7738236

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020720\
Data File : VU036693.D
Acq On : 07 Feb 2020 11:11
Operator : JC/MD
Sample : VU0207MBL01
Misc : 5.00uL/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

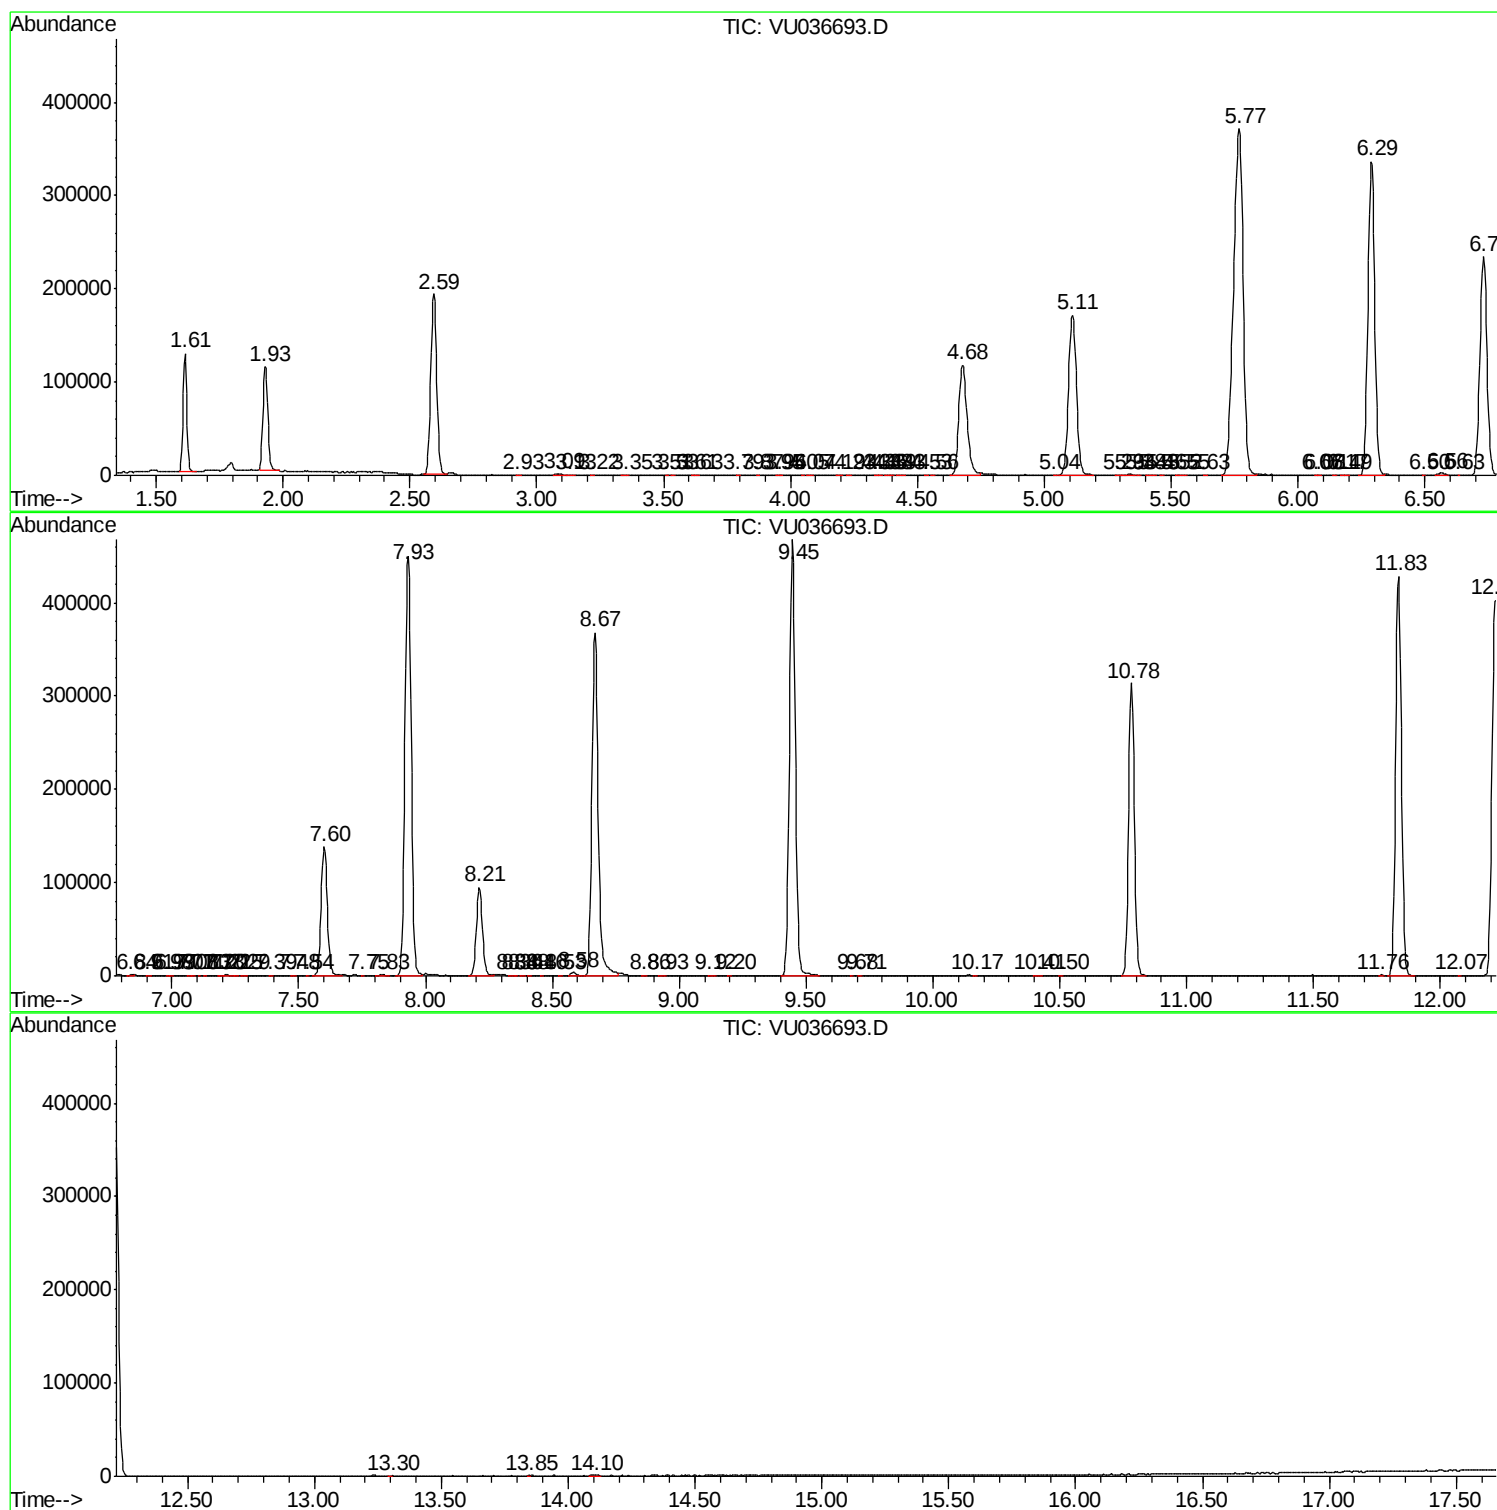

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU020720\
Data File : VU036693.D
Acq On : 07 Feb 2020 11:11
Operator : JC/MD
Sample : VU0207MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU020720\
Data File : VU036693.D
Acq On : 07 Feb 2020 11:11
Operator : JC/MD
Sample : VU0207MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc