

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036694.D
 Acq On : 07 Feb 2020 11:42
 Operator : JC/MD
 Sample : VU0207WBL04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	98	rVB	122218	125121	13.26%	1.659%
2	1.928	176	183	202	rVB	108116	142732	15.13%	1.893%
3	2.591	377	389	404	rBV	186424	303779	32.20%	4.029%
4	3.002	514	517	521	rBV	205	153	0.02%	0.002%
5	3.079	533	541	548	rVB3	1758	2991	0.32%	0.040%
6	3.218	582	584	587	rVB	220	96	0.01%	0.001%
7	3.343	621	623	624	rBV	117	31	0.00%	0.000%
8	3.562	688	691	693	rBV	109	61	0.01%	0.001%
9	3.742	743	747	750	rBV	119	94	0.01%	0.001%
10	3.771	753	756	758	rBV	65	48	0.01%	0.001%
11	3.928	802	805	809	rBV	64	59	0.01%	0.001%
12	4.083	849	853	858	rBV	105	135	0.01%	0.002%
13	4.128	865	867	872	rVB	217	97	0.01%	0.001%
14	4.153	872	875	878	rBV	81	61	0.01%	0.001%
15	4.192	884	887	893	rBV	134	108	0.01%	0.001%
16	4.366	938	941	946	rBV	96	86	0.01%	0.001%
17	4.388	946	948	950	rBV	67	37	0.00%	0.000%
18	4.414	954	956	957	rBV	174	69	0.01%	0.001%
19	4.488	976	979	982	rBV	113	92	0.01%	0.001%
20	4.607	1012	1016	1019	rBV	81	56	0.01%	0.001%
21	4.674	1019	1037	1062	rBV	107146	249084	26.40%	3.303%
22	5.108	1155	1172	1196	rBV	166955	358990	38.05%	4.761%
23	5.285	1224	1227	1228	rBV2	205	96	0.01%	0.001%
24	5.330	1235	1241	1248	rBV4	560	901	0.10%	0.012%
25	5.375	1253	1255	1257	rBV	84	36	0.00%	0.000%
26	5.411	1262	1266	1268	rBV3	379	361	0.04%	0.005%
27	5.533	1301	1304	1308	rBV	97	92	0.01%	0.001%
28	5.552	1308	1310	1313	rVB	65	36	0.00%	0.000%
29	5.629	1332	1334	1336	rBV	46	23	0.00%	0.000%
30	5.655	1341	1342	1343	rVV	107	22	0.00%	0.000%
31	5.764	1354	1376	1398	rBV2	358954	943461	100.00%	12.513%
32	6.112	1482	1484	1488	rVB	127	61	0.01%	0.001%
33	6.137	1488	1492	1494	rBV	227	171	0.02%	0.002%
34	6.202	1511	1512	1515	rVB	179	69	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036694.D
 Acq On : 07 Feb 2020 11:42
 Operator : JC/MD
 Sample : VU0207WBL04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

35	6.237	1517	1523	1524	rBV	96	69	0.01%	0.001%
36	6.285	1524	1538	1558	rBV	344461	638901	67.72%	8.473%
37	6.513	1606	1609	1611	rVB	189	100	0.01%	0.001%
38	6.529	1611	1614	1616	rVV	188	138	0.01%	0.002%
39	6.562	1617	1624	1635	rVB4	1837	3205	0.34%	0.043%
40	6.610	1635	1639	1640	rBV	167	112	0.01%	0.001%
41	6.632	1643	1646	1650	rVB	214	152	0.02%	0.002%
42	6.729	1659	1676	1693	rBV	229890	439295	46.56%	5.826%
43	6.880	1720	1723	1724	rBV	159	58	0.01%	0.001%
44	6.909	1729	1732	1734	rVB2	149	84	0.01%	0.001%
45	7.047	1772	1775	1777	rBV	176	72	0.01%	0.001%
46	7.063	1777	1780	1785	rVB	194	133	0.01%	0.002%
47	7.086	1785	1787	1789	rBV	46	26	0.00%	0.000%
48	7.166	1808	1812	1817	rBV2	416	484	0.05%	0.006%
49	7.218	1821	1828	1835	rVB3	889	1227	0.13%	0.016%
50	7.288	1848	1850	1854	rVB	154	83	0.01%	0.001%
51	7.375	1875	1877	1878	rBV	160	49	0.01%	0.001%
52	7.410	1884	1888	1889	rBV2	182	114	0.01%	0.002%
53	7.449	1897	1900	1902	rVB	100	58	0.01%	0.001%
54	7.465	1902	1905	1906	rBV	109	58	0.01%	0.001%
55	7.494	1912	1914	1917	rBV	137	60	0.01%	0.001%
56	7.517	1917	1921	1923	rBV	171	152	0.02%	0.002%
57	7.597	1932	1946	1966	rBV	131012	228882	24.26%	3.036%
58	7.790	2003	2006	2009	rBV2	149	137	0.01%	0.002%
59	7.828	2014	2018	2025	rVV4	662	936	0.10%	0.012%
60	7.857	2025	2027	2029	rVB	44	18	0.00%	0.000%
61	7.928	2035	2049	2066	rBV	444325	753741	79.89%	9.996%
62	8.211	2125	2137	2155	rBV	92010	154171	16.34%	2.045%
63	8.369	2184	2186	2190	rVB	242	87	0.01%	0.001%
64	8.430	2203	2205	2208	rVB	171	89	0.01%	0.001%
65	8.449	2208	2211	2215	rBV	124	103	0.01%	0.001%
66	8.472	2215	2218	2219	rBV	112	60	0.01%	0.001%
67	8.581	2249	2252	2257	rVB3	1028	812	0.09%	0.011%
68	8.664	2266	2278	2305	rBV	332336	578184	61.28%	7.668%
69	8.854	2336	2337	2339	rVB	123	26	0.00%	0.000%
70	8.909	2350	2354	2356	rBV	176	79	0.01%	0.001%
71	8.980	2372	2376	2379	rBV	262	163	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036694.D
 Acq On : 07 Feb 2020 11:42
 Operator : JC/MD
 Sample : VU0207WBL04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

72	9.086	2407	2409	2411	rBV	171	100	0.01%	0.001%
73	9.172	2434	2436	2437	rBV	125	37	0.00%	0.000%
74	9.234	2449	2455	2460	rBV	172	166	0.02%	0.002%
75	9.291	2471	2473	2478	rVB	181	75	0.01%	0.001%
76	9.359	2490	2494	2498	rBV	145	135	0.01%	0.002%
77	9.443	2507	2520	2556	rVB	472365	784117	83.11%	10.399%
78	9.574	2559	2561	2562	rBV	127	37	0.00%	0.000%
79	9.713	2601	2604	2605	rBV	261	146	0.02%	0.002%
80	9.819	2632	2637	2639	rBV2	215	176	0.02%	0.002%
81	9.925	2668	2670	2673	rVB	142	60	0.01%	0.001%
82	10.070	2712	2715	2717	rBV	204	127	0.01%	0.002%
83	10.134	2730	2735	2738	rBV3	617	638	0.07%	0.008%
84	10.333	2795	2797	2800	rVB	280	120	0.01%	0.002%
85	10.352	2800	2803	2804	rBV	125	71	0.01%	0.001%
86	10.597	2877	2879	2881	rBV	147	60	0.01%	0.001%
87	10.632	2887	2890	2893	rBV2	189	122	0.01%	0.002%
88	10.674	2901	2903	2904	rBV	138	36	0.00%	0.000%
89	10.780	2924	2936	2957	rVB	297489	484455	51.35%	6.425%
90	10.979	2995	2998	3002	rBV2	180	122	0.01%	0.002%
91	11.115	3031	3040	3045	rBV3	330	417	0.04%	0.006%
92	11.446	3141	3143	3144	rBV3	142	36	0.00%	0.000%
93	11.835	3252	3264	3283	rVB	429794	696195	73.79%	9.233%
94	12.214	3369	3382	3399	rBV	397725	640520	67.89%	8.495%
95	12.574	3492	3494	3496	rBV	251	133	0.01%	0.002%
96	13.237	3696	3700	3705	rVB4	617	606	0.06%	0.008%


Sum of corrected areas: 7540134

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020720\
Data File : VU036694.D
Acq On : 07 Feb 2020 11:42
Operator : JC/MD
Sample : VU0207WBL04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK105

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

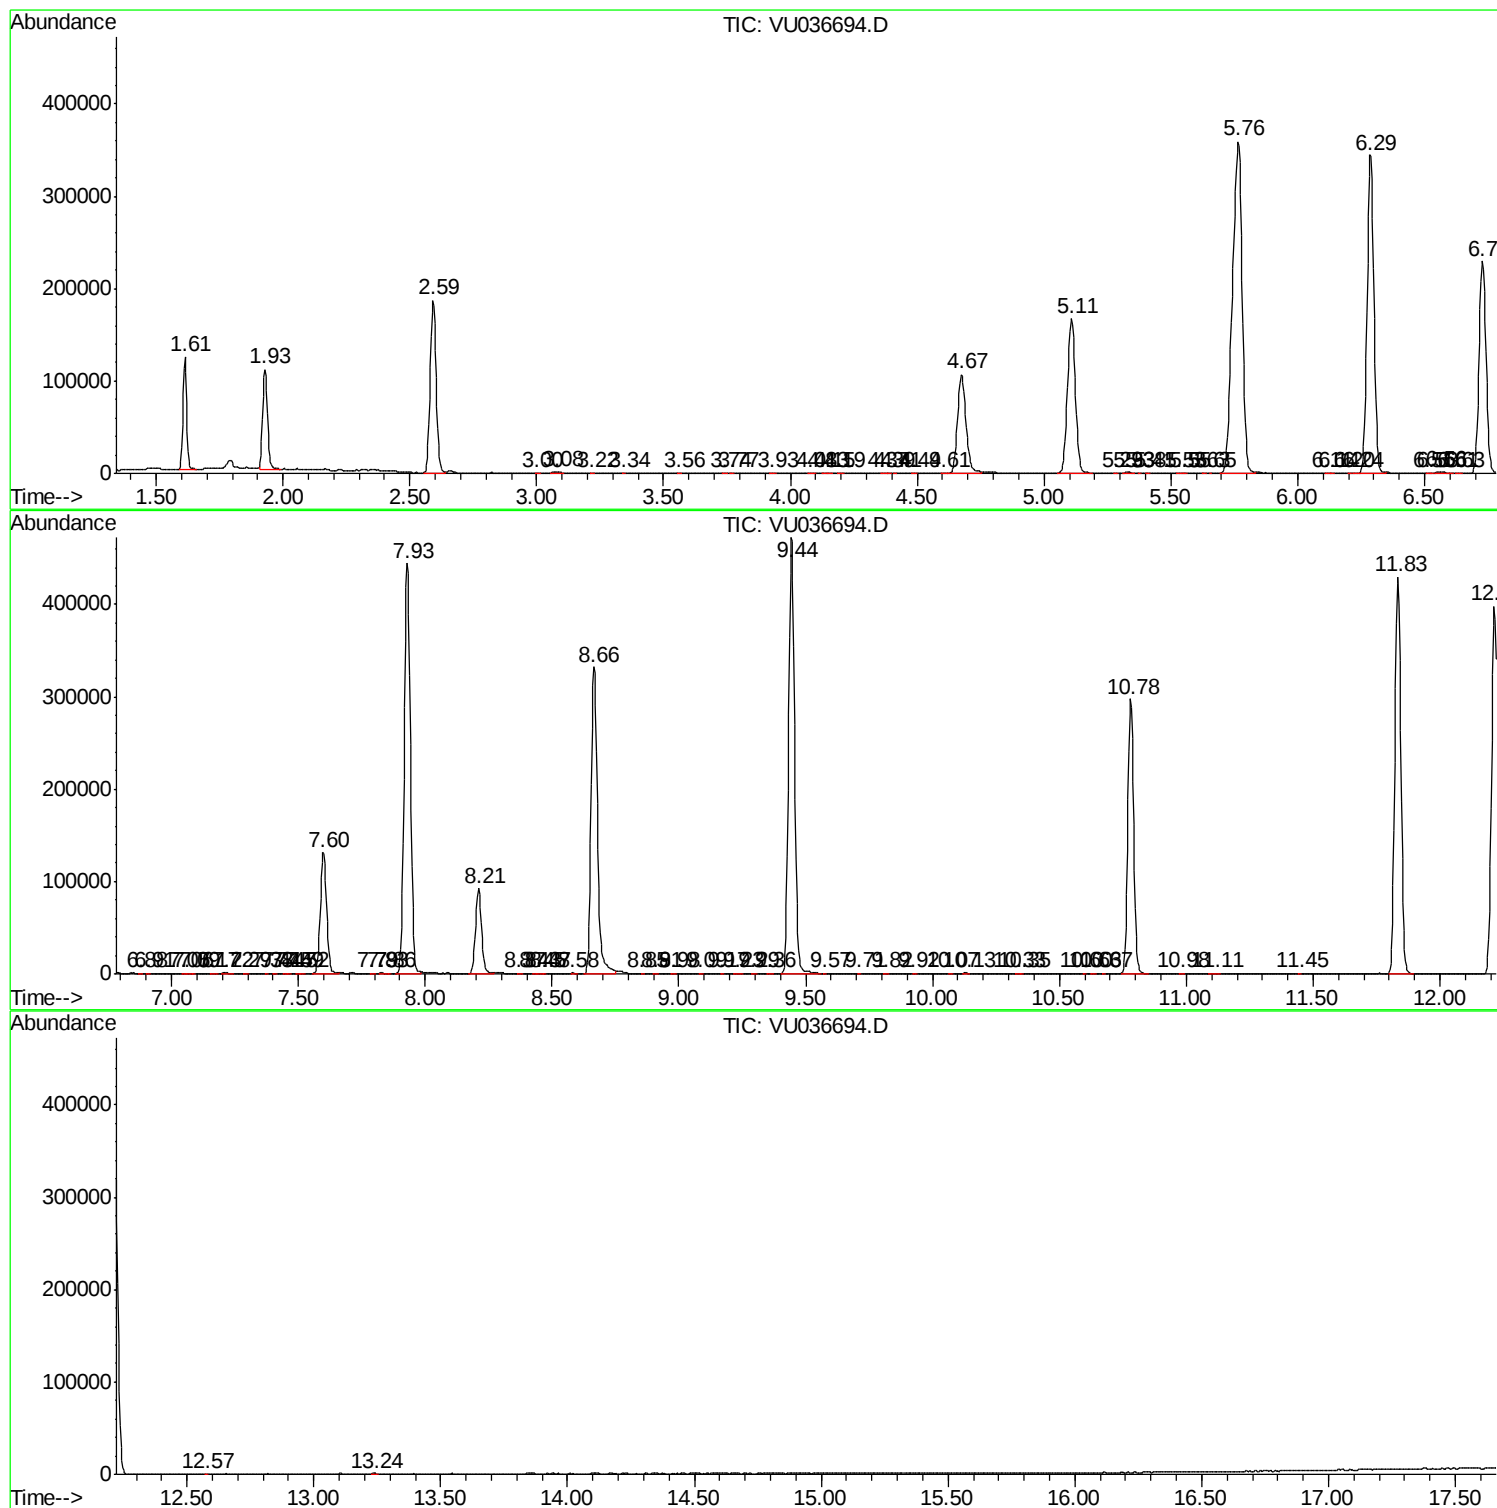

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU020720\
Data File : VU036694.D
Acq On : 07 Feb 2020 11:42
Operator : JC/MD
Sample : VU0207WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK105

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU020720\
Data File : VU036694.D
Acq On : 07 Feb 2020 11:42
Operator : JC/MD
Sample : VU0207WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK105

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc