

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036695.D
 Acq On : 07 Feb 2020 12:04
 Operator : JC/MD
 Sample : VU0207MBL02
 Misc : 5.00µL/5.0mL/100µL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	97	rBV	112141	121378	13.15%	1.639%
2	1.928	176	183	201	rVB	103477	137058	14.85%	1.851%
3	2.594	378	390	405	rBV	178595	294794	31.94%	3.981%
4	3.079	533	541	550	rVB3	1887	3035	0.33%	0.041%
5	3.224	581	586	588	rBV	382	409	0.04%	0.006%
6	3.626	707	711	713	rBV2	302	202	0.02%	0.003%
7	3.665	721	723	725	rVB	243	86	0.01%	0.001%
8	3.678	725	727	732	rVB	176	91	0.01%	0.001%
9	3.703	732	735	737	rBV	170	112	0.01%	0.002%
10	3.835	775	776	777	rBV	92	20	0.00%	0.000%
11	3.964	810	816	820	rBV	109	120	0.01%	0.002%
12	4.041	838	840	843	rVB2	139	80	0.01%	0.001%
13	4.153	872	875	877	rBV	89	51	0.01%	0.001%
14	4.295	916	919	921	rBV	115	67	0.01%	0.001%
15	4.321	924	927	929	rBV2	306	232	0.03%	0.003%
16	4.475	971	975	978	rBV2	178	123	0.01%	0.002%
17	4.504	981	984	989	rVB	222	147	0.02%	0.002%
18	4.539	993	995	999	rBV	152	67	0.01%	0.001%
19	4.565	1001	1003	1007	rVB	181	89	0.01%	0.001%
20	4.584	1007	1009	1011	rBV	107	60	0.01%	0.001%
21	4.678	1022	1038	1061	rBV	111428	257938	27.95%	3.483%
22	5.031	1141	1148	1151	rBV2	279	383	0.04%	0.005%
23	5.112	1157	1173	1194	rBV	161461	352691	38.22%	4.762%
24	5.301	1229	1232	1235	rBV2	226	205	0.02%	0.003%
25	5.369	1250	1253	1254	rBV	145	77	0.01%	0.001%
26	5.472	1282	1285	1288	rBV	125	89	0.01%	0.001%
27	5.639	1335	1337	1340	rBV	144	81	0.01%	0.001%
28	5.768	1355	1377	1395	rBV2	351990	922872	100.00%	12.461%
29	6.044	1460	1463	1466	rBV	192	180	0.02%	0.002%
30	6.079	1472	1474	1475	rBV	322	116	0.01%	0.002%
31	6.121	1485	1487	1489	rBV	183	95	0.01%	0.001%
32	6.288	1523	1539	1559	rBV	331497	618093	66.97%	8.346%
33	6.565	1618	1625	1636	rVB4	2200	3680	0.40%	0.050%
34	6.607	1637	1638	1644	rVB	208	147	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036695.D
 Acq On : 07 Feb 2020 12:04
 Operator : JC/MD
 Sample : VU0207MBL02
 Misc : 5.00µ/5.0mL/100µL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

35	6.636	1644	1647	1649	rBV	100	68	0.01%	0.001%
36	6.652	1650	1652	1657	rVB	247	130	0.01%	0.002%
37	6.681	1658	1661	1662	rBV	88	48	0.01%	0.001%
38	6.732	1662	1677	1701	rBV	221736	430884	46.69%	5.818%
39	6.870	1718	1720	1722	rBV	153	73	0.01%	0.001%
40	6.886	1722	1725	1730	rVV2	251	136	0.01%	0.002%
41	6.909	1730	1732	1736	rVV	119	85	0.01%	0.001%
42	6.964	1747	1749	1751	rBV	99	58	0.01%	0.001%
43	7.012	1762	1764	1766	rVB	138	57	0.01%	0.001%
44	7.076	1783	1784	1785	rBV	110	25	0.00%	0.000%
45	7.105	1789	1793	1801	rBV	259	224	0.02%	0.003%
46	7.205	1820	1824	1827	rBV2	382	344	0.04%	0.005%
47	7.388	1880	1881	1883	rVB2	95	32	0.00%	0.000%
48	7.411	1887	1888	1893	rBV	164	108	0.01%	0.001%
49	7.443	1896	1898	1908	rVB2	277	341	0.04%	0.005%
50	7.484	1908	1911	1914	rBV	139	135	0.01%	0.002%
51	7.600	1933	1947	1963	rBV	127614	222280	24.09%	3.001%
52	7.767	1997	1999	2002	rVB	146	63	0.01%	0.001%
53	7.796	2007	2008	2011	rVB	223	84	0.01%	0.001%
54	7.822	2012	2016	2018	rBV2	516	424	0.05%	0.006%
55	7.931	2035	2050	2069	rBV	429376	730732	79.18%	9.867%
56	8.211	2125	2137	2155	rBV	87592	149204	16.17%	2.015%
57	8.359	2181	2183	2188	rBV2	232	160	0.02%	0.002%
58	8.394	2191	2194	2198	rVB2	272	174	0.02%	0.002%
59	8.446	2205	2210	2212	rBV2	227	217	0.02%	0.003%
60	8.504	2223	2228	2231	rVB2	332	309	0.03%	0.004%
61	8.520	2231	2233	2236	rBV	195	109	0.01%	0.001%
62	8.584	2247	2253	2260	rBV2	2897	3700	0.40%	0.050%
63	8.668	2265	2279	2323	rVB	340323	601431	65.17%	8.121%
64	8.883	2345	2346	2352	rVB	208	96	0.01%	0.001%
65	8.912	2352	2355	2356	rBV	133	61	0.01%	0.001%
66	8.947	2363	2366	2373	rBV	155	186	0.02%	0.003%
67	9.060	2398	2401	2402	rBV	137	61	0.01%	0.001%
68	9.102	2412	2414	2417	rVB	178	73	0.01%	0.001%
69	9.243	2456	2458	2461	rVB	160	85	0.01%	0.001%
70	9.269	2463	2466	2469	rBV2	201	139	0.02%	0.002%
71	9.446	2507	2521	2544	rBV	460226	758424	82.18%	10.241%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020720\
 Data File : VU036695.D
 Acq On : 07 Feb 2020 12:04
 Operator : JC/MD
 Sample : VU0207MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

72	9.619	2573	2575	2577	rBV	128	58	0.01%	0.001%
73	9.632	2577	2579	2581	rVV	184	78	0.01%	0.001%
74	9.674	2589	2592	2595	rBV2	155	122	0.01%	0.002%
75	9.722	2600	2607	2611	rVV2	302	398	0.04%	0.005%
76	9.751	2613	2616	2619	rVB2	202	122	0.01%	0.002%
77	10.211	2755	2759	2769	rVB2	215	248	0.03%	0.003%
78	10.565	2867	2869	2871	rBV	173	94	0.01%	0.001%
79	10.783	2923	2937	2953	rBV	300727	485861	52.65%	6.560%
80	11.468	3144	3150	3152	rBV	245	291	0.03%	0.004%
81	11.835	3252	3264	3281	rVB	415327	675820	73.23%	9.125%
82	12.214	3369	3382	3400	rVB	379933	626572	67.89%	8.460%
83	12.378	3430	3433	3435	rBV	250	130	0.01%	0.002%
84	13.233	3696	3699	3701	rBV	352	211	0.02%	0.003%
85	13.266	3706	3709	3711	rBV2	393	238	0.03%	0.003%


Sum of corrected areas: 7405871

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020720\
Data File : VU036695.D
Acq On : 07 Feb 2020 12:04
Operator : JC/MD
Sample : VU0207MBL02
Misc : 5.00µ/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

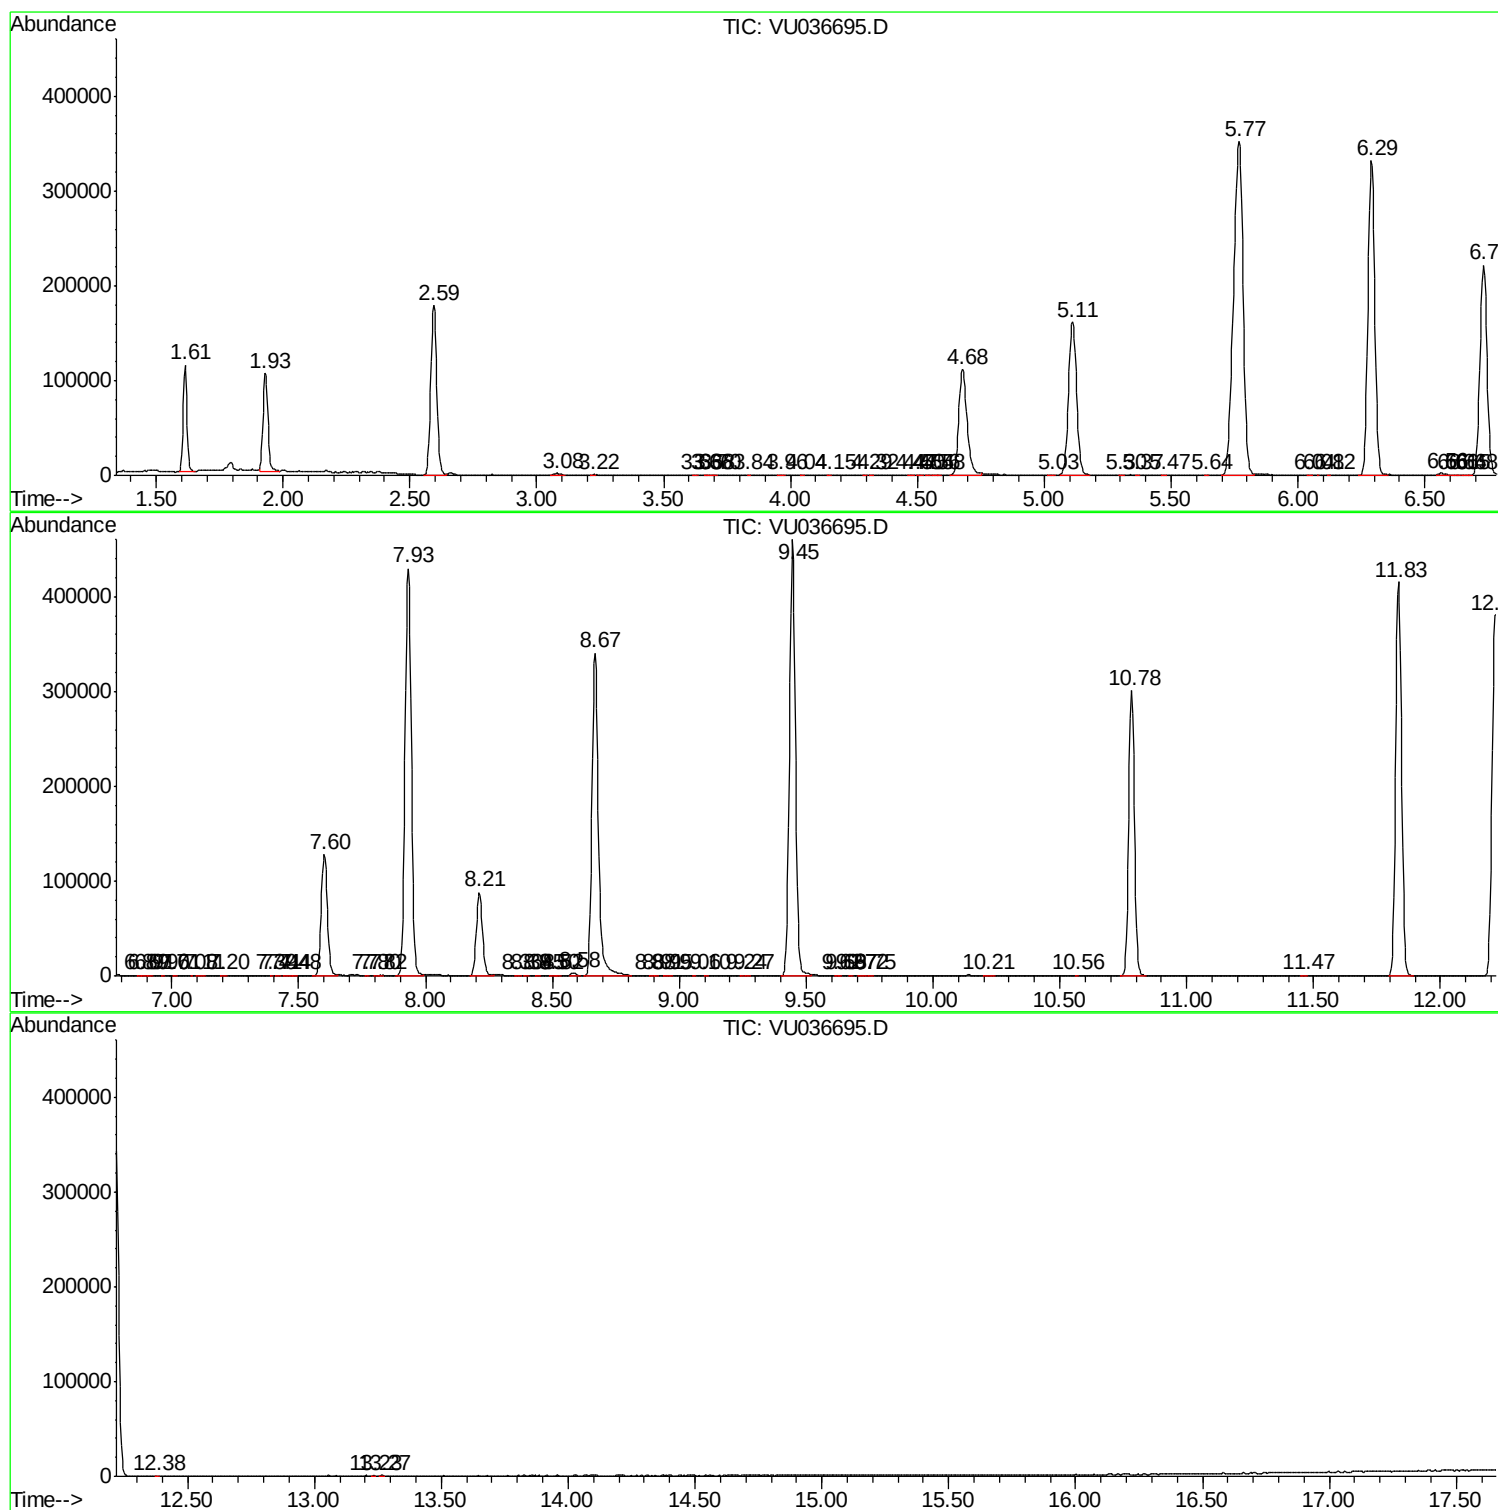

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU020720\
Data File : VU036695.D
Acq On : 07 Feb 2020 12:04
Operator : JC/MD
Sample : VU0207MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSV0A_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
VBLK106

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU020720\
Data File : VU036695.D
Acq On : 07 Feb 2020 12:04
Operator : JC/MD
Sample : VU0207MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSV0A_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
VBLK106

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc