


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU020720\
 Data File : VU036690.D
 Acq On : 07 Feb 2020 09:08
 Operator : JC/MD
 Sample : BFB49
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB102

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis
 Last Update : Fri Feb 07 22:36:50 2020

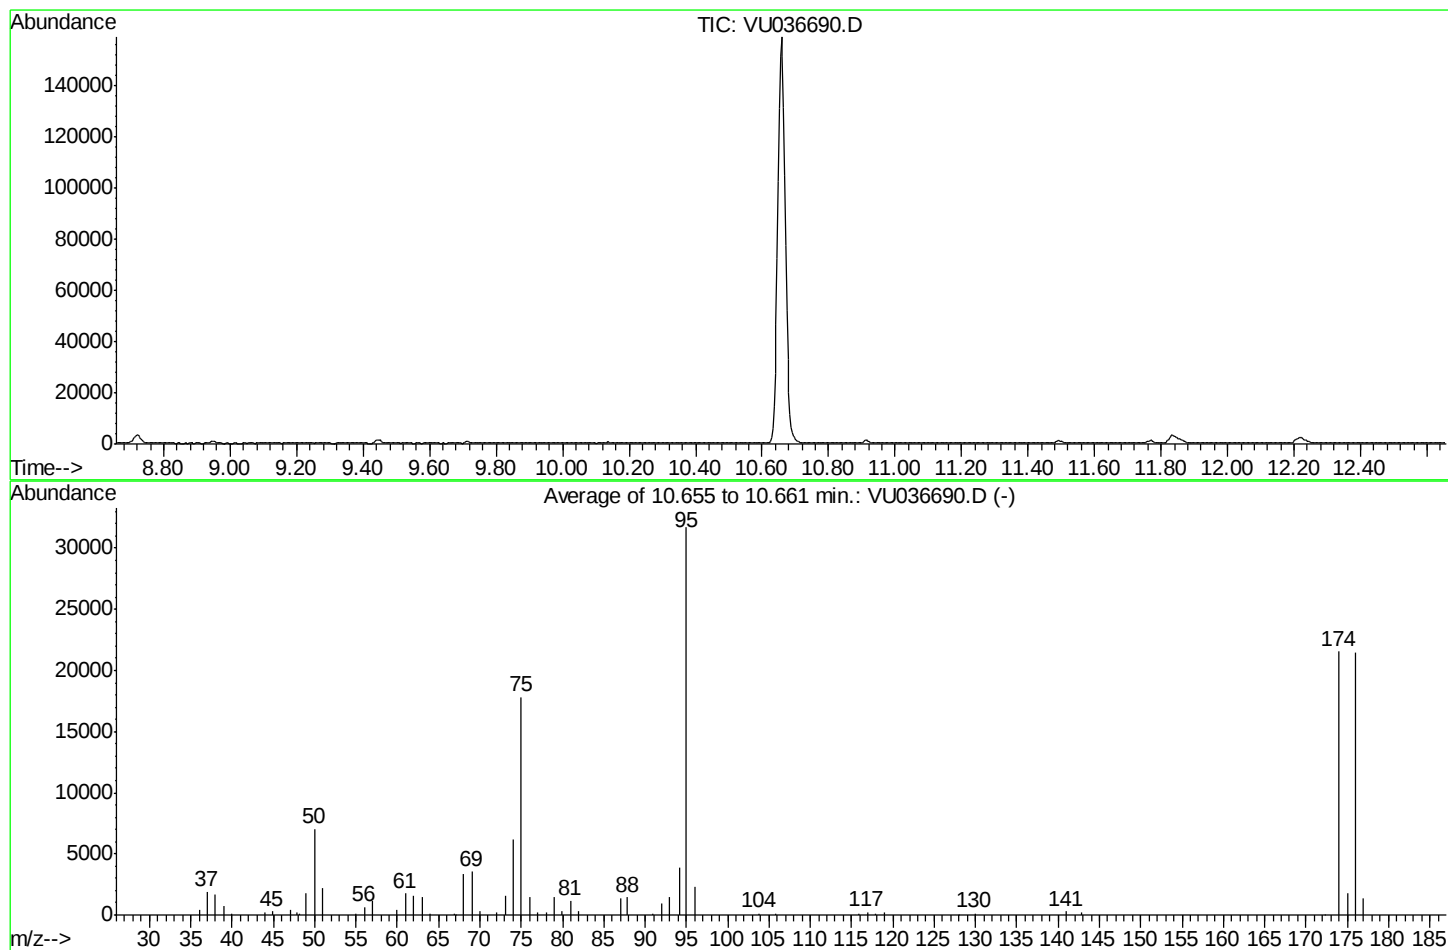

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	7026	PASS
75	95	30	80	56.2	17834	PASS
95	95	100	100	100.0	31709	PASS
96	95	5	9	7.2	2298	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.0	21554	PASS
175	174	5	9	8.4	1810	PASS
176	174	95	101	99.7	21485	PASS
177	176	5	9	6.6	1408	PASS

m/z	Abundance
36.00	412.0
37.00	1924.0
38.00	1761.0
39.10	708.0
39.90	127.0
44.00	665.0
44.90	304.0
47.00	477.0
47.80	217.0
49.00	1860.0
50.00	7320.0
51.00	2245.0
55.00	105.0
56.00	677.0
57.00	1194.0
60.00	416.0
61.00	1796.0
62.00	1624.0
63.00	1541.0
63.90	112.0
66.80	143.0
68.00	3450.0
69.10	3686.0
70.00	285.0
72.00	257.0
73.10	1593.0
74.00	6385.0
75.00	18408.0
76.00	1546.0
77.00	252.0
78.10	196.0
79.00	1533.0
79.90	367.0
80.90	1228.0
81.90	334.0
87.10	1423.0
87.90	1503.0
90.90	126.0
92.00	1003.0
93.00	1502.0
94.10	3968.0
95.00	32736.0
96.00	2396.0
103.90	175.0
105.90	122.0
115.90	116.0
117.00	216.0
117.90	115.0
118.90	172.0
129.90	139.0
141.00	306.0
142.90	223.0
174.00	22176.0
175.00	1865.0
176.00	22224.0
177.00	1467.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
36.00	400.0
37.00	1922.0
38.00	1687.0
39.10	736.0
44.00	698.0
44.90	278.0
47.10	437.0
47.80	208.0
48.10	202.0
49.00	1788.0
50.00	6873.0
51.00	2240.0
55.00	106.0
56.00	686.0
57.00	1135.0
60.00	368.0
61.00	1744.0
62.00	1591.0
63.00	1382.0
66.90	130.0
68.00	3320.0
69.10	3559.0
70.00	270.0
72.00	225.0
73.10	1527.0
74.00	6185.0
75.00	17464.0
76.00	1563.0
77.00	212.0
78.10	188.0
79.00	1359.0
79.90	363.0
80.90	1284.0
81.90	325.0
87.00	1477.0
87.90	1438.0
91.00	117.0
92.00	881.0
93.00	1475.0
94.10	3940.0
95.00	31336.0
96.00	2247.0
103.80	130.0
105.90	142.0
115.80	111.0
116.90	219.0
117.90	141.0
118.90	166.0
129.90	122.0
141.00	274.0
142.90	251.0
172.20	114.0
174.00	20568.0
175.00	1771.0
176.00	20888.0
177.00	1353.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
43.90	403.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
36.00	398.0
37.00	1817.0
38.00	1658.0
39.00	610.0
39.90	135.0
44.00	567.0
44.90	284.0
47.00	462.0
47.90	216.0
49.00	1808.0
50.00	6885.0
51.00	2062.0
56.00	617.0
57.00	1117.0
60.00	382.0
61.00	1715.0
62.00	1549.0
63.00	1487.0
63.90	127.0
66.80	137.0
67.10	122.0
68.00	3311.0
69.00	3359.0
70.10	293.0
72.00	227.0
73.10	1506.0
74.00	5933.0
75.00	17632.0
76.00	1434.0
77.00	263.0
78.10	181.0
79.00	1472.0
79.90	345.0
81.00	1084.0
81.90	315.0
87.00	1290.0
87.90	1451.0
90.90	120.0
92.00	954.0
93.00	1392.0
94.10	3785.0
95.00	31056.0
96.00	2251.0
103.90	177.0
105.80	104.0
115.90	115.0
117.00	205.0
118.90	160.0
128.00	110.0
129.90	136.0
141.00	291.0
142.90	208.0
174.00	21920.0
175.00	1794.0
176.00	21344.0
177.00	1404.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102