

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057842.D
 Acq On : 07 Feb 2024 15:59
 Operator : MD/SY
 Sample : P1329-03ME
 Misc : 5.86g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Feb 08 01:28:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 08 01:18:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	273380	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	271614	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	136330	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	98552	45.039	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.080%
7) Chloroethane-d5	1.872	69	27577	16.245	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	32.500%#
11) 1,1-Dichloroethene-d2	2.538	63	127731	31.784	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.560%
21) 2-Butanone-d5	4.618	46	100152	82.472	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.470%
24) Chloroform-d	5.049	84	162726	41.923	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.840%
26) 1,2-Dichloroethane-d4	5.689	65	111564	45.339	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.680%
32) Benzene-d6	5.714	84	342701	41.765	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.520%
36) 1,2-Dichloropropane-d6	6.679	67	108812	41.992	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.980%
41) Toluene-d8	7.891	98	307883	41.388	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.780%
43) trans-1,3-Dichloroprop...	8.177	79	52667	41.548	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.100%
47) 2-Hexanone-d5	8.644	63	103446	97.803	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.800%
56) 1,1,2,2-Tetrachloroeth...	10.756	84	162482	48.169	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.340%
66) 1,2-Dichlorobenzene-d4	12.190	152	119384	45.581	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.160%
Target Compounds						
37) 1,2-Dichloropropane	6.682	63	11891	5.044	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057842.D
Acq On : 07 Feb 2024 15:59
Operator : MD/SY
Sample : P1329-03ME
Misc : 5.86g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Feb 08 01:28:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 08 01:18:21 2024
Response via : Initial Calibration

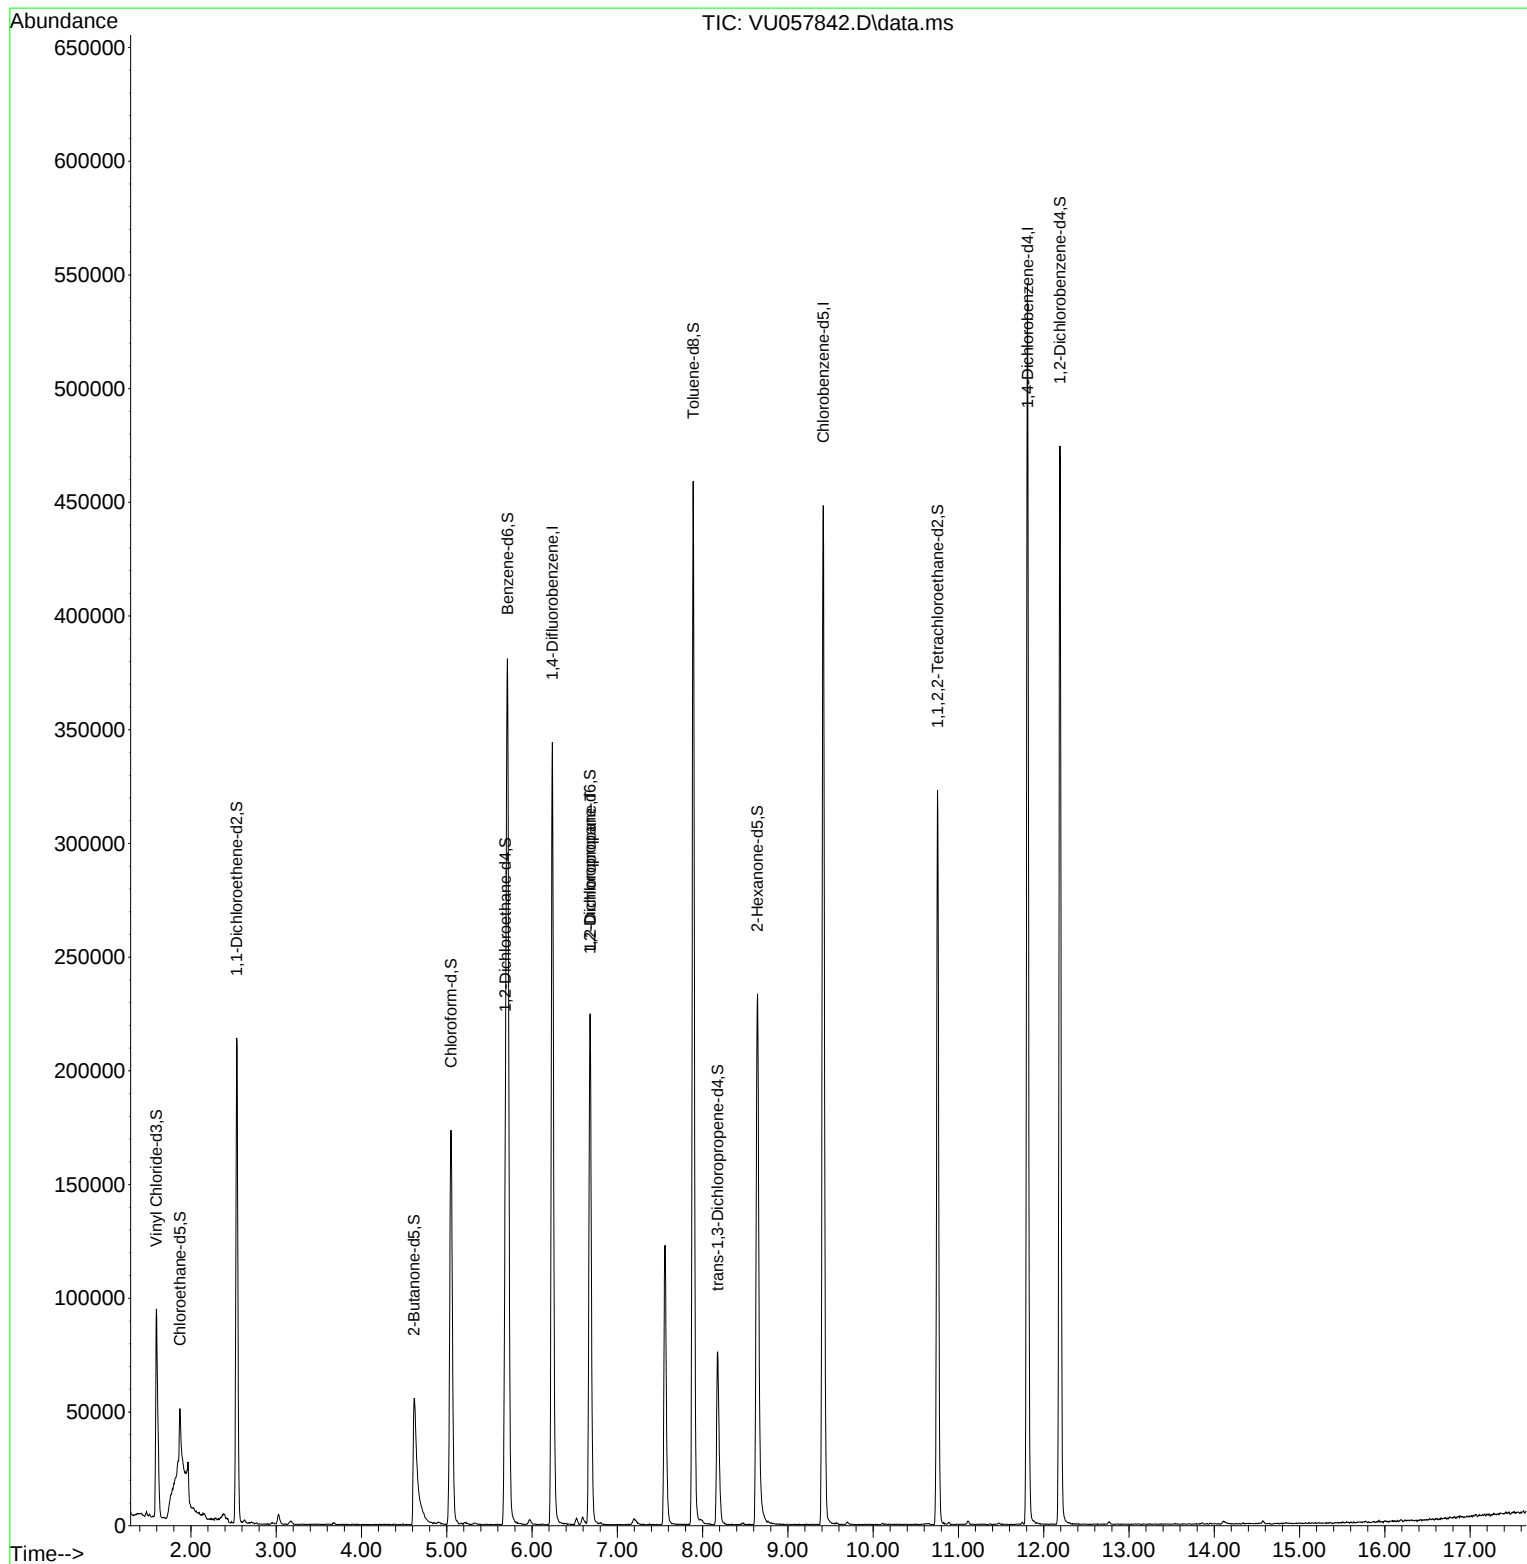

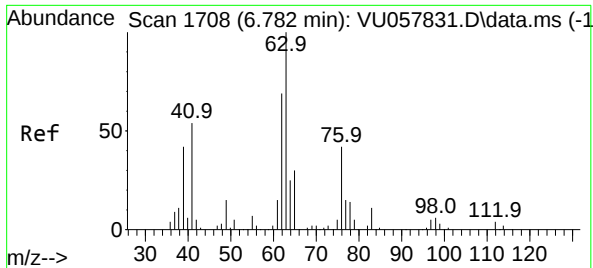

#37
 1,2-Dichloropropane
 Concen: 5.044 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.100 min
 Lab File: VU057842.D
 Acq: 07 Feb 2024 15:59

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 63 Resp: 11891
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.0 4.6#

