

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057843.D
 Acq On : 07 Feb 2024 16:23
 Operator : MD/SY
 Sample : P1329-09ME
 Misc : 5.23g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Feb 08 01:28:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 08 01:18:21 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	340981	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	338067	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	170305	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	148162	54.287	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 108.580%	
7) Chloroethane-d5	1.869	69	42571	20.106	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	= 40.220%#	
11) 1,1-Dichloroethene-d2	2.538	63	198717	39.644	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	= 79.280%	
21) 2-Butanone-d5	4.618	46	162645	107.380	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	= 107.380%	
24) Chloroform-d	5.049	84	252725	52.201	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 104.400%	
26) 1,2-Dichloroethane-d4	5.689	65	169299	55.162	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 110.320%	
32) Benzene-d6	5.711	84	526942	51.595	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 103.200%	
36) 1,2-Dichloropropane-d6	6.679	67	166343	51.576	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	= 103.160%	
41) Toluene-d8	7.891	98	475801	51.388	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 102.780%	
43) trans-1,3-Dichloroprop...	8.174	79	82812	52.488	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 104.980%	
47) 2-Hexanone-d5	8.643	63	162340	123.315	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	= 123.310%	
56) 1,1,2,2-Tetrachloroeth...	10.756	84	251935	60.007	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 120.020%#	
66) 1,2-Dichlorobenzene-d4	12.190	152	188940	57.746	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 115.500%	
Target Compounds						
37) 1,2-Dichloropropane	6.679	63	18472	6.296	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057843.D
Acq On : 07 Feb 2024 16:23
Operator : MD/SY
Sample : P1329-09ME
Misc : 5.23g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Feb 08 01:28:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 08 01:18:21 2024
Response via : Initial Calibration

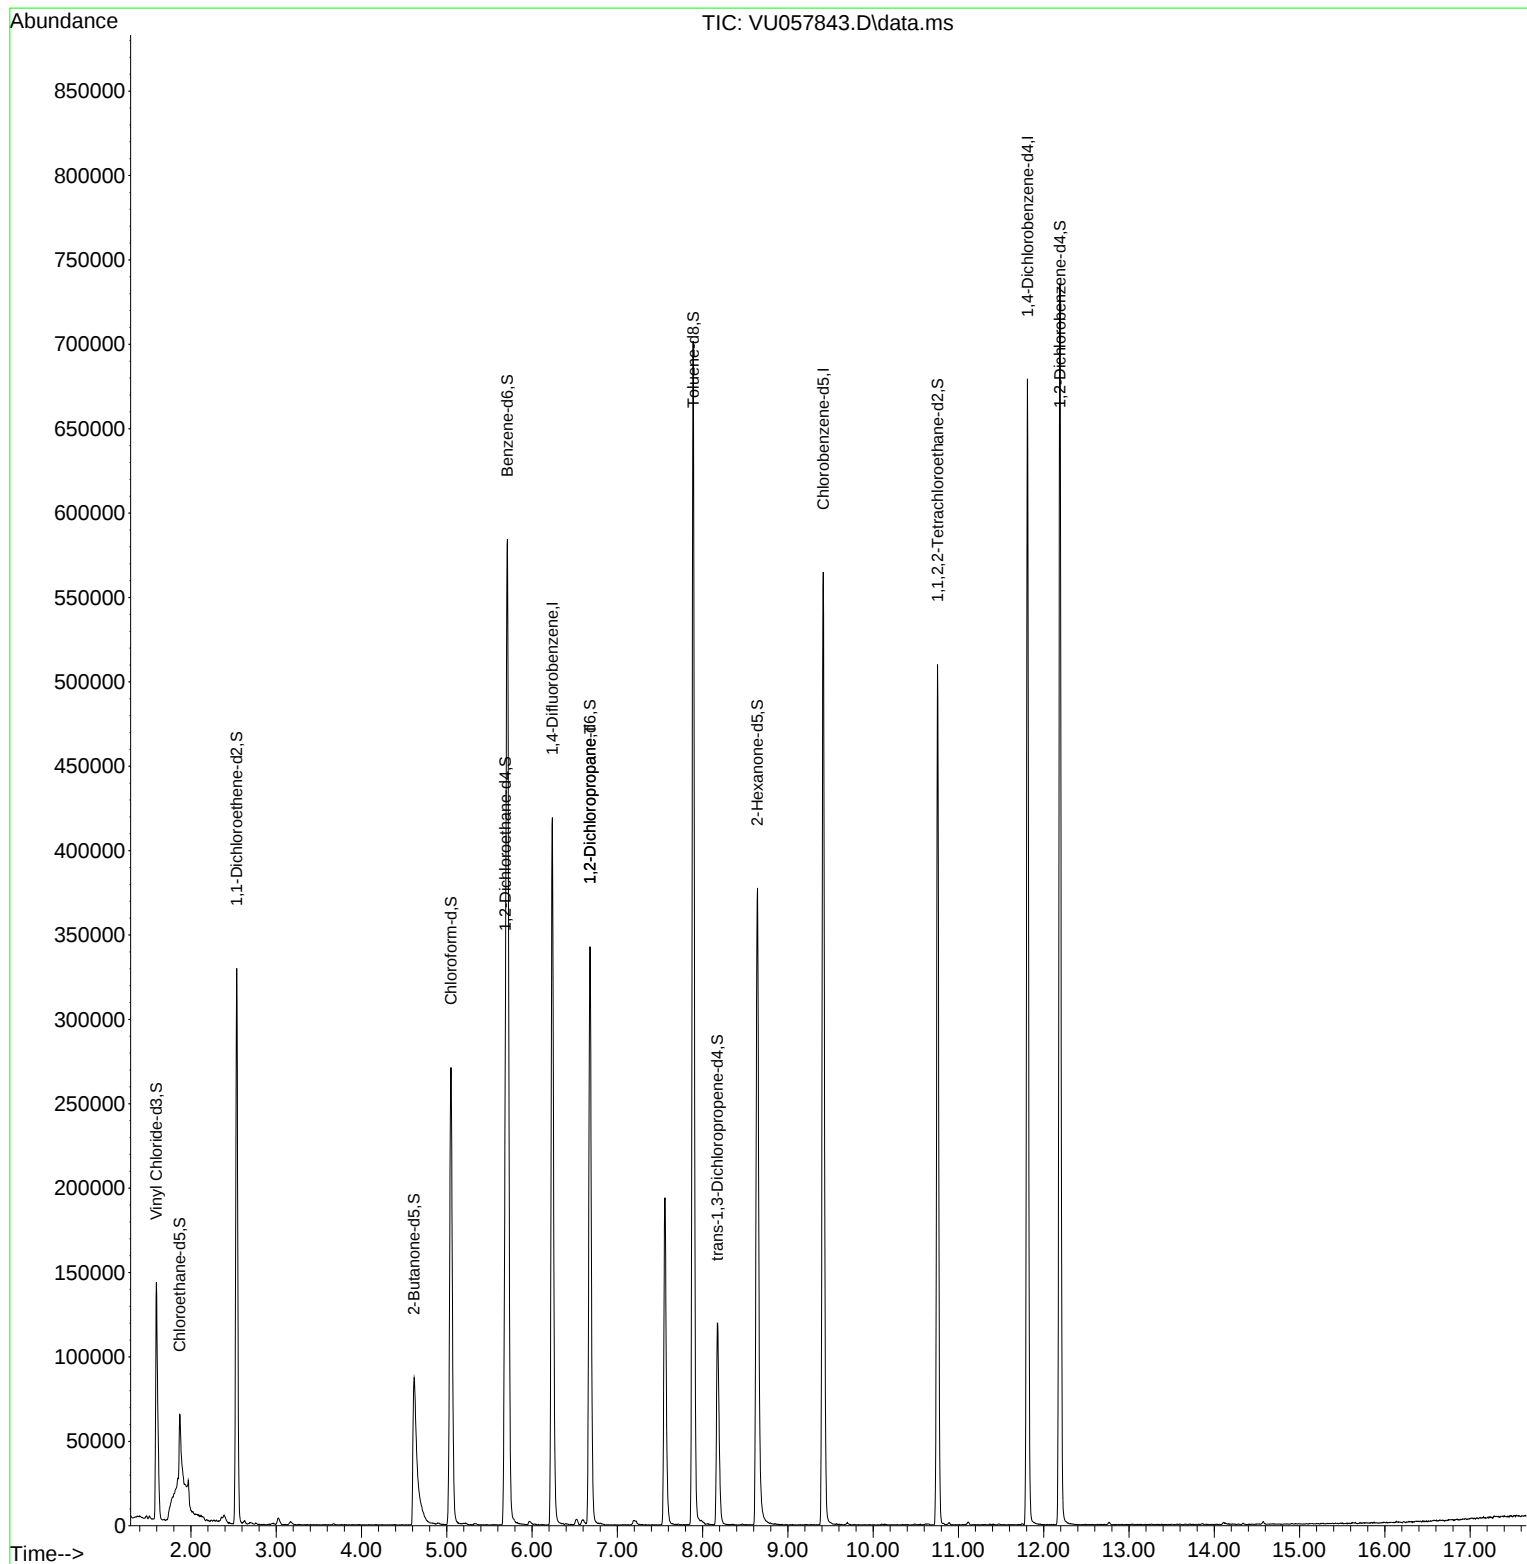

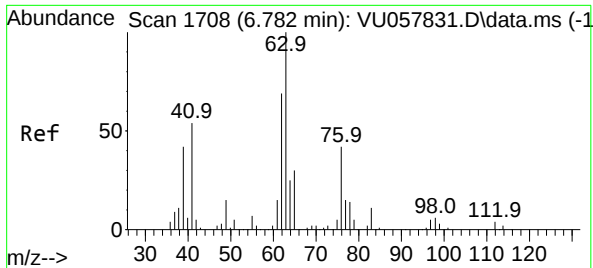

#37
1,2-Dichloropropane
Concen: 6.296 ug/L
RT: 6.679 min Scan# 1
Delta R.T. -0.103 min
Lab File: VU057843.D
Acq: 07 Feb 2024 16:23

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 18472
Ion Ratio Lower Upper
63 100
112 0.0 3.0 4.6#

