

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057836.D
 Acq On : 07 Feb 2024 13:33
 Operator : MD/SY
 Sample : VU0207WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M

Title : VOC Analysis

Signal : TIC: VU057836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	111	rVB	123240	152196	15.54%	2.057%
2	1.885	177	185	203	rVB	92882	137359	14.02%	1.856%
3	2.557	382	394	412	rBV	205639	335744	34.27%	4.537%
4	2.628	412	416	423	rVB4	1156	1227	0.13%	0.017%
5	2.692	434	436	439	rBV2	248	191	0.02%	0.003%
6	2.724	444	446	449	rVB2	209	132	0.01%	0.002%
7	2.779	456	463	473	rBV2	1362	2185	0.22%	0.030%
8	2.821	473	476	482	rVB2	232	223	0.02%	0.003%
9	3.004	530	533	535	rBV	257	184	0.02%	0.002%
10	3.033	535	542	553	rVV3	2847	5156	0.53%	0.070%
11	3.075	553	555	560	rVB	204	141	0.01%	0.002%
12	3.174	577	586	597	rVB2	1121	2331	0.24%	0.032%
13	3.245	603	608	610	rBV2	222	201	0.02%	0.003%
14	3.441	663	669	673	rBV2	192	241	0.02%	0.003%
15	3.666	736	739	745	rBV2	204	225	0.02%	0.003%
16	3.850	792	796	800	rVV	164	146	0.01%	0.002%
17	3.914	811	816	820	rBV2	313	383	0.04%	0.005%
18	4.145	885	888	891	rVB	238	163	0.02%	0.002%
19	4.348	948	951	954	rBV2	160	127	0.01%	0.002%
20	4.612	1023	1033	1065	rBV	68558	182213	18.60%	2.462%
21	4.981	1145	1148	1153	rBV3	202	161	0.02%	0.002%
22	5.052	1154	1170	1190	rBV	171423	376884	38.47%	5.093%
23	5.197	1212	1215	1219	rVB3	384	289	0.03%	0.004%
24	5.213	1219	1220	1223	rVB	293	156	0.02%	0.002%
25	5.232	1224	1226	1230	rVB2	397	261	0.03%	0.004%
26	5.255	1230	1233	1244	rVB4	360	496	0.05%	0.007%
27	5.329	1246	1256	1260	rBV3	692	1121	0.11%	0.015%
28	5.544	1320	1323	1328	rVB2	233	176	0.02%	0.002%
29	5.573	1328	1332	1336	rVB2	229	179	0.02%	0.002%
30	5.634	1344	1351	1353	rBV2	185	204	0.02%	0.003%
31	5.714	1356	1376	1415	rBV3	359191	979585	100.00%	13.238%
32	5.930	1440	1443	1450	rVB3	375	288	0.03%	0.004%
33	5.972	1453	1456	1458	rBV	285	174	0.02%	0.002%
34	6.010	1464	1468	1471	rBV3	319	287	0.03%	0.004%
35	6.049	1476	1480	1482	rBV3	314	256	0.03%	0.003%
36	6.078	1487	1489	1493	rVV2	239	139	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057836.D
 Acq On : 07 Feb 2024 13:33
 Operator : MD/SY
 Sample : VU0207WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	6.132	1503	1506	1511	rVB3	184	147	0.02%	0.002%
38	6.158	1511	1514	1518	rBV	170	135	0.01%	0.002%
39	6.242	1526	1540	1565	rBV	298743	567573	57.94%	7.670%
40	6.476	1610	1613	1617	rVB2	225	152	0.02%	0.002%
41	6.531	1620	1630	1638	rVB5	1421	2653	0.27%	0.036%
42	6.586	1643	1647	1648	rBV	232	167	0.02%	0.002%
43	6.682	1664	1677	1707	rBV	222605	433195	44.22%	5.854%
44	6.788	1708	1710	1712	rVB2	321	171	0.02%	0.002%
45	6.804	1712	1715	1717	rBV2	300	179	0.02%	0.002%
46	7.168	1823	1828	1834	rBV3	395	579	0.06%	0.008%
47	7.197	1835	1837	1841	rVV2	423	339	0.03%	0.005%
48	7.293	1863	1867	1871	rBV2	178	170	0.02%	0.002%
49	7.412	1901	1904	1908	rVB	172	147	0.02%	0.002%
50	7.560	1937	1950	1978	rBV	126153	227103	23.18%	3.069%
51	7.673	1983	1985	1990	rBV2	206	162	0.02%	0.002%
52	7.808	2023	2027	2032	rVB2	249	277	0.03%	0.004%
53	7.891	2040	2053	2076	rBV	443310	765317	78.13%	10.343%
54	8.174	2127	2141	2158	rBV	84194	146642	14.97%	1.982%
55	8.473	2224	2234	2241	rVB2	616	1027	0.10%	0.014%
56	8.554	2257	2259	2262	rVB2	422	264	0.03%	0.004%
57	8.628	2271	2282	2318	rBV	257507	493028	50.33%	6.663%
58	8.820	2340	2342	2347	rBV2	265	172	0.02%	0.002%
59	8.869	2354	2357	2359	rBV3	255	169	0.02%	0.002%
60	8.946	2378	2381	2384	rVB2	271	166	0.02%	0.002%
61	9.216	2462	2465	2469	rBV2	240	200	0.02%	0.003%
62	9.412	2513	2526	2554	rBV	408018	681994	69.62%	9.217%
63	9.650	2595	2600	2602	rBV	236	227	0.02%	0.003%
64	9.698	2609	2615	2625	rVB3	1146	1473	0.15%	0.020%
65	9.804	2644	2648	2649	rBV	225	154	0.02%	0.002%
66	10.036	2716	2720	2724	rVV2	162	148	0.02%	0.002%
67	10.100	2735	2740	2741	rBV	297	296	0.03%	0.004%
68	10.171	2758	2762	2765	rBV2	190	162	0.02%	0.002%
69	10.238	2779	2783	2787	rVB2	198	176	0.02%	0.002%
70	10.271	2788	2793	2797	rBV2	239	263	0.03%	0.004%
71	10.383	2824	2828	2832	rBV	164	157	0.02%	0.002%
72	10.409	2832	2836	2839	rVV2	227	173	0.02%	0.002%
73	10.454	2847	2850	2853	rBV2	176	137	0.01%	0.002%
74	10.586	2888	2891	2894	rVB	259	166	0.02%	0.002%
75	10.605	2894	2897	2901	rBV	193	183	0.02%	0.002%
76	10.750	2929	2942	2965	rBV	292524	490260	50.05%	6.626%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057836.D
 Acq On : 07 Feb 2024 13:33
 Operator : MD/SY
 Sample : VU0207WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	10.888	2979	2985	2992	rBV3	637	1016	0.10%	0.014%
78	11.200	3079	3082	3087	rVB2	274	240	0.02%	0.003%
79	11.245	3093	3096	3102	rBV2	154	194	0.02%	0.003%
80	11.476	3162	3168	3174	rVB4	795	1075	0.11%	0.015%
81	11.746	3246	3252	3259	rVB4	1232	1588	0.16%	0.021%
82	11.807	3259	3271	3292	rBV	429640	680863	69.51%	9.201%
83	11.930	3306	3309	3312	rVB2	365	255	0.03%	0.003%
84	11.975	3320	3323	3327	rVB2	206	169	0.02%	0.002%
85	12.187	3377	3389	3426	rBV	415048	698634	71.32%	9.442%
86	12.348	3437	3439	3442	rBV3	194	139	0.01%	0.002%
87	12.762	3565	3568	3576	rVB3	780	968	0.10%	0.013%
88	13.232	3705	3714	3725	rBV4	1566	2416	0.25%	0.033%
89	13.425	3770	3774	3783	rBV	231	380	0.04%	0.005%
90	13.811	3890	3894	3899	rBV2	329	330	0.03%	0.004%
91	13.849	3899	3906	3916	rVB3	2510	3336	0.34%	0.045%
92	14.106	3976	3986	3997	rBV3	2250	4437	0.45%	0.060%
93	14.203	4013	4016	4019	rVB2	469	300	0.03%	0.004%
94	14.331	4050	4056	4065	rVB4	2941	4191	0.43%	0.057%
95	14.405	4076	4079	4082	rBV	292	240	0.02%	0.003%
96	14.531	4115	4118	4121	rBV2	389	204	0.02%	0.003%
97	14.550	4121	4124	4125	rBV2	262	137	0.01%	0.002%
98	15.344	4369	4371	4376	rBV2	419	254	0.03%	0.003%
99	15.534	4427	4430	4435	rVB4	472	387	0.04%	0.005%
100	15.872	4533	4535	4538	rBV	482	269	0.03%	0.004%




Sum of corrected areas: 7399549

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057836.D
Acq On : 07 Feb 2024 13:33
Operator : MD/SY
Sample : VU0207WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

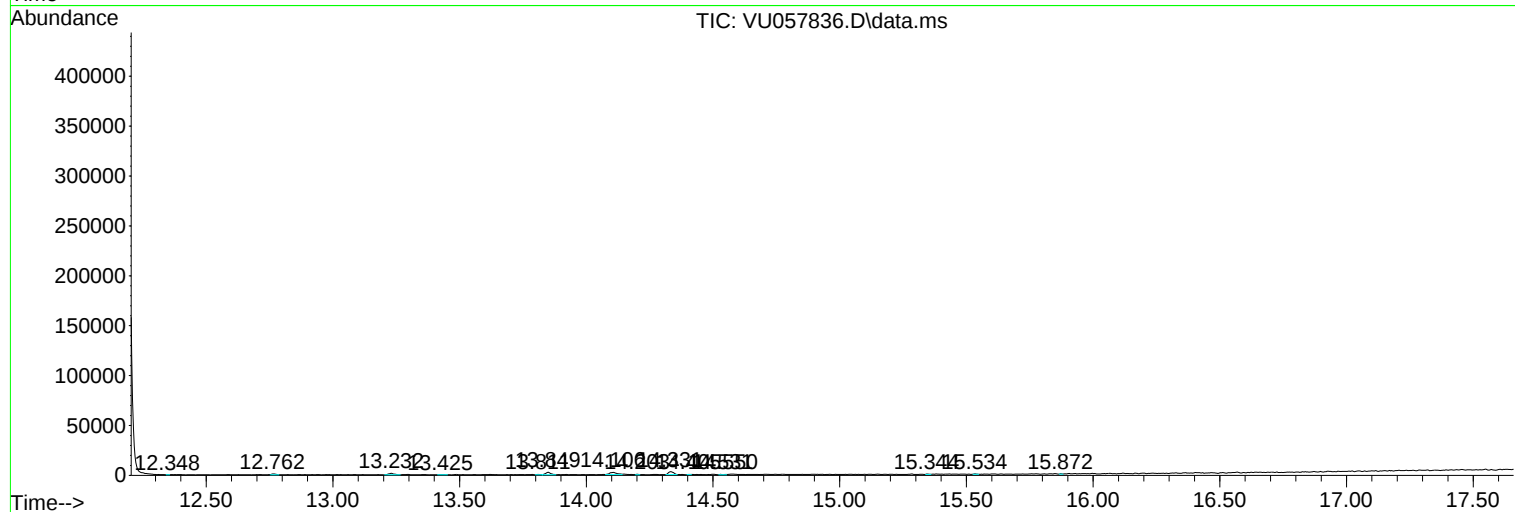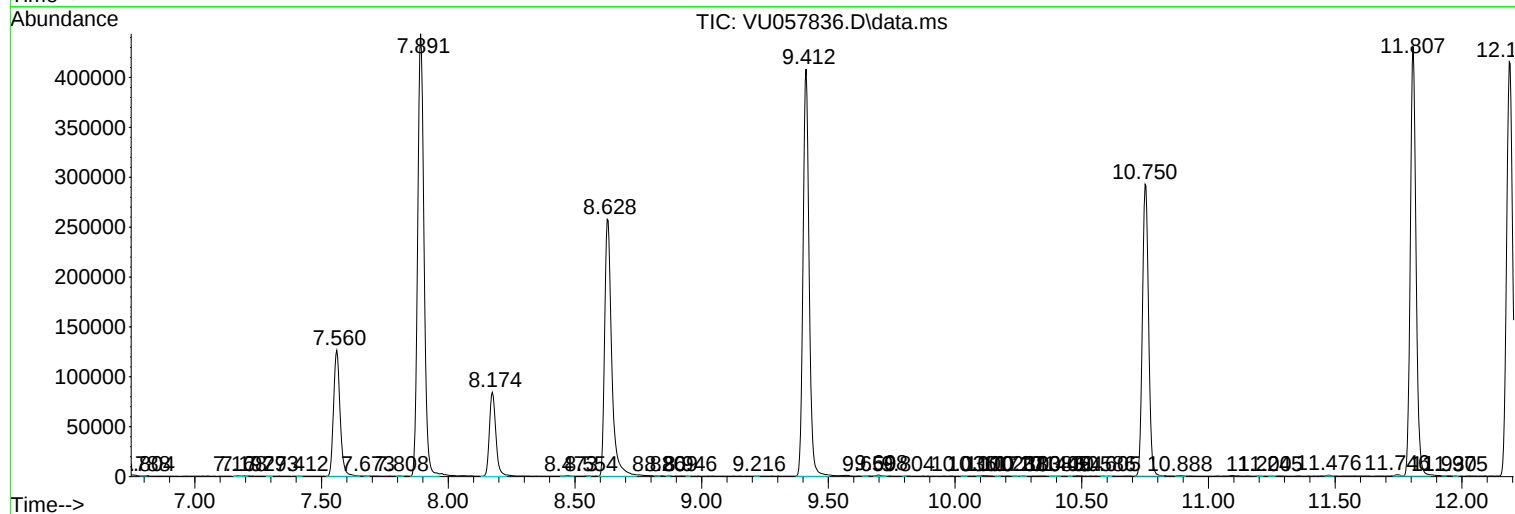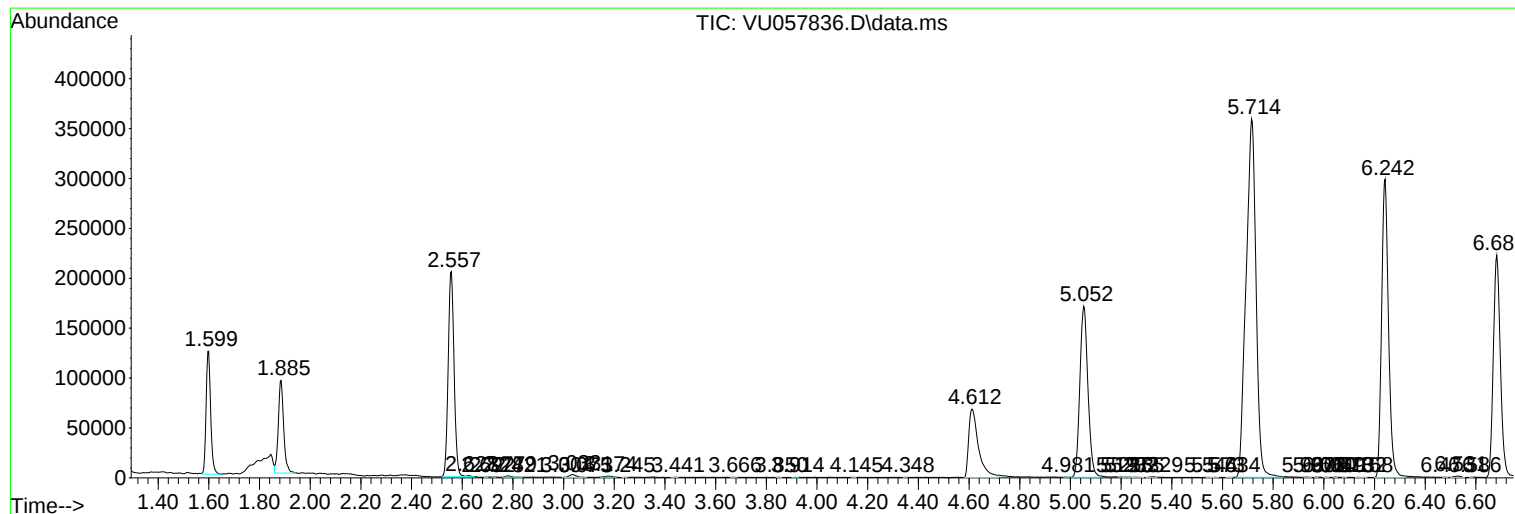

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057836.D
Acq On : 07 Feb 2024 13:33
Operator : MD/SY
Sample : VU0207WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057836.D
Acq On : 07 Feb 2024 13:33
Operator : MD/SY
Sample : VU0207WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------