

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057840.D
 Acq On : 07 Feb 2024 15:10
 Operator : MD/SY
 Sample : P1370-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

Signal : TIC: VU057840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	110	rVB	129598	153176	15.80%	2.074%
2	1.892	179	187	211	rVB	94969	135615	13.98%	1.836%
3	2.557	380	394	409	rBV	208450	337129	34.76%	4.565%
4	2.728	444	447	449	rBV	317	148	0.02%	0.002%
5	2.779	459	463	475	rVB2	775	1309	0.13%	0.018%
6	2.824	475	477	481	rBV	263	215	0.02%	0.003%
7	2.882	491	495	497	rBV2	187	170	0.02%	0.002%
8	3.036	533	543	553	rBV2	4861	8742	0.90%	0.118%
9	3.174	575	586	602	rBV3	2411	5042	0.52%	0.068%
10	3.316	627	630	633	rBV	199	135	0.01%	0.002%
11	3.641	724	731	734	rBV2	219	281	0.03%	0.004%
12	3.882	801	806	809	rVB	198	190	0.02%	0.003%
13	4.017	844	848	851	rBV	232	188	0.02%	0.003%
14	4.236	909	916	918	rBV2	135	159	0.02%	0.002%
15	4.358	949	954	959	rBV	218	263	0.03%	0.004%
16	4.399	963	967	971	rBV2	199	159	0.02%	0.002%
17	4.538	1005	1010	1012	rBV2	193	192	0.02%	0.003%
18	4.608	1023	1032	1068	rVV	71152	183889	18.96%	2.490%
19	4.911	1123	1126	1130	rBV3	407	259	0.03%	0.004%
20	5.052	1154	1170	1197	rBV	171663	379620	39.15%	5.141%
21	5.280	1238	1241	1243	rBV3	311	194	0.02%	0.003%
22	5.319	1249	1253	1254	rBV	224	167	0.02%	0.002%
23	5.374	1268	1270	1274	rVB2	330	204	0.02%	0.003%
24	5.489	1302	1306	1309	rBV2	184	155	0.02%	0.002%
25	5.715	1357	1376	1409	rBV2	353050	969751	100.00%	13.132%
26	6.020	1467	1471	1475	rBV2	191	227	0.02%	0.003%
27	6.113	1497	1500	1503	rBV2	315	189	0.02%	0.003%
28	6.242	1527	1540	1565	rBV	300678	576774	59.48%	7.811%
29	6.534	1624	1631	1638	rVB7	1107	1469	0.15%	0.020%
30	6.563	1638	1640	1644	rVB3	283	190	0.02%	0.003%
31	6.599	1645	1651	1652	rBV	430	351	0.04%	0.005%
32	6.682	1663	1677	1697	rBV	222070	429628	44.30%	5.818%
33	6.801	1712	1714	1720	rVB3	662	633	0.07%	0.009%
34	6.830	1721	1723	1727	rVV2	505	270	0.03%	0.004%
35	6.856	1729	1731	1736	rVB2	228	168	0.02%	0.002%
36	6.972	1763	1767	1772	rVB2	267	283	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057840.D
 Acq On : 07 Feb 2024 15:10
 Operator : MD/SY
 Sample : P1370-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	6.997	1772	1775	1778	rBV	210	176	0.02%	0.002%
38	7.126	1810	1815	1817	rBV	174	167	0.02%	0.002%
39	7.178	1826	1831	1832	rBV	491	425	0.04%	0.006%
40	7.370	1888	1891	1895	rVB2	163	136	0.01%	0.002%
41	7.432	1904	1910	1913	rBV2	205	218	0.02%	0.003%
42	7.560	1935	1950	1970	rBV	123779	223136	23.01%	3.022%
43	7.734	2000	2004	2007	rVB2	270	189	0.02%	0.003%
44	7.821	2028	2031	2034	rVB2	266	161	0.02%	0.002%
45	7.891	2040	2053	2075	rBV	445700	768927	79.29%	10.413%
46	8.132	2123	2128	2130	rBV2	261	200	0.02%	0.003%
47	8.174	2130	2141	2165	rVV	85267	147065	15.17%	1.992%
48	8.464	2226	2231	2235	rBV3	507	467	0.05%	0.006%
49	8.502	2241	2243	2247	rBV2	231	144	0.01%	0.002%
50	8.550	2257	2258	2264	rVB	373	195	0.02%	0.003%
51	8.628	2267	2282	2318	rBV	256606	479298	49.42%	6.491%
52	9.013	2399	2402	2405	rBV2	191	133	0.01%	0.002%
53	9.087	2422	2425	2429	rBV2	221	175	0.02%	0.002%
54	9.293	2483	2489	2496	rVB2	162	270	0.03%	0.004%
55	9.412	2510	2526	2557	rBV	411181	694456	71.61%	9.404%
56	9.573	2572	2576	2580	rVB3	731	670	0.07%	0.009%
57	9.595	2580	2583	2587	rBV	208	141	0.01%	0.002%
58	9.660	2600	2603	2607	rBV	229	139	0.01%	0.002%
59	9.698	2607	2615	2625	rBV	811	1508	0.16%	0.020%
60	9.817	2646	2652	2654	rBV	171	201	0.02%	0.003%
61	9.866	2664	2667	2673	rBV2	174	180	0.02%	0.002%
62	9.904	2673	2679	2682	rBV	240	248	0.03%	0.003%
63	10.097	2731	2739	2741	rBV3	463	534	0.06%	0.007%
64	10.422	2837	2840	2846	rVB2	212	156	0.02%	0.002%
65	10.480	2855	2858	2861	rBV2	259	205	0.02%	0.003%
66	10.750	2929	2942	2964	rVV	297430	481181	49.62%	6.516%
67	10.894	2978	2987	2992	rBV2	662	1006	0.10%	0.014%
68	11.274	3102	3105	3108	rVV2	276	185	0.02%	0.003%
69	11.419	3146	3150	3153	rVB2	186	157	0.02%	0.002%
70	11.438	3153	3156	3162	rBV2	169	173	0.02%	0.002%
71	11.473	3162	3167	3179	rVB4	677	1193	0.12%	0.016%
72	11.721	3241	3244	3246	rBV2	233	153	0.02%	0.002%
73	11.750	3246	3253	3258	rVB4	1119	1378	0.14%	0.019%
74	11.808	3258	3271	3294	rBV	427307	685487	70.69%	9.283%
75	11.975	3319	3323	3327	rVB3	417	460	0.05%	0.006%
76	12.007	3330	3333	3336	rVV	300	246	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057840.D
 Acq On : 07 Feb 2024 15:10
 Operator : MD/SY
 Sample : P1370-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	12.036	3339	3342	3347	rVB2	276	202	0.02%	0.003%
78	12.084	3352	3357	3361	rBV2	296	309	0.03%	0.004%
79	12.187	3377	3389	3417	rBV	411153	691115	71.27%	9.359%
80	12.370	3443	3446	3447	rBV	279	128	0.01%	0.002%
81	12.769	3566	3570	3581	rVB3	825	1032	0.11%	0.014%
82	12.853	3594	3596	3602	rVB2	373	267	0.03%	0.004%
83	12.923	3615	3618	3620	rBV	195	127	0.01%	0.002%
84	13.081	3663	3667	3671	rBV2	191	159	0.02%	0.002%
85	13.238	3713	3716	3720	rBV2	210	177	0.02%	0.002%
86	13.303	3732	3736	3740	rBV2	326	242	0.02%	0.003%
87	13.325	3740	3743	3745	rBV2	260	187	0.02%	0.003%
88	13.364	3752	3755	3757	rBV2	241	162	0.02%	0.002%
89	14.013	3954	3957	3961	rBV2	268	219	0.02%	0.003%
90	14.100	3975	3984	3991	rBV4	4734	7662	0.79%	0.104%
91	14.235	4022	4026	4027	rBV2	240	156	0.02%	0.002%
92	14.280	4037	4040	4042	rBV	258	179	0.02%	0.002%
93	14.332	4053	4056	4063	rVB4	762	828	0.09%	0.011%
94	14.631	4147	4149	4153	rBV	327	179	0.02%	0.002%
95	14.705	4168	4172	4174	rBV2	306	318	0.03%	0.004%
96	15.116	4297	4300	4304	rBV3	507	397	0.04%	0.005%
97	15.524	4425	4427	4430	rVB	339	148	0.02%	0.002%
98	15.682	4473	4476	4481	rBV2	505	333	0.03%	0.005%
99	15.737	4489	4493	4496	rBV3	466	423	0.04%	0.006%
100	15.949	4555	4559	4560	rBV2	586	496	0.05%	0.007%




Sum of corrected areas: 7384518

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057840.D
Acq On : 07 Feb 2024 15:10
Operator : MD/SY
Sample : P1370-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

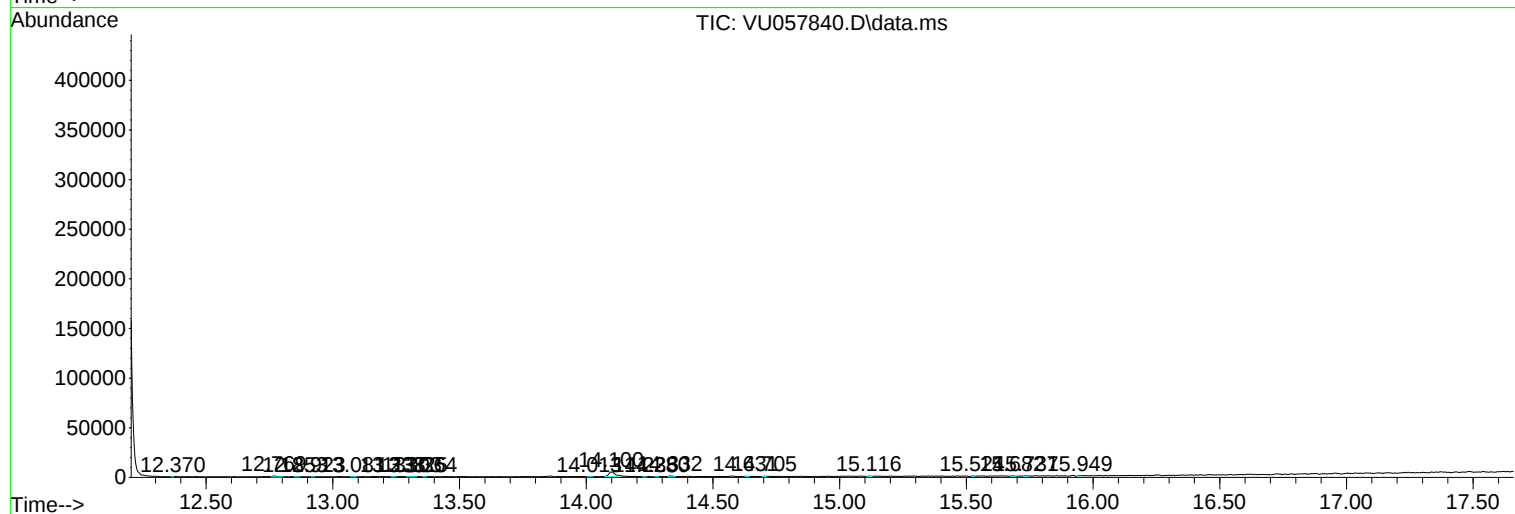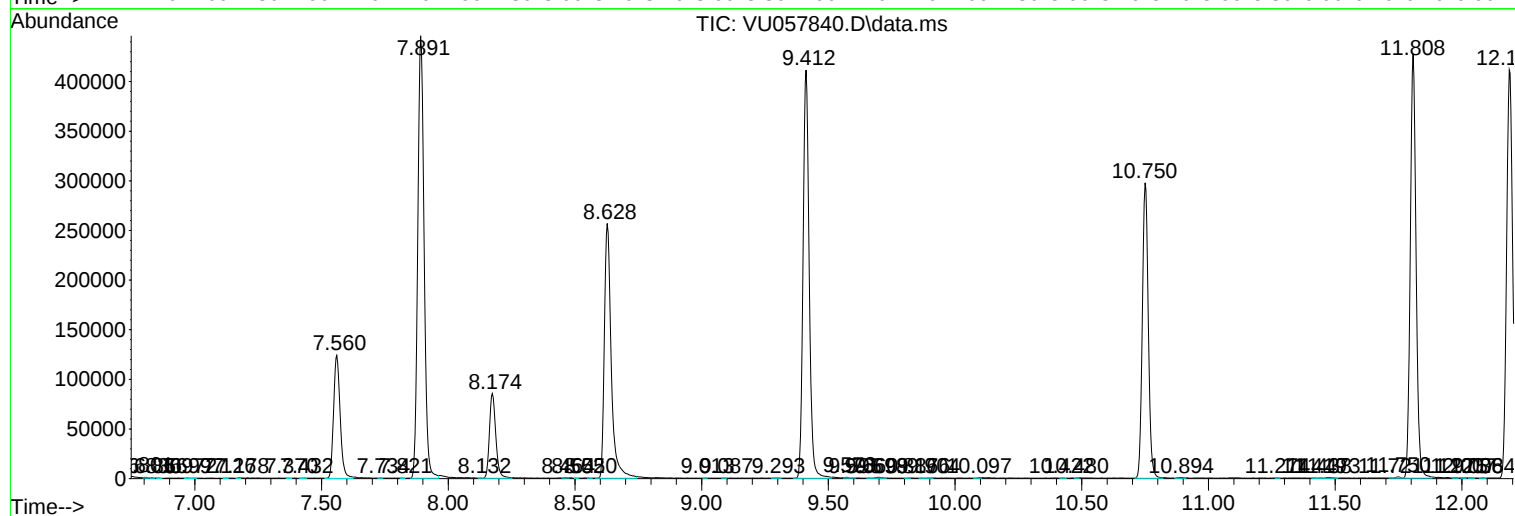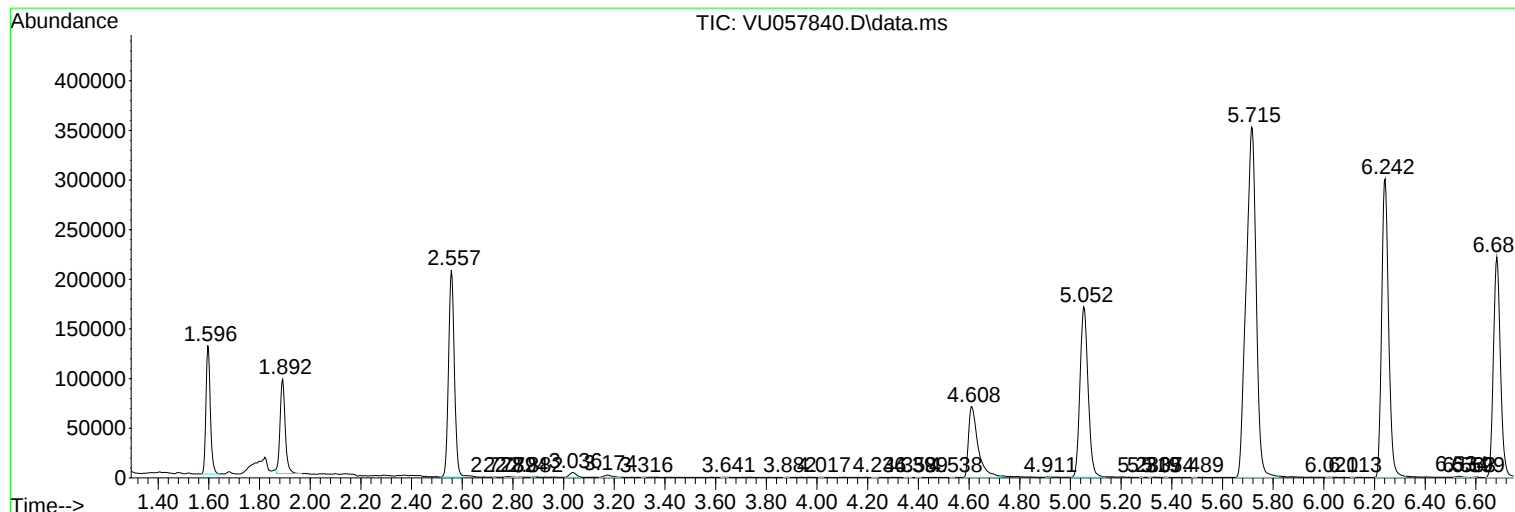

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057840.D
Acq On : 07 Feb 2024 15:10
Operator : MD/SY
Sample : P1370-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057840.D
Acq On : 07 Feb 2024 15:10
Operator : MD/SY
Sample : P1370-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc