

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057842.D
 Acq On : 07 Feb 2024 15:59
 Operator : MD/SY
 Sample : P1329-03ME
 Misc : 5.86g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COFLOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M

Title : VOC Analysis

Signal : TIC: VU057842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	117	rVB	91949	159142	15.89%	1.996%
2	2.538	377	388	404	rBV	213205	343254	34.27%	4.306%
3	2.898	497	500	502	rBV3	320	195	0.02%	0.002%
4	2.943	506	514	515	rBV	532	553	0.06%	0.007%
5	3.030	532	541	555	rVB4	4178	7861	0.78%	0.099%
6	3.168	573	584	585	rBV3	1344	1813	0.18%	0.023%
7	3.338	635	637	640	rVB	204	92	0.01%	0.001%
8	3.557	702	705	708	rBV	213	168	0.02%	0.002%
9	3.669	734	740	741	rBV	790	580	0.06%	0.007%
10	3.798	777	780	784	rVB2	157	100	0.01%	0.001%
11	3.898	801	811	813	rBV	206	309	0.03%	0.004%
12	3.930	816	821	824	rVV	209	209	0.02%	0.003%
13	3.949	824	827	831	rVB	281	174	0.02%	0.002%
14	3.972	831	834	838	rVB	136	101	0.01%	0.001%
15	4.010	842	846	851	rVB2	163	144	0.01%	0.002%
16	4.036	851	854	859	rBV2	161	146	0.01%	0.002%
17	4.081	865	868	871	rVB	146	92	0.01%	0.001%
18	4.322	940	943	947	rVB2	254	168	0.02%	0.002%
19	4.370	955	958	960	rBV2	149	106	0.01%	0.001%
20	4.525	1003	1006	1010	rBV	200	144	0.01%	0.002%
21	4.570	1015	1020	1023	rBV	76	85	0.01%	0.001%
22	4.618	1023	1035	1091	rBV	55487	191731	19.14%	2.405%
23	5.049	1154	1169	1191	rBV	173298	386118	38.55%	4.843%
24	5.206	1215	1218	1219	rBV3	674	435	0.04%	0.005%
25	5.277	1238	1240	1244	rVB2	164	96	0.01%	0.001%
26	5.300	1244	1247	1248	rBV	288	188	0.02%	0.002%
27	5.383	1270	1273	1277	rBV2	231	204	0.02%	0.003%
28	5.399	1277	1278	1282	rVB	180	77	0.01%	0.001%
29	5.457	1289	1296	1299	rBV	286	324	0.03%	0.004%
30	5.534	1317	1320	1325	rVB2	191	126	0.01%	0.002%
31	5.592	1334	1338	1343	rBV2	196	236	0.02%	0.003%
32	5.711	1355	1375	1404	rBV2	380713	1001691	100.00%	12.565%
33	5.972	1447	1456	1471	rBV7	1998	4030	0.40%	0.051%
34	6.190	1516	1524	1526	rBV2	161	195	0.02%	0.002%
35	6.238	1526	1539	1566	rBV	344027	653951	65.28%	8.203%
36	6.464	1607	1609	1613	rBV2	194	161	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057842.D
 Acq On : 07 Feb 2024 15:59
 Operator : MD/SY
 Sample : P1329-03ME
 Misc : 5.86g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COFLOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	6.521	1618	1627	1636	rBV7	2871	4902	0.49%	0.061%
38	6.592	1636	1649	1658	rBV3	3300	6622	0.66%	0.083%
39	6.682	1663	1677	1705	rVV	224227	440251	43.95%	5.522%
40	6.901	1742	1745	1747	rBV	125	77	0.01%	0.001%
41	6.988	1768	1772	1775	rBV2	121	94	0.01%	0.001%
42	7.004	1775	1777	1780	rBV2	131	80	0.01%	0.001%
43	7.036	1785	1787	1792	rBV2	123	88	0.01%	0.001%
44	7.094	1801	1805	1808	rBV2	166	124	0.01%	0.002%
45	7.123	1812	1814	1817	rBV	124	77	0.01%	0.001%
46	7.197	1825	1837	1841	rBV5	2503	4427	0.44%	0.056%
47	7.357	1879	1887	1890	rBV2	169	208	0.02%	0.003%
48	7.377	1890	1893	1896	rBV2	322	174	0.02%	0.002%
49	7.560	1938	1950	1975	rBV2	122870	232938	23.25%	2.922%
50	7.785	2017	2020	2023	rVB2	267	147	0.01%	0.002%
51	7.808	2023	2027	2029	rVB	228	166	0.02%	0.002%
52	7.833	2029	2035	2036	rBV2	237	167	0.02%	0.002%
53	7.891	2040	2053	2075	rBV	458706	805266	80.39%	10.101%
54	8.091	2112	2115	2117	rVB2	317	196	0.02%	0.002%
55	8.177	2130	2142	2164	rBV	75448	157047	15.68%	1.970%
56	8.303	2178	2181	2184	rBV	176	115	0.01%	0.001%
57	8.341	2192	2193	2197	rVB2	327	205	0.02%	0.003%
58	8.370	2197	2202	2204	rBV	123	116	0.01%	0.001%
59	8.454	2224	2228	2229	rBV2	468	269	0.03%	0.003%
60	8.547	2255	2257	2260	rVB	257	129	0.01%	0.002%
61	8.570	2260	2264	2266	rVB2	165	112	0.01%	0.001%
62	8.589	2266	2270	2273	rBV2	173	153	0.02%	0.002%
63	8.644	2273	2287	2322	rBV	233342	527603	52.67%	6.618%
64	8.949	2378	2382	2384	rBV	210	128	0.01%	0.002%
65	8.988	2390	2394	2398	rBV2	252	294	0.03%	0.004%
66	9.135	2438	2440	2445	rVB	180	83	0.01%	0.001%
67	9.180	2449	2454	2456	rVB2	147	111	0.01%	0.001%
68	9.197	2456	2459	2461	rBV2	118	78	0.01%	0.001%
69	9.322	2494	2498	2503	rBV2	207	250	0.02%	0.003%
70	9.415	2513	2527	2557	rBV	448102	842226	84.08%	10.565%
71	9.557	2569	2571	2572	rBV	311	94	0.01%	0.001%
72	9.698	2606	2615	2626	rBV3	1196	2195	0.22%	0.028%
73	9.743	2626	2629	2633	rVV	204	152	0.02%	0.002%
74	9.791	2641	2644	2647	rVB	159	94	0.01%	0.001%
75	9.817	2647	2652	2655	rBV2	156	173	0.02%	0.002%
76	10.033	2714	2719	2721	rBV2	198	166	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057842.D
 Acq On : 07 Feb 2024 15:59
 Operator : MD/SY
 Sample : P1329-03ME
 Misc : 5.86g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COFLOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	10.110	2735	2743	2749	rBV4	684	804	0.08%	0.010%
78	10.139	2749	2752	2756	rBV2	325	283	0.03%	0.004%
79	10.309	2802	2805	2808	rBV	192	112	0.01%	0.001%
80	10.367	2819	2823	2828	rBV	204	229	0.02%	0.003%
81	10.457	2848	2851	2853	rBV	148	98	0.01%	0.001%
82	10.483	2857	2859	2864	rVV2	243	202	0.02%	0.003%
83	10.521	2868	2871	2877	rVB2	210	179	0.02%	0.002%
84	10.557	2877	2882	2884	rBV2	182	159	0.02%	0.002%
85	10.573	2884	2887	2891	rBV2	174	177	0.02%	0.002%
86	10.756	2931	2944	2964	rBV	322922	538207	53.73%	6.751%
87	10.920	2992	2995	2996	rBV	194	113	0.01%	0.001%
88	11.377	3130	3137	3142	rBV4	412	540	0.05%	0.007%
89	11.415	3147	3149	3150	rBV4	242	118	0.01%	0.001%
90	11.811	3259	3272	3295	rBV	545626	863206	86.17%	10.828%
91	12.068	3348	3352	3358	rBV2	325	380	0.04%	0.005%
92	12.190	3377	3390	3412	rBV	474237	780098	77.88%	9.785%
93	12.634	3526	3528	3533	rVB2	246	171	0.02%	0.002%
94	12.721	3553	3555	3558	rBV	222	141	0.01%	0.002%
95	12.769	3563	3570	3579	rVB	1075	1750	0.17%	0.022%
96	12.907	3610	3613	3616	rBV	221	179	0.02%	0.002%
97	13.032	3649	3652	3654	rBV	243	167	0.02%	0.002%
98	13.370	3754	3757	3759	rBV2	192	137	0.01%	0.002%
99	13.794	3886	3889	3891	rBV	328	168	0.02%	0.002%
100	14.110	3977	3987	3988	rBV3	1319	1749	0.17%	0.022%




Sum of corrected areas: 7972163

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057842.D
Acq On : 07 Feb 2024 15:59
Operator : MD/SY
Sample : P1329-03ME
Misc : 5.86g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COFLOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

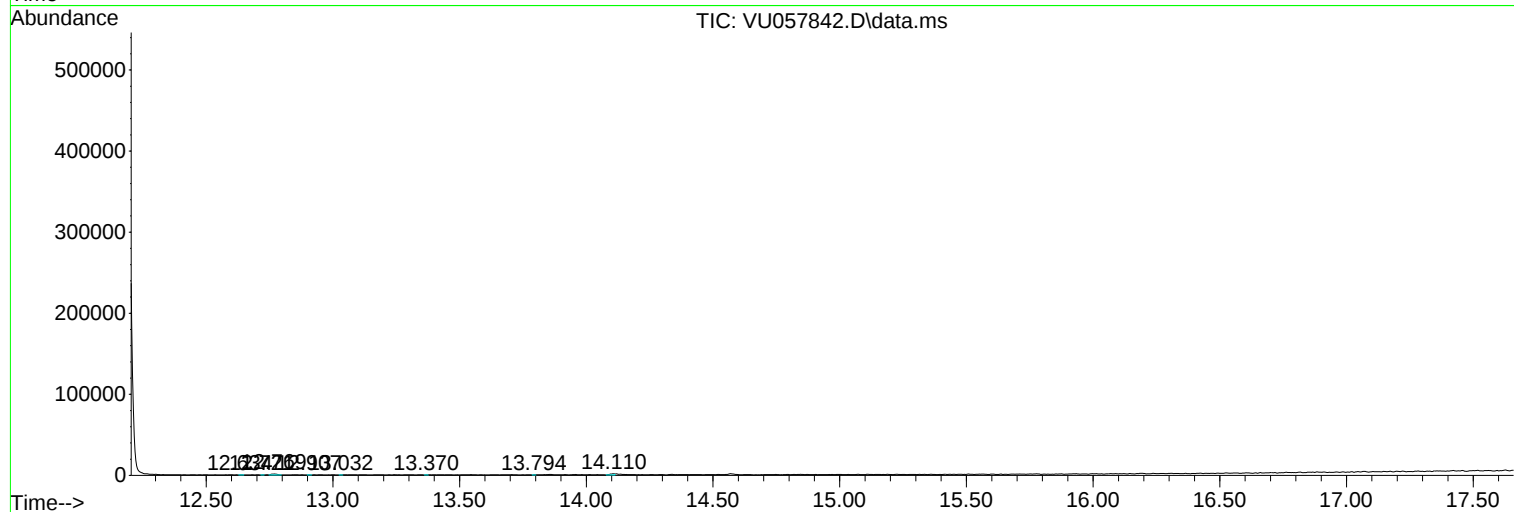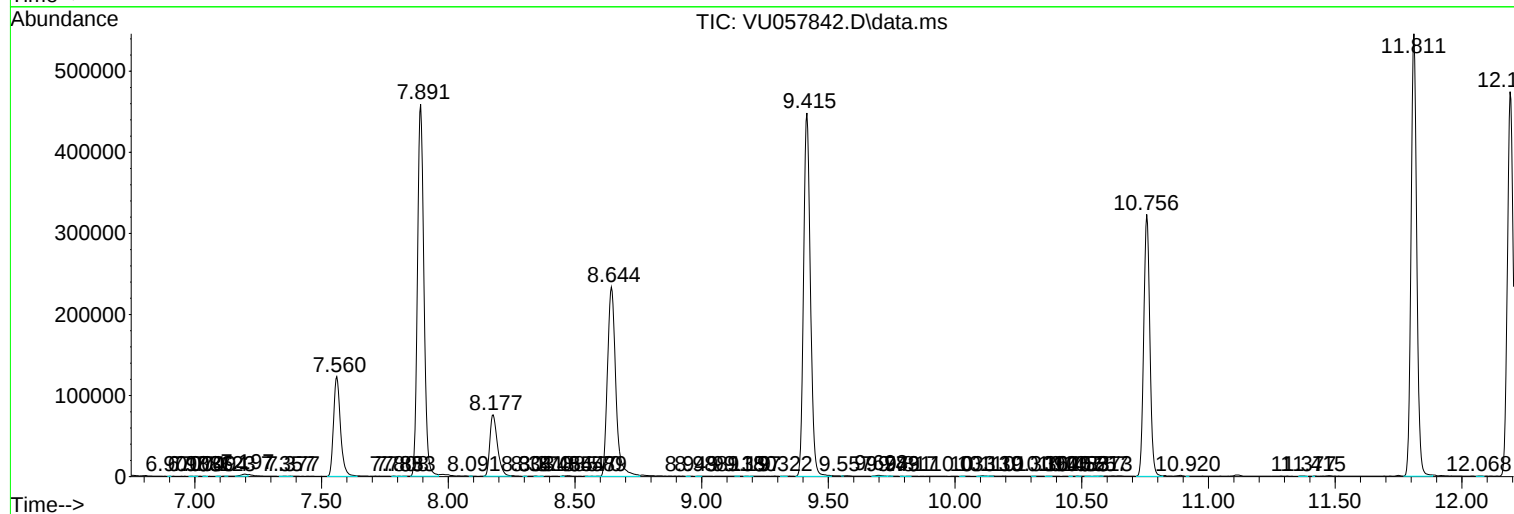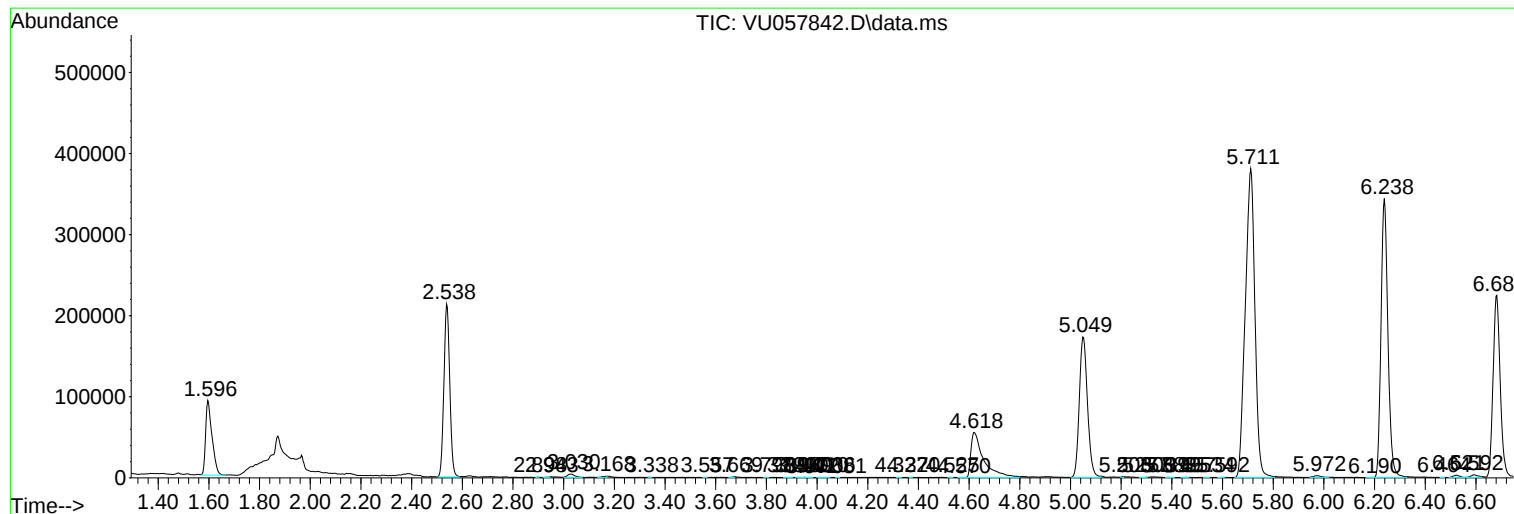

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057842.D
Acq On : 07 Feb 2024 15:59
Operator : MD/SY
Sample : P1329-03ME
Misc : 5.86g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COFLOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057842.D
Acq On : 07 Feb 2024 15:59
Operator : MD/SY
Sample : P1329-03ME
Misc : 5.86g/5.0ml/100uL//5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COFLOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------