

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057848.D
 Acq On : 07 Feb 2024 18:24
 Operator : MD/SY
 Sample : P1081-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

Signal : TIC: VU057848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	111	rVB	144185	169088	0.30%	0.124%
2	1.891	181	187	212	rVB	105793	148391	0.27%	0.109%
3	2.557	382	394	407	rBV	220018	358925	0.64%	0.263%
4	3.129	570	572	574	rBV2	475	217	0.00%	0.000%
5	3.178	574	587	604	rVB	8379	19498	0.03%	0.014%
6	3.679	741	743	746	rBV2	424	216	0.00%	0.000%
7	4.306	935	938	941	rBV2	332	255	0.00%	0.000%
8	4.351	949	952	954	rBV	184	119	0.00%	0.000%
9	4.422	972	974	980	rBV3	155	145	0.00%	0.000%
10	4.525	991	1006	1017	rBV5	2247	5413	0.01%	0.004%
11	4.615	1023	1034	1071	rBV2	74181	215327	0.39%	0.158%
12	4.985	1147	1149	1153	rBV	261	194	0.00%	0.000%
13	5.052	1155	1170	1201	rBV	187416	443570	0.79%	0.325%
14	5.370	1262	1269	1271	rBV5	1206	1351	0.00%	0.001%
15	5.483	1299	1304	1305	rBV2	260	224	0.00%	0.000%
16	5.576	1327	1333	1335	rBV3	278	249	0.00%	0.000%
17	5.718	1355	1377	1387	rBV2	387888	1062723	1.90%	0.779%
18	6.046	1476	1479	1482	rVB4	650	415	0.00%	0.000%
19	6.062	1482	1484	1487	rBV3	223	138	0.00%	0.000%
20	6.097	1492	1495	1497	rBB	193	94	0.00%	0.000%
21	6.123	1497	1503	1507	rBV3	505	613	0.00%	0.000%
22	6.142	1507	1509	1512	rVB	220	96	0.00%	0.000%
23	6.177	1519	1520	1523	rBV	174	90	0.00%	0.000%
24	6.242	1525	1540	1562	rBV	349116	662742	1.19%	0.486%
25	6.470	1608	1611	1612	rBV2	227	137	0.00%	0.000%
26	6.563	1637	1640	1643	rBV2	264	159	0.00%	0.000%
27	6.602	1643	1652	1654	rBV4	591	753	0.00%	0.001%
28	6.682	1663	1677	1697	rBV2	240748	469619	0.84%	0.344%
29	6.878	1735	1738	1740	rBV	242	196	0.00%	0.000%
30	6.968	1762	1766	1767	rVV	221	140	0.00%	0.000%
31	6.988	1770	1772	1774	rVV	312	134	0.00%	0.000%
32	7.010	1775	1779	1780	rVB2	238	120	0.00%	0.000%
33	7.033	1782	1786	1789	rBV2	200	116	0.00%	0.000%
34	7.120	1810	1813	1816	rBV	119	88	0.00%	0.000%
35	7.296	1866	1868	1870	rVB	188	97	0.00%	0.000%
36	7.338	1877	1881	1885	rBV2	362	320	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057848.D
 Acq On : 07 Feb 2024 18:24
 Operator : MD/SY
 Sample : P1081-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	7.393	1895	1898	1900	rVV2	219	126	0.00%	0.000%
38	7.406	1900	1902	1906	rVV	137	88	0.00%	0.000%
39	7.431	1907	1910	1913	rVB3	266	175	0.00%	0.000%
40	7.457	1913	1918	1924	rBV3	375	458	0.00%	0.000%
41	7.560	1938	1950	1977	rBV	141527	250875	0.45%	0.184%
42	7.808	2021	2027	2032	rVB4	446	571	0.00%	0.000%
43	7.837	2032	2036	2040	rBV	228	217	0.00%	0.000%
44	7.891	2040	2053	2073	rBV	486083	850956	1.52%	0.624%
45	8.174	2129	2141	2160	rBV	96887	166641	0.30%	0.122%
46	8.380	2201	2205	2209	rBV2	343	300	0.00%	0.000%
47	8.467	2220	2232	2243	rVB3	3661	6883	0.01%	0.005%
48	8.515	2243	2247	2252	rBV3	619	472	0.00%	0.000%
49	8.550	2252	2258	2265	rBV6	1396	2060	0.00%	0.002%
50	8.628	2269	2282	2318	rBV	291719	545381	0.98%	0.400%
51	8.853	2349	2352	2356	rVB2	230	133	0.00%	0.000%
52	8.885	2360	2362	2366	rVV2	253	163	0.00%	0.000%
53	8.920	2370	2373	2374	rBV	328	169	0.00%	0.000%
54	9.036	2407	2409	2410	rBV2	182	92	0.00%	0.000%
55	9.071	2417	2420	2423	rBV	188	134	0.00%	0.000%
56	9.087	2423	2425	2427	rVB	252	129	0.00%	0.000%
57	9.168	2448	2450	2452	rBV	150	85	0.00%	0.000%
58	9.187	2452	2456	2459	rBV2	452	371	0.00%	0.000%
59	9.277	2482	2484	2486	rBV	195	86	0.00%	0.000%
60	9.293	2486	2489	2490	rBV	176	80	0.00%	0.000%
61	9.332	2498	2501	2503	rBV2	216	112	0.00%	0.000%
62	9.348	2503	2506	2508	rVB3	351	210	0.00%	0.000%
63	9.441	2513	2535	2574	rBV2	2947350	5676217	10.15%	4.162%
64	9.904	2676	2679	2681	rVB3	318	167	0.00%	0.000%
65	10.010	2710	2712	2714	rBV	288	132	0.00%	0.000%
66	10.052	2722	2725	2726	rBV	194	112	0.00%	0.000%
67	10.087	2732	2736	2738	rBV2	281	228	0.00%	0.000%
68	10.110	2740	2743	2745	rBV2	306	213	0.00%	0.000%
69	10.190	2766	2768	2773	rVB2	371	233	0.00%	0.000%
70	10.219	2773	2777	2779	rBV2	234	175	0.00%	0.000%
71	10.251	2783	2787	2789	rBV3	314	229	0.00%	0.000%
72	10.316	2800	2807	2810	rBV3	423	453	0.00%	0.000%
73	10.418	2835	2839	2841	rBV	363	276	0.00%	0.000%
74	10.505	2864	2866	2869	rBV	244	124	0.00%	0.000%
75	10.595	2891	2894	2896	rBV	252	157	0.00%	0.000%
76	10.666	2914	2916	2920	rVB2	254	146	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057848.D
 Acq On : 07 Feb 2024 18:24
 Operator : MD/SY
 Sample : P1081-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	10.685	2920	2922	2925	rBV	212	159	0.00%	0.000%
78	10.750	2930	2942	2965	rBV	324052	535514	0.96%	0.393%
79	10.888	2977	2985	2997	rVB4	5505	8733	0.02%	0.006%
80	10.984	3010	3015	3025	rVB2	5586	7846	0.01%	0.006%
81	11.052	3033	3036	3040	rVB3	424	320	0.00%	0.000%
82	11.078	3040	3044	3045	rBV2	521	293	0.00%	0.000%
83	11.103	3046	3052	3053	rBV5	1547	1567	0.00%	0.001%
84	11.155	3065	3068	3071	rBV2	284	153	0.00%	0.000%
85	11.200	3080	3082	3085	rBV	189	131	0.00%	0.000%
86	11.386	3136	3140	3143	rVB3	357	311	0.00%	0.000%
87	11.473	3159	3167	3169	rBV5	715	869	0.00%	0.001%
88	11.621	3210	3213	3215	rBV	254	141	0.00%	0.000%
89	11.740	3236	3250	3263	rVV	6524263	10302515	18.43%	7.554%
90	11.836	3264	3280	3325	rVB	24240194	39489693	70.64%	28.956%
91	12.216	3378	3398	3437	rBV	33364342	55902857	100.00%	40.991%
92	12.968	3622	3632	3650	rVB3	45022	74784	0.13%	0.055%
93	13.148	3678	3688	3701	rBV4	14171	31770	0.06%	0.023%
94	13.219	3703	3710	3719	rVB6	6323	9872	0.02%	0.007%
95	13.325	3733	3743	3758	rVB2	29302	47571	0.09%	0.035%
96	13.836	3887	3902	3940	rBV	8578877	13433132	24.03%	9.850%
97	14.087	3975	3980	3991	rVB2	3711	4932	0.01%	0.004%
98	14.325	4039	4054	4077	rBV	3451941	5413494	9.68%	3.969%
99	14.553	4122	4125	4128	rBV3	818	694	0.00%	0.001%
100	15.997	4566	4574	4589	rVB2	27111	42755	0.08%	0.031%




Sum of corrected areas: 136377907

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057848.D
Acq On : 07 Feb 2024 18:24
Operator : MD/SY
Sample : P1081-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

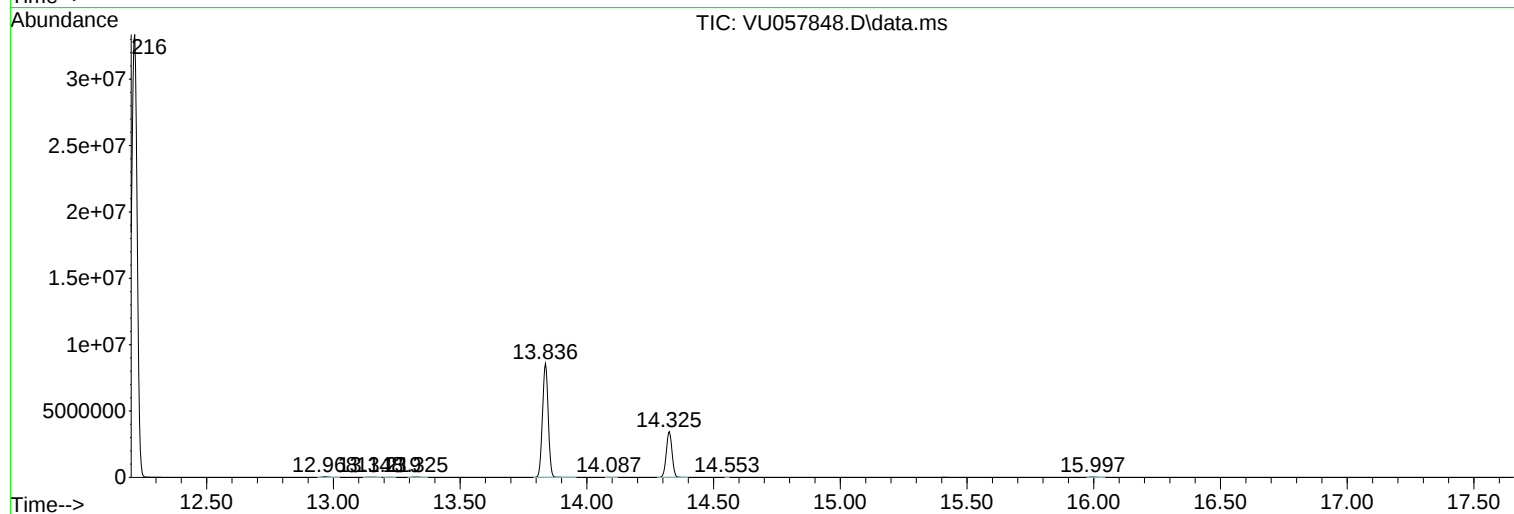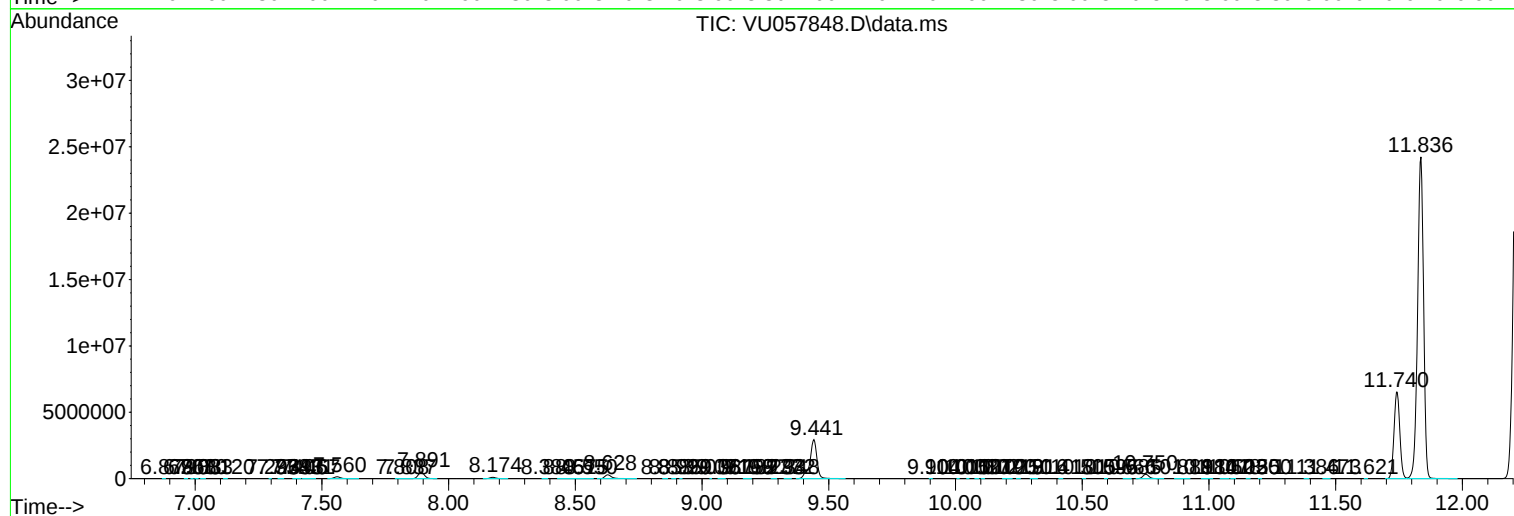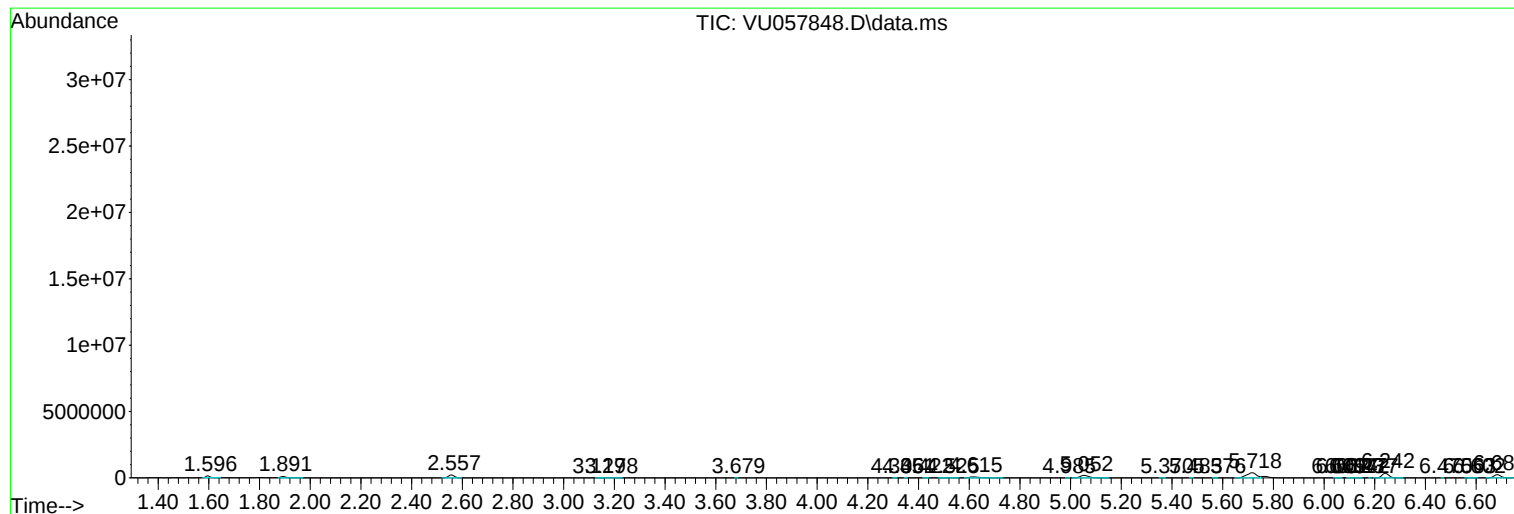

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057848.D
Acq On : 07 Feb 2024 18:24
Operator : MD/SY
Sample : P1081-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057848.D
Acq On : 07 Feb 2024 18:24
Operator : MD/SY
Sample : P1081-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------