

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057849.D
 Acq On : 07 Feb 2024 18:48
 Operator : MD/SY
 Sample : P1081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M

Title : VOC Analysis

Signal : TIC: VU057849.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	113	rVB	145878	173176	0.68%	0.169%
2	1.888	179	186	198	rVB	102196	139314	0.55%	0.136%
3	2.557	381	394	408	rBV	218949	358208	1.41%	0.349%
4	2.763	450	458	459	rBV4	1131	1280	0.01%	0.001%
5	2.949	512	516	520	rBV3	302	364	0.00%	0.000%
6	3.036	535	543	553	rBV5	2462	4636	0.02%	0.005%
7	3.129	566	572	574	rVV	870	1010	0.00%	0.001%
8	3.177	574	587	604	rVB	8051	18713	0.07%	0.018%
9	3.345	637	639	645	rBV2	212	201	0.00%	0.000%
10	3.576	708	711	715	rVB2	260	220	0.00%	0.000%
11	3.611	715	722	725	rVB	328	334	0.00%	0.000%
12	3.730	756	759	764	rVB	285	274	0.00%	0.000%
13	3.759	764	768	772	rBV2	387	393	0.00%	0.000%
14	3.920	813	818	821	rBV3	288	318	0.00%	0.000%
15	3.955	826	829	833	rBV	338	283	0.00%	0.000%
16	4.158	889	892	895	rBV3	252	215	0.00%	0.000%
17	4.187	895	901	906	rVB3	246	231	0.00%	0.000%
18	4.255	916	922	925	rBV2	266	251	0.00%	0.000%
19	4.412	965	971	975	rBV2	375	356	0.00%	0.000%
20	4.470	986	989	993	rVB3	270	195	0.00%	0.000%
21	4.521	993	1005	1016	rBV8	2143	4666	0.02%	0.005%
22	4.618	1022	1035	1080	rBV2	69170	216115	0.85%	0.211%
23	4.878	1113	1116	1120	rVB2	362	283	0.00%	0.000%
24	4.901	1120	1123	1127	rBV	369	301	0.00%	0.000%
25	5.055	1150	1171	1200	rBV2	192692	497230	1.96%	0.485%
26	5.213	1217	1220	1226	rVB3	428	283	0.00%	0.000%
27	5.277	1238	1240	1244	rVB3	365	250	0.00%	0.000%
28	5.309	1244	1250	1252	rBV2	654	602	0.00%	0.001%
29	5.380	1266	1272	1281	rVB5	1613	2504	0.01%	0.002%
30	5.441	1288	1291	1296	rBV	310	200	0.00%	0.000%
31	5.515	1301	1314	1329	rBV4	10552	23333	0.09%	0.023%
32	5.717	1355	1377	1380	rBV2	406827	906035	3.57%	0.883%
33	5.766	1381	1392	1426	rVB	4562507	9317628	36.71%	9.084%
34	6.242	1526	1540	1568	rBV	333512	635162	2.50%	0.619%
35	6.528	1623	1629	1631	rBV4	802	604	0.00%	0.001%
36	6.547	1631	1635	1639	rVB4	642	540	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057849.D
 Acq On : 07 Feb 2024 18:48
 Operator : MD/SY
 Sample : P1081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	6.589	1645	1648	1652	rBV3	554	457	0.00%	0.000%
38	6.682	1663	1677	1705	rBV	241746	473990	1.87%	0.462%
39	6.846	1725	1728	1731	rVB2	417	219	0.00%	0.000%
40	6.901	1742	1745	1755	rVB	284	243	0.00%	0.000%
41	7.560	1938	1950	1973	rBV	140885	250529	0.99%	0.244%
42	7.676	1979	1986	1994	rVB6	1128	1806	0.01%	0.002%
43	7.756	2009	2011	2015	rVB2	335	251	0.00%	0.000%
44	7.785	2015	2020	2022	rBV	282	201	0.00%	0.000%
45	7.891	2040	2053	2071	rBV	488429	843608	3.32%	0.822%
46	8.174	2125	2141	2160	rBV	95716	164067	0.65%	0.160%
47	8.422	2214	2218	2223	rBV2	379	438	0.00%	0.000%
48	8.467	2223	2232	2247	rVB3	4090	7922	0.03%	0.008%
49	8.547	2251	2257	2264	rVB4	1090	1244	0.00%	0.001%
50	8.627	2271	2282	2312	rBV	300510	551594	2.17%	0.538%
51	9.004	2394	2399	2404	rVB2	193	217	0.00%	0.000%
52	9.119	2429	2435	2440	rBV2	229	197	0.00%	0.000%
53	9.145	2440	2443	2446	rBV3	325	195	0.00%	0.000%
54	9.167	2446	2450	2457	rVB3	275	323	0.00%	0.000%
55	9.441	2513	2535	2576	rBV	11780358	20279481	79.90%	19.770%
56	9.733	2624	2626	2628	rVB	537	266	0.00%	0.000%
57	9.939	2687	2690	2693	rBV2	306	250	0.00%	0.000%
58	10.026	2712	2717	2718	rBV2	246	212	0.00%	0.000%
59	10.055	2721	2726	2729	rBV3	360	302	0.00%	0.000%
60	10.100	2735	2740	2745	rBV4	538	792	0.00%	0.001%
61	10.235	2776	2782	2785	rVB3	308	314	0.00%	0.000%
62	10.476	2855	2857	2862	rBV3	354	223	0.00%	0.000%
63	10.749	2929	2942	2963	rBV	325380	542676	2.14%	0.529%
64	10.888	2973	2985	2996	rVB3	5832	9659	0.04%	0.009%
65	10.984	3008	3015	3029	rVB3	3783	5361	0.02%	0.005%
66	11.087	3040	3047	3048	rBV3	593	490	0.00%	0.000%
67	11.103	3048	3052	3054	rBV4	1126	948	0.00%	0.001%
68	11.441	3152	3157	3161	rVB2	207	201	0.00%	0.000%
69	11.463	3161	3164	3165	rBV	400	253	0.00%	0.000%
70	11.544	3184	3189	3192	rBV2	228	227	0.00%	0.000%
71	11.640	3211	3219	3221	rBV	441	458	0.00%	0.000%
72	11.740	3236	3250	3262	rBV	3886461	6057790	23.87%	5.906%
73	11.833	3262	3279	3317	rVB	15813656	25380493	100.00%	24.743%
74	12.209	3378	3396	3430	rBV	14725771	23972565	94.45%	23.370%
75	12.601	3514	3518	3524	rBV4	422	571	0.00%	0.001%
76	12.724	3553	3556	3560	rBV2	360	371	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057849.D
 Acq On : 07 Feb 2024 18:48
 Operator : MD/SY
 Sample : P1081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	12.765	3562	3569	3583	rVV2	3325	5600	0.02%	0.005%
78	12.891	3605	3608	3610	rBV2	404	214	0.00%	0.000%
79	12.971	3622	3633	3646	rVB2	21659	35296	0.14%	0.034%
80	13.064	3658	3662	3666	rVV3	319	364	0.00%	0.000%
81	13.148	3676	3688	3700	rBV4	13317	30862	0.12%	0.030%
82	13.216	3700	3709	3719	rVB6	13603	24547	0.10%	0.024%
83	13.325	3733	3743	3756	rBV4	15171	24454	0.10%	0.024%
84	13.492	3790	3795	3797	rBV2	281	284	0.00%	0.000%
85	13.540	3805	3810	3811	rBV2	304	279	0.00%	0.000%
86	13.566	3814	3818	3820	rBV4	1137	882	0.00%	0.001%
87	13.656	3844	3846	3849	rVB2	364	195	0.00%	0.000%
88	13.691	3853	3857	3863	rVV2	583	546	0.00%	0.001%
89	13.836	3888	3902	3932	rBV	4905104	7608245	29.98%	7.417%
90	14.048	3966	3968	3971	rVB	476	281	0.00%	0.000%
91	14.090	3972	3981	3991	rVV2	2071	3682	0.01%	0.004%
92	14.154	3999	4001	4003	rBV	419	258	0.00%	0.000%
93	14.325	4040	4054	4078	rBV	2459716	3872776	15.26%	3.775%
94	14.495	4103	4107	4109	rBV3	437	417	0.00%	0.000%
95	14.527	4115	4117	4120	rBV2	579	352	0.00%	0.000%
96	14.871	4216	4224	4226	rBV4	818	1046	0.00%	0.001%
97	15.029	4270	4273	4278	rVB3	457	316	0.00%	0.000%
98	15.209	4327	4329	4332	rBV2	324	236	0.00%	0.000%
99	15.412	4380	4392	4407	rVB4	22465	39485	0.16%	0.038%
100	15.994	4564	4573	4589	rVB2	41539	69676	0.27%	0.068%




Sum of corrected areas: 102577405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057849.D
Acq On : 07 Feb 2024 18:48
Operator : MD/SY
Sample : P1081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

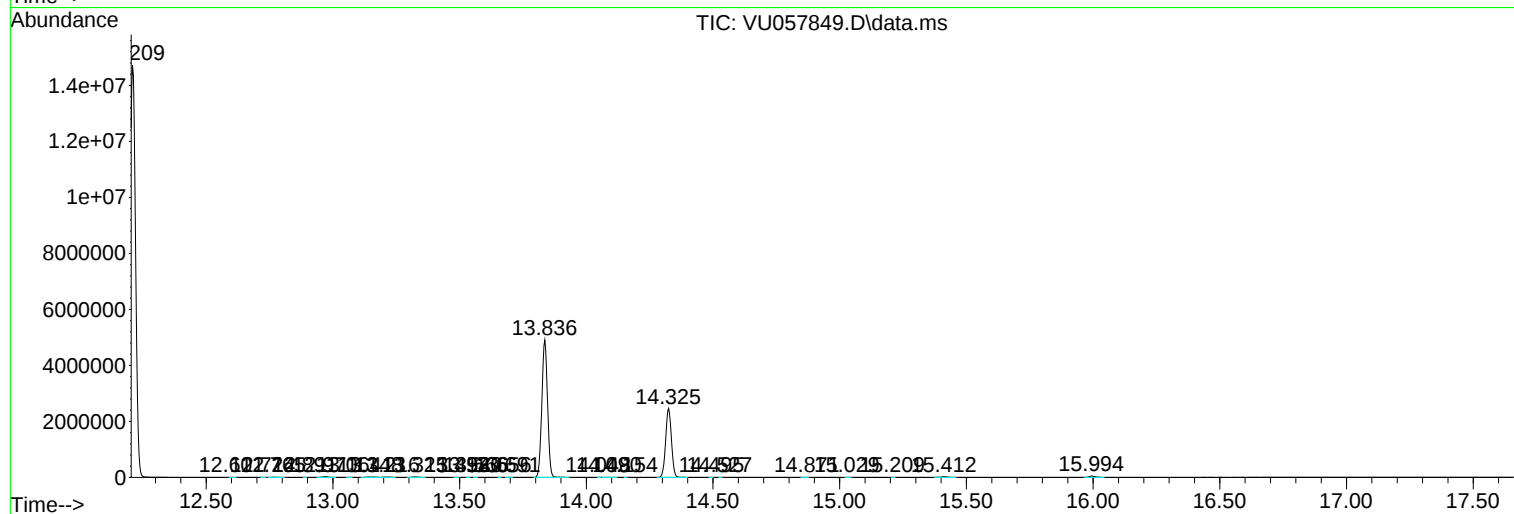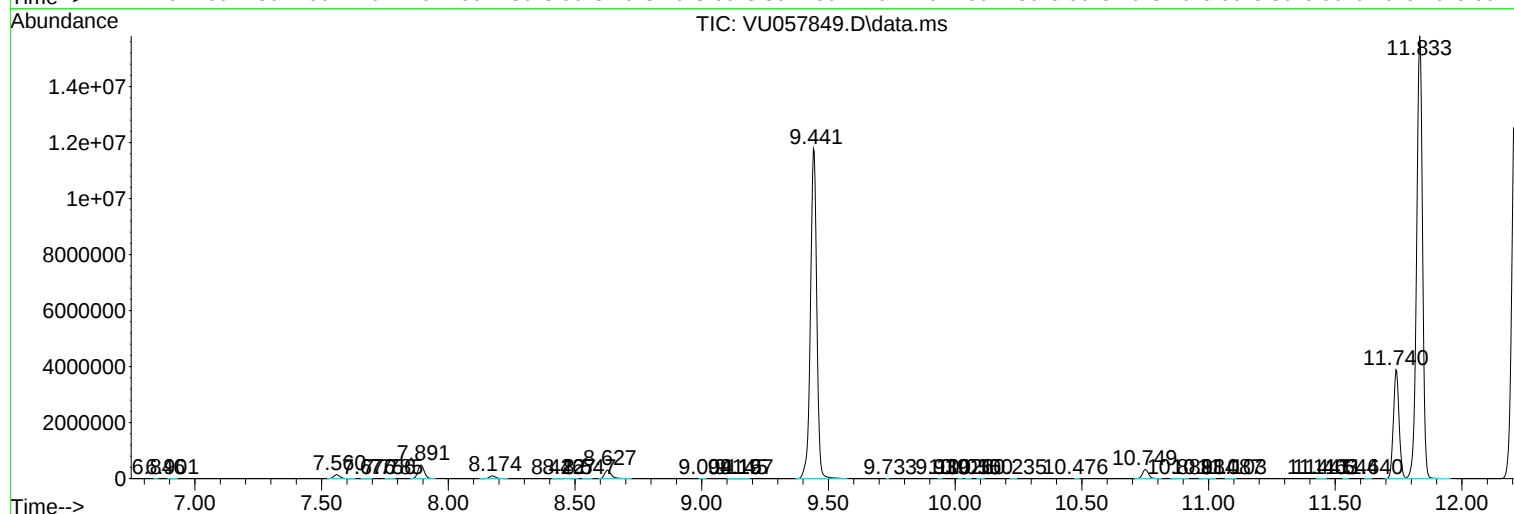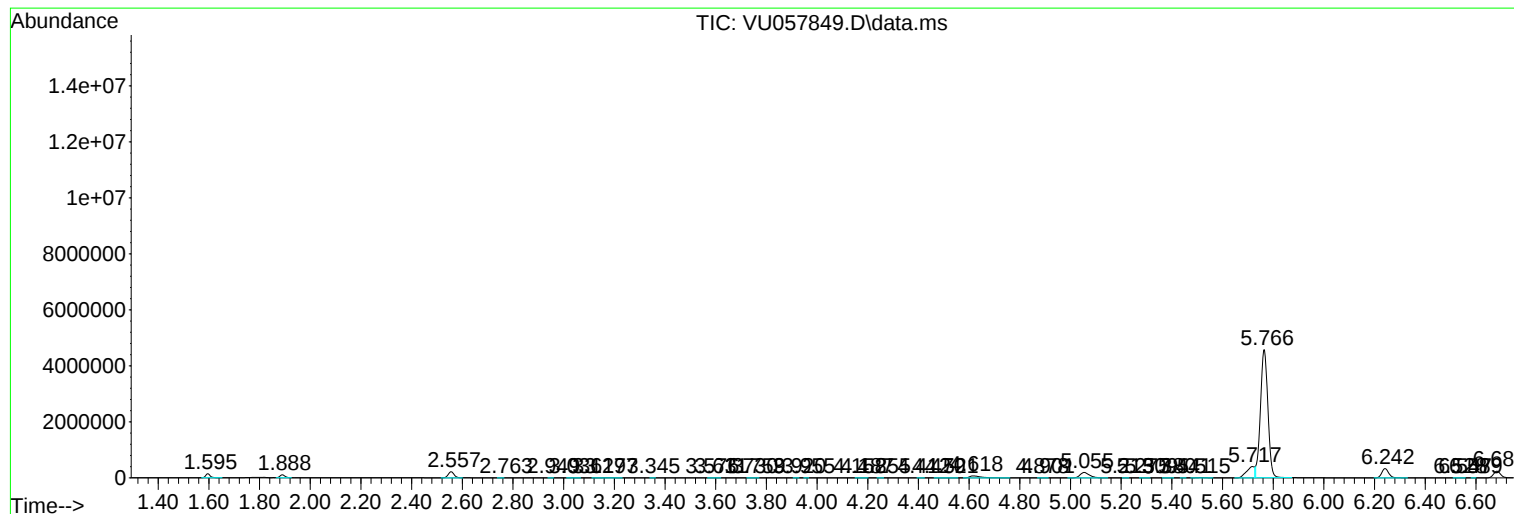

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057849.D
Acq On : 07 Feb 2024 18:48
Operator : MD/SY
Sample : P1081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057849.D
Acq On : 07 Feb 2024 18:48
Operator : MD/SY
Sample : P1081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------