

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057851.D
 Acq On : 07 Feb 2024 19:45
 Operator : MD/SY
 Sample : P1081-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M

Title : VOC Analysis

Signal : TIC: VU057851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	111	rVB	158150	184184	0.13%	0.116%
2	1.907	184	192	206	rVB	116488	153800	0.11%	0.097%
3	2.563	383	396	408	rBV	232301	382154	0.27%	0.241%
4	2.679	423	432	444	rVB	19617	32315	0.02%	0.020%
5	2.747	444	453	462	rBV2	5916	10473	0.01%	0.007%
6	2.946	507	515	528	rBV2	5649	11480	0.01%	0.007%
7	3.036	537	543	544	rBV4	995	900	0.00%	0.001%
8	3.177	576	587	611	rVB	41879	97230	0.07%	0.061%
9	3.705	748	751	756	rBV2	296	252	0.00%	0.000%
10	3.837	789	792	795	rBV3	522	435	0.00%	0.000%
11	3.972	828	834	839	rBV3	324	349	0.00%	0.000%
12	3.997	839	842	849	rVB2	246	285	0.00%	0.000%
13	4.097	869	873	881	rBV3	279	286	0.00%	0.000%
14	4.483	987	993	994	rBV2	550	395	0.00%	0.000%
15	4.528	994	1007	1020	rVV	13454	30566	0.02%	0.019%
16	4.615	1020	1034	1076	rVV3	94309	286563	0.20%	0.181%
17	4.917	1126	1128	1131	rBV3	361	255	0.00%	0.000%
18	5.055	1149	1171	1198	rBV	195917	433391	0.31%	0.273%
19	5.190	1210	1213	1215	rBV3	514	251	0.00%	0.000%
20	5.203	1215	1217	1219	rBV2	831	460	0.00%	0.000%
21	5.322	1251	1254	1256	rBV2	485	236	0.00%	0.000%
22	5.383	1261	1273	1287	rVB4	8638	17903	0.01%	0.011%
23	5.721	1357	1378	1381	rBV3	421448	949768	0.68%	0.598%
24	5.766	1383	1392	1422	rVB	3589793	7255958	5.16%	4.571%
25	6.242	1528	1540	1564	rBV	354484	673466	0.48%	0.424%
26	6.399	1587	1589	1592	rVB2	496	218	0.00%	0.000%
27	6.531	1625	1630	1632	rBV3	772	641	0.00%	0.000%
28	6.589	1646	1648	1652	rBV3	260	212	0.00%	0.000%
29	6.685	1664	1678	1705	rBV	247591	490388	0.35%	0.309%
30	6.791	1708	1711	1713	rBV3	535	400	0.00%	0.000%
31	6.930	1747	1754	1759	rBV2	331	409	0.00%	0.000%
32	7.145	1814	1821	1826	rBV3	327	439	0.00%	0.000%
33	7.193	1830	1836	1838	rVV4	626	538	0.00%	0.000%
34	7.206	1838	1840	1846	rVB4	649	521	0.00%	0.000%
35	7.406	1900	1902	1904	rVV2	413	212	0.00%	0.000%
36	7.422	1905	1907	1911	rVB2	427	233	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057851.D
 Acq On : 07 Feb 2024 19:45
 Operator : MD/SY
 Sample : P1081-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	7.560	1937	1950	1971	rBV	146054	267148	0.19%	0.168%
38	7.679	1982	1987	1997	rVB4	1809	2931	0.00%	0.002%
39	7.737	2003	2005	2011	rVB3	336	302	0.00%	0.000%
40	7.824	2029	2032	2035	rVB3	317	205	0.00%	0.000%
41	7.894	2041	2054	2070	rBV	522603	908650	0.65%	0.572%
42	8.174	2130	2141	2160	rBV	100717	174072	0.12%	0.110%
43	8.280	2171	2174	2179	rVB2	468	371	0.00%	0.000%
44	8.303	2179	2181	2184	rVV3	460	274	0.00%	0.000%
45	8.319	2184	2186	2190	rVB3	428	234	0.00%	0.000%
46	8.338	2190	2192	2196	rVB2	315	216	0.00%	0.000%
47	8.367	2196	2201	2205	rBV3	184	221	0.00%	0.000%
48	8.470	2221	2233	2245	rBV	6340	11608	0.01%	0.007%
49	8.627	2270	2282	2316	rBV	278679	553708	0.39%	0.349%
50	8.901	2362	2367	2372	rBV4	393	409	0.00%	0.000%
51	8.936	2375	2378	2381	rVB2	399	255	0.00%	0.000%
52	8.955	2381	2384	2387	rBV2	305	217	0.00%	0.000%
53	9.090	2420	2426	2428	rBV2	303	263	0.00%	0.000%
54	9.460	2515	2541	2594	rBV3	65627578	140603925	100.00%	88.570%
55	9.907	2678	2680	2683	rBV2	429	299	0.00%	0.000%
56	10.036	2718	2720	2722	rBV2	385	232	0.00%	0.000%
57	10.084	2733	2735	2737	rBV2	642	362	0.00%	0.000%
58	10.270	2790	2793	2795	rBV3	349	205	0.00%	0.000%
59	10.479	2856	2858	2863	rBV5	279	235	0.00%	0.000%
60	10.592	2889	2893	2897	rBV4	469	448	0.00%	0.000%
61	10.753	2930	2943	2967	rBV	321343	525250	0.37%	0.331%
62	10.894	2977	2987	2997	rVB4	7168	11832	0.01%	0.007%
63	10.987	3009	3016	3026	rVB4	3395	4979	0.00%	0.003%
64	11.058	3035	3038	3041	rVB2	335	224	0.00%	0.000%
65	11.097	3041	3050	3053	rBV3	838	1144	0.00%	0.001%
66	11.151	3064	3067	3071	rBV3	332	255	0.00%	0.000%
67	11.344	3122	3127	3130	rBV4	1094	1018	0.00%	0.001%
68	11.569	3191	3197	3199	rBV2	902	814	0.00%	0.001%
69	11.602	3204	3207	3209	rVB2	647	383	0.00%	0.000%
70	11.743	3239	3251	3261	rBV	158893	265234	0.19%	0.167%
71	11.830	3261	3278	3302	rVB2	785086	2074433	1.48%	1.307%
72	12.203	3377	3394	3415	rBV3	751546	1816072	1.29%	1.144%
73	12.576	3507	3510	3516	rBV3	320	230	0.00%	0.000%
74	12.682	3536	3543	3547	rBV5	1161	1383	0.00%	0.001%
75	12.769	3560	3570	3584	rVB	5636	9889	0.01%	0.006%
76	12.823	3584	3587	3589	rBV2	390	281	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
 Data File : VU057851.D
 Acq On : 07 Feb 2024 19:45
 Operator : MD/SY
 Sample : P1081-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	12.878	3601	3604	3607	rBV2	282	222	0.00%	0.000%
78	12.968	3629	3632	3633	rBV2	437	225	0.00%	0.000%
79	12.978	3633	3635	3642	rVB4	1226	1066	0.00%	0.001%
80	13.119	3677	3679	3686	rVB2	337	250	0.00%	0.000%
81	13.158	3686	3691	3693	rBV3	368	280	0.00%	0.000%
82	13.229	3708	3713	3717	rVB4	846	938	0.00%	0.001%
83	13.293	3732	3733	3737	rVB2	403	255	0.00%	0.000%
84	13.335	3744	3746	3749	rBV	508	317	0.00%	0.000%
85	13.460	3777	3785	3791	rVB5	1088	1236	0.00%	0.001%
86	13.521	3798	3804	3807	rBV2	360	519	0.00%	0.000%
87	13.618	3830	3834	3837	rBV2	441	302	0.00%	0.000%
88	13.708	3860	3862	3865	rBV2	388	264	0.00%	0.000%
89	13.778	3881	3884	3888	rVV2	333	359	0.00%	0.000%
90	13.839	3891	3903	3922	rVV	194479	325863	0.23%	0.205%
91	14.010	3953	3956	3960	rBV3	314	278	0.00%	0.000%
92	14.093	3973	3982	3995	rVV3	4899	7656	0.01%	0.005%
93	14.219	4017	4021	4027	rVB3	503	435	0.00%	0.000%
94	14.270	4035	4037	4038	rBV	393	210	0.00%	0.000%
95	14.328	4044	4055	4072	rVB	86754	142310	0.10%	0.090%
96	14.679	4161	4164	4174	rVB5	957	1373	0.00%	0.001%
97	14.855	4216	4219	4222	rBV	528	330	0.00%	0.000%
98	14.875	4223	4225	4229	rVV4	380	259	0.00%	0.000%
99	15.016	4265	4269	4279	rVB5	1045	1421	0.00%	0.001%
100	16.003	4569	4576	4583	rBV5	3432	4827	0.00%	0.003%




Sum of corrected areas: 158748972

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057851.D
Acq On : 07 Feb 2024 19:45
Operator : MD/SY
Sample : P1081-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

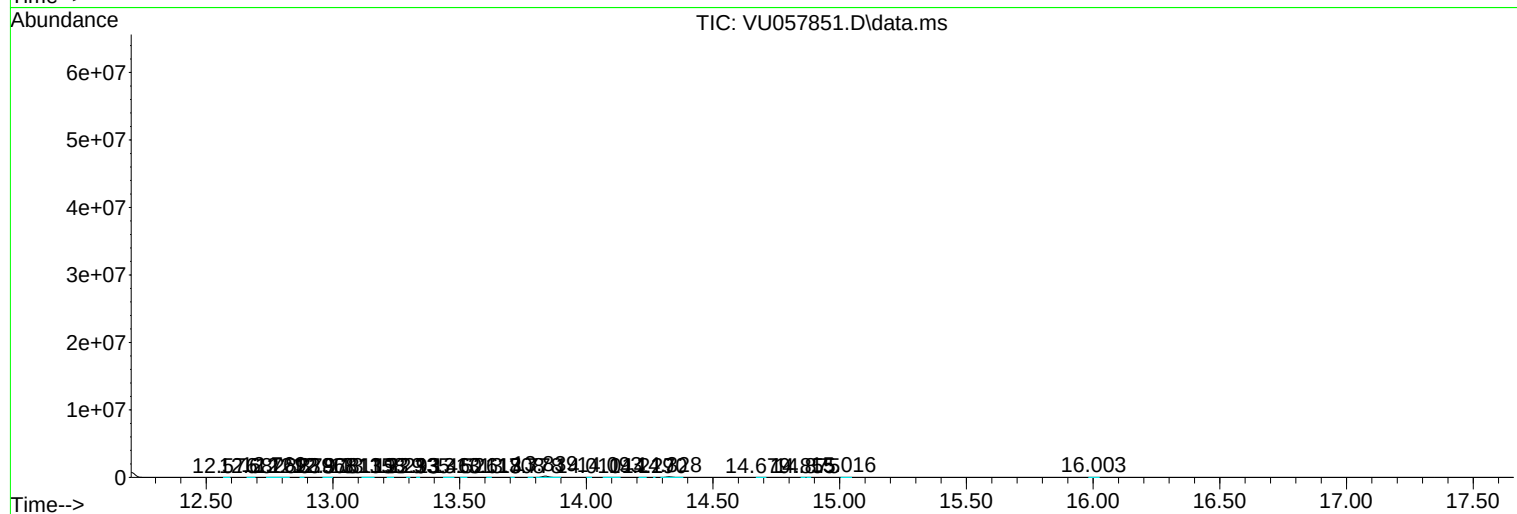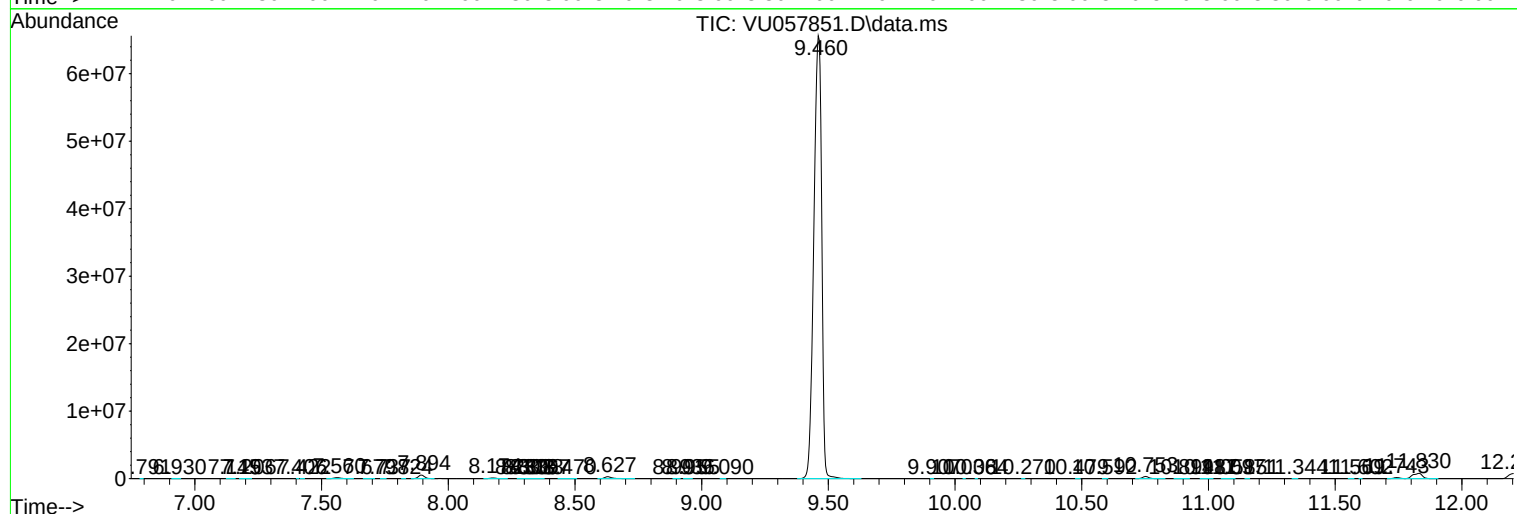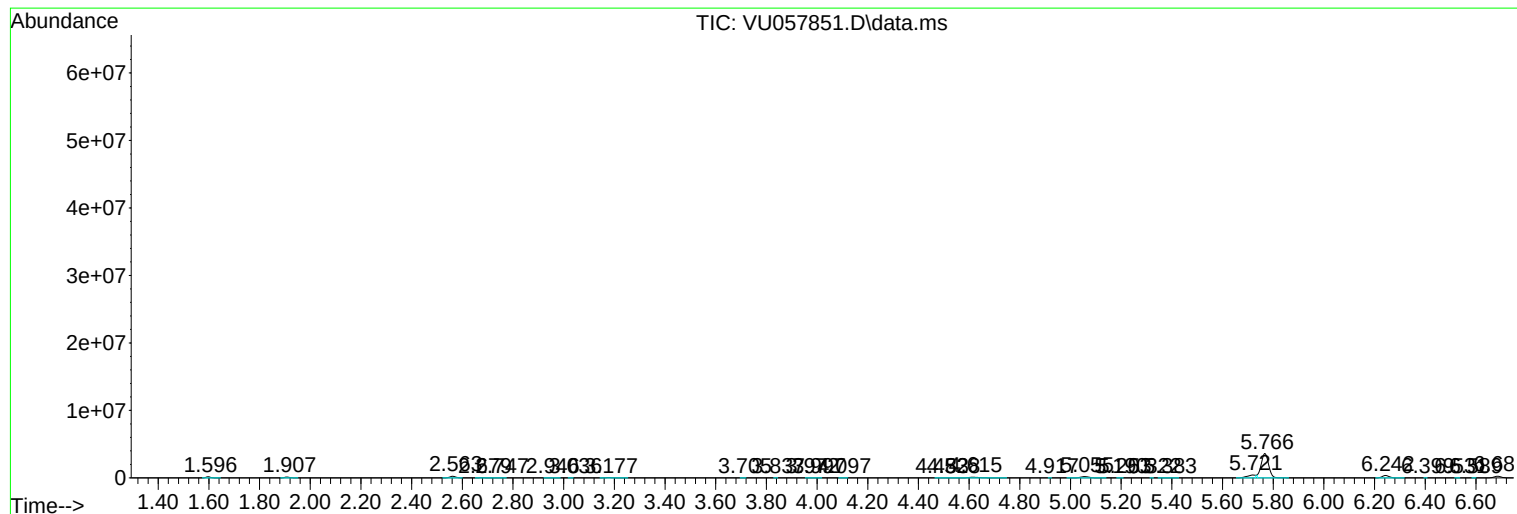

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057851.D
Acq On : 07 Feb 2024 19:45
Operator : MD/SY
Sample : P1081-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057851.D
Acq On : 07 Feb 2024 19:45
Operator : MD/SY
Sample : P1081-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------