


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020724\
Data File : VU057828.D
Acq On : 07 Feb 2024 08:29
Operator : MD/SY
Sample : BFB035
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB035

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Title : VOC Analysis
Last Update : Fri Feb 09 04:07:11 2024

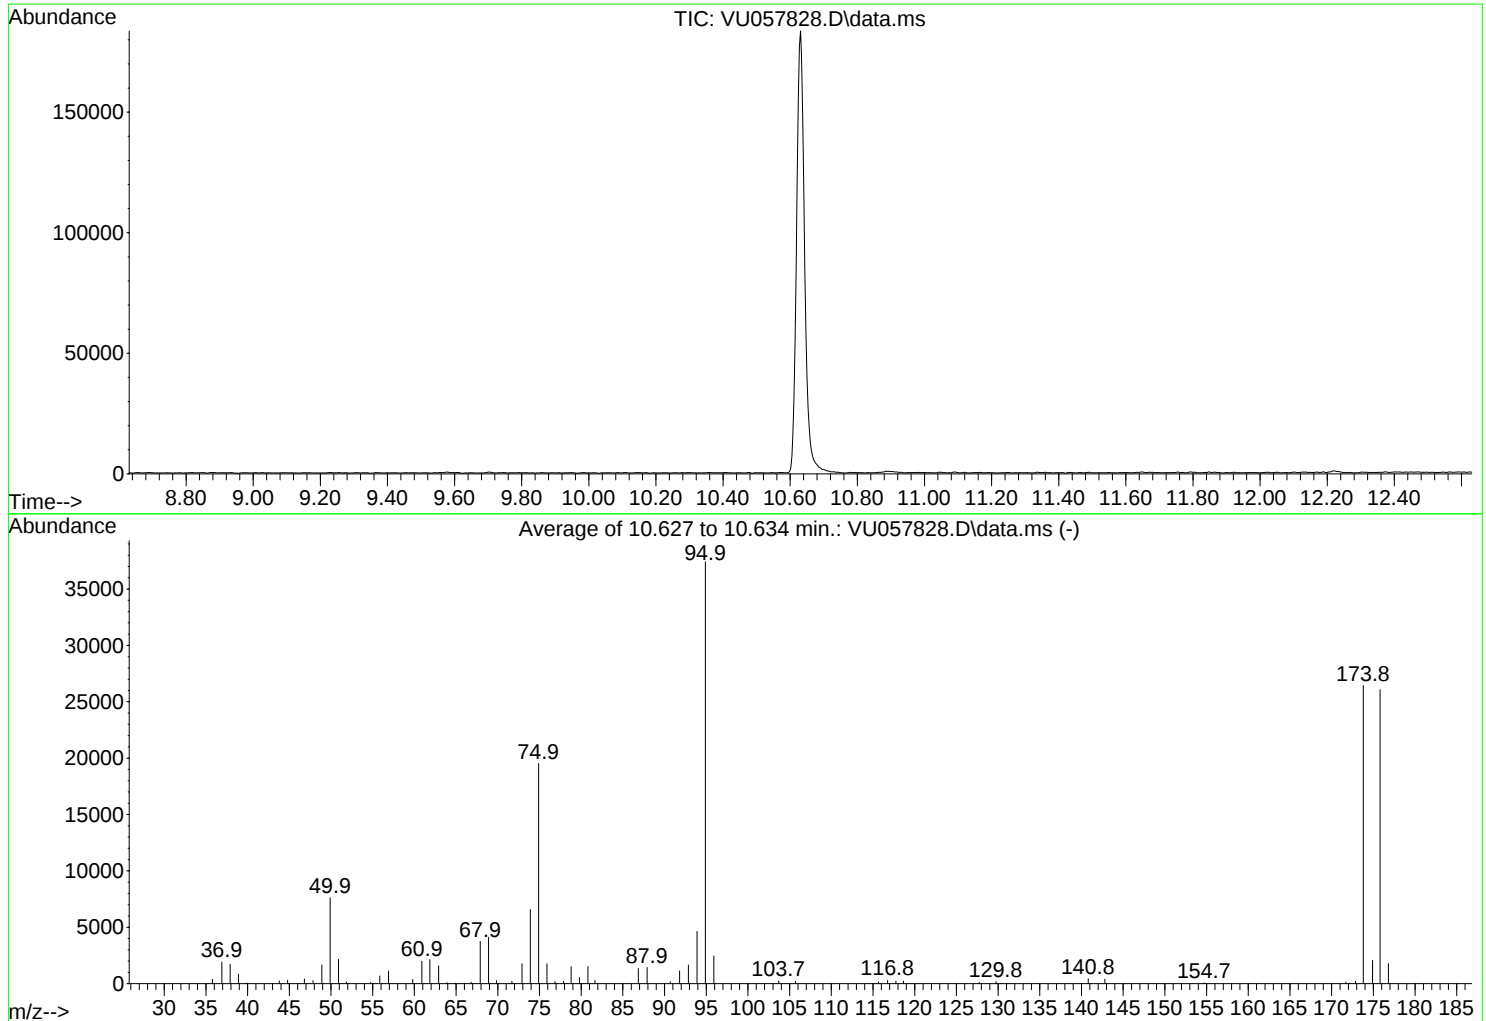

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	7610	PASS
75	95	30	80	52.2	19528	PASS
95	95	100	100	100.0	37413	PASS
96	95	5	9	6.6	2461	PASS
173	174	0.00	2	0.8	207	PASS
174	95	50	120	70.7	26453	PASS
175	174	5	9	7.8	2054	PASS
176	174	95	101	98.5	26069	PASS
177	176	5	9	6.8	1769	PASS

m/z	Abundance
39.80	150.0
43.80	317.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.80	401.0
36.90	1954.0
37.90	1716.0
38.90	915.0
39.80	199.0
43.80	530.0
44.80	314.0
46.80	433.0
47.90	241.0
48.90	1740.0
49.90	7639.0
50.90	2157.0
51.90	133.0
54.70	105.0
55.80	611.0
56.90	1095.0
59.80	317.0
60.90	1868.0
61.90	2166.0
62.90	1497.0
66.80	119.0
67.90	3790.0
68.90	4106.0
69.80	271.0
71.70	217.0
72.90	1767.0
73.90	6605.0
74.90	19424.0
75.90	1835.0
76.80	172.0
77.90	227.0
78.80	1461.0
79.80	466.0
80.80	1462.0
81.70	307.0
86.80	1373.0
87.90	1403.0
90.70	181.0
91.80	1137.0
92.80	1636.0
93.90	4842.0
94.90	37536.0
95.90	2493.0
103.70	237.0
105.70	212.0
115.60	126.0
116.80	320.0
117.70	219.0
118.70	239.0
127.70	101.0
129.80	189.0
140.80	369.0
142.80	398.0
171.70	147.0
172.10	128.0
172.80	226.0
173.80	26176.0
174.90	1930.0
175.80	25904.0
176.80	1743.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.80	403.0
36.90	1993.0
37.90	1772.0
38.90	900.0
39.80	223.0
43.80	571.0
44.80	336.0
46.80	425.0
47.80	279.0
48.90	1736.0
49.90	7855.0
50.90	2176.0
51.80	156.0
54.70	110.0
55.80	694.0
56.90	1136.0
59.80	380.0
60.90	2057.0
61.80	2225.0
62.90	1643.0
63.90	112.0
64.90	107.0
66.80	128.0
67.90	3816.0
68.90	4258.0
69.90	283.0
71.70	203.0
72.90	1803.0
73.90	6708.0
74.90	20088.0
75.90	1842.0
76.90	184.0
77.90	228.0
78.80	1525.0
79.80	535.0
80.80	1553.0
81.60	276.0
86.80	1370.0
87.90	1492.0
90.70	169.0
91.80	1150.0
92.80	1709.0
93.90	4734.0
94.90	38720.0
95.90	2538.0
103.70	240.0
105.70	200.0
115.70	162.0
116.70	292.0
117.70	242.0
118.70	235.0
127.70	106.0
129.70	200.0
140.80	425.0
142.80	402.0
154.70	110.0
171.70	169.0
172.80	207.0
173.80	27264.0
174.90	2130.0
175.80	26832.0
176.80	1803.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.80	332.0
36.90	1817.0
37.90	1686.0
38.90	715.0
39.80	205.0
43.80	566.0
44.80	275.0
46.80	370.0
47.80	279.0
48.90	1522.0
49.90	7336.0
50.90	2116.0
51.80	157.0
54.80	142.0
55.90	729.0
56.90	1090.0
59.80	402.0
60.90	2022.0
61.80	1990.0
62.90	1606.0
63.90	144.0
66.80	119.0
67.90	3635.0
68.90	3937.0
69.90	306.0
71.70	172.0
72.90	1720.0
73.90	6420.0
74.90	19072.0
75.90	1599.0
76.80	181.0
77.90	165.0
78.80	1537.0
79.80	573.0
80.80	1544.0
81.60	264.0
86.90	1306.0
87.90	1411.0
90.70	152.0
91.80	1136.0
92.90	1594.0
93.90	4316.0
94.90	35984.0
95.90	2351.0
103.70	238.0
105.70	174.0
115.70	163.0
116.70	247.0
117.80	227.0
118.60	220.0
127.80	113.0
129.70	179.0
140.80	483.0
142.80	386.0
154.70	114.0
171.70	124.0
172.90	187.0
173.80	25920.0
174.90	2101.0
175.80	25472.0
176.80	1760.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035