


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020819\
 Data File : VU029371.D
 Acq On : 08 Feb 2019 09:52
 Operator : JC/SP
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U020519DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Feb 08 10:52:46 2019

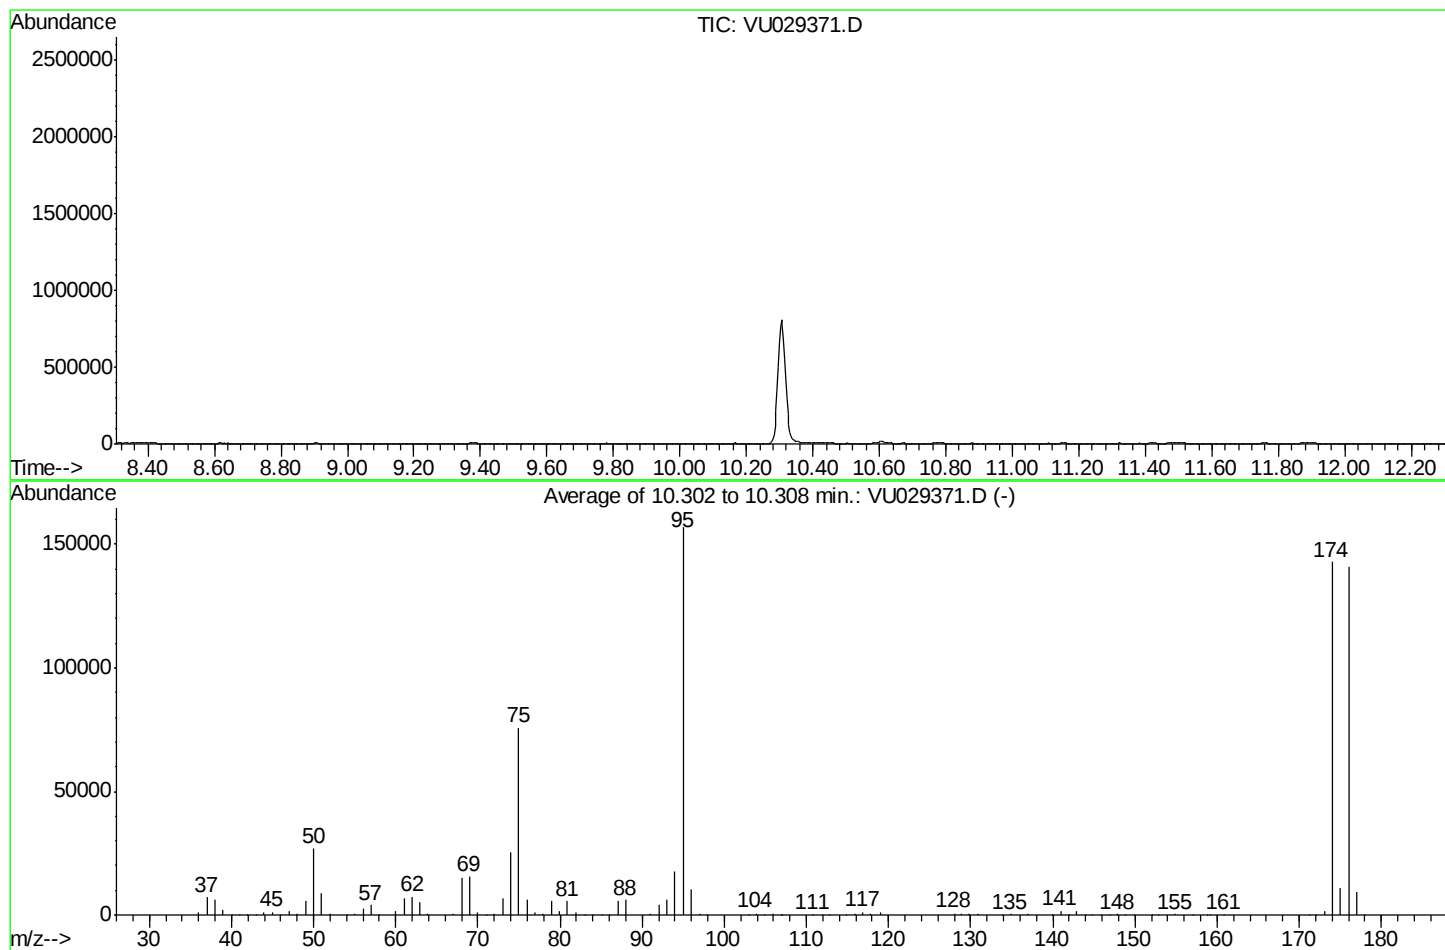

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	26864	PASS
75	95	30	60	48.3	75850	PASS
95	95	100	100	100.0	156885	PASS
96	95	5	9	6.6	10317	PASS
173	174	0.00	2	1.1	1607	PASS
174	95	50	100	91.0	142784	PASS
175	174	5	9	7.7	11031	PASS
176	174	95	101	98.6	140714	PASS
177	176	5	9	6.7	9370	PASS