

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020821\
 Data File : VU042290.D
 Acq On : 08 Feb 2021 12:23
 Operator : SY/MD
 Sample : M1310-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0A18

Quant Time: Feb 09 00:19:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR012021WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Feb 09 00:18:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	93372	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	88131	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	45410	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	25452	4.23	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 84.60%			
7) Chloroethane-d5	1.919	69	22909	4.72	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 94.40%			
11) 1,1-Dichloroethene-d2	2.575	63	46402	3.50	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 70.00%			
20) 2-Butanone-d5	4.645	46	99363	45.21	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 90.42%			
24) Chloroform-d	5.073	84	60122	4.78	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 95.60%			
26) 1,2-Dichloroethane-d4	5.713	65	38203	5.08	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 101.60%			
32) Benzene-d6	5.739	84	111734	4.85	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 97.00%			
36) 1,2-Dichloropropane-d6	6.700	67	37233	5.02	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 100.40%			
41) Toluene-d8	7.906	98	101597	4.67	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 93.40%			
43) trans-1,3-Dichloroprop...	8.189	79	15680	4.17	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 83.40%			
46) 2-Hexanone-d5	8.645	63	81610	49.82	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 99.64%			
57) 1,1,2,2-Tetrachloroeth...	10.764	84	30617	4.81	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 96.20%			
64) 1,2-Dichlorobenzene-d4	12.201	152	39617	4.86	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 97.20%			
Target Compounds					Qvalue	
13) Acetone	2.655	43	1206	0.82	ug/L	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020821\
Data File : VU042290.D
Acq On : 08 Feb 2021 12:23
Operator : SY/MD
Sample : M1310-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0A18

Quant Time: Feb 09 00:19:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Feb 09 00:18:31 2021
Response via : Initial Calibration

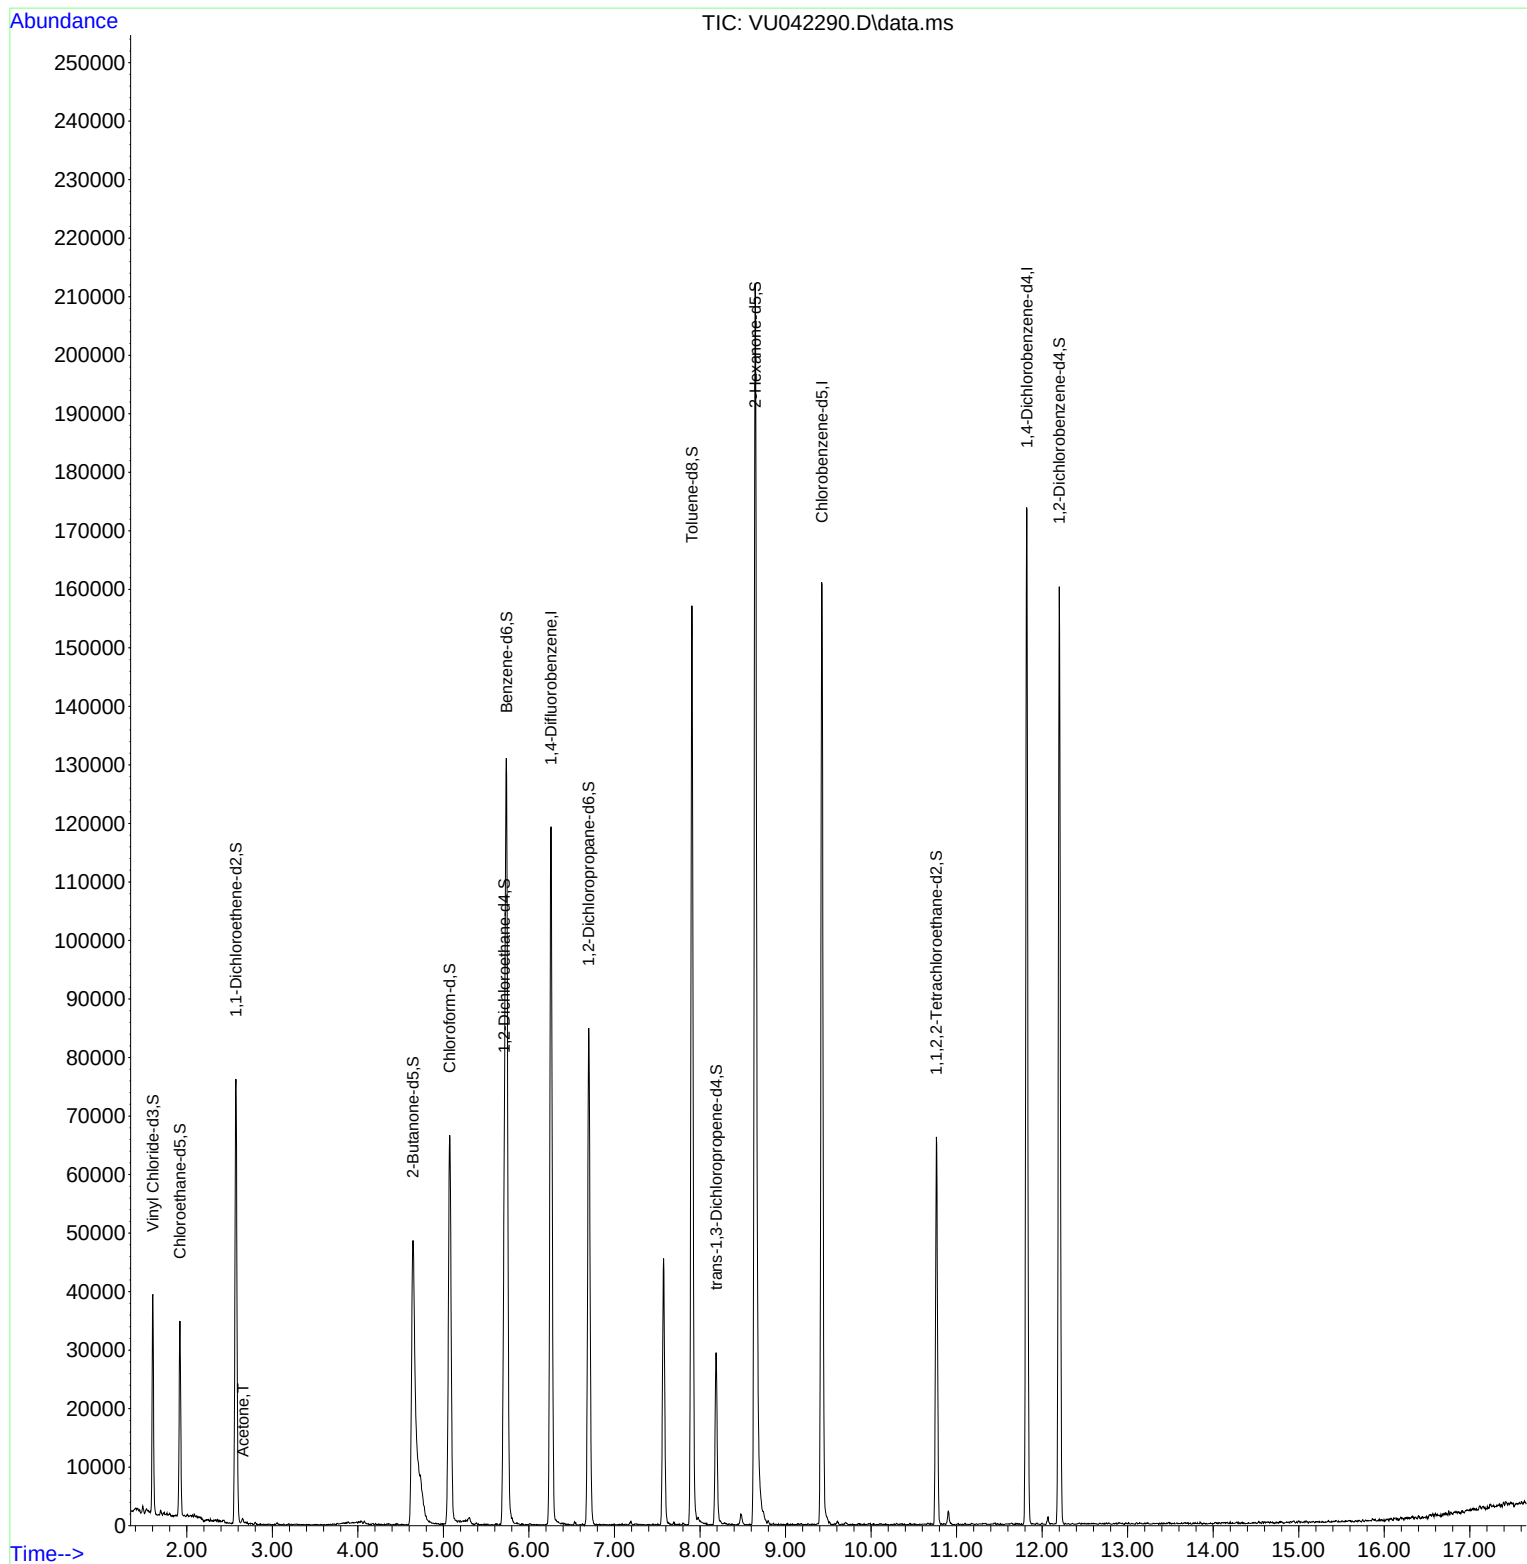

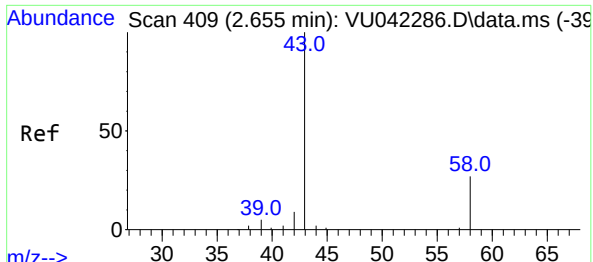

#13
 Acetone
 Concen: 0.82 ug/L
 RT: 2.655 min Scan# 409
 Delta R.T. -0.000 min
 Lab File: VU042290.D
 Acq: 08 Feb 2021 12:23

Instrument :
 MSVOA_U
 ClientSampleId :
 C0A18

Tgt Ion: 43 Resp: 1206
 Ion Ratio Lower Upper
 43 100
 58 11.2 0.0 55.8

