
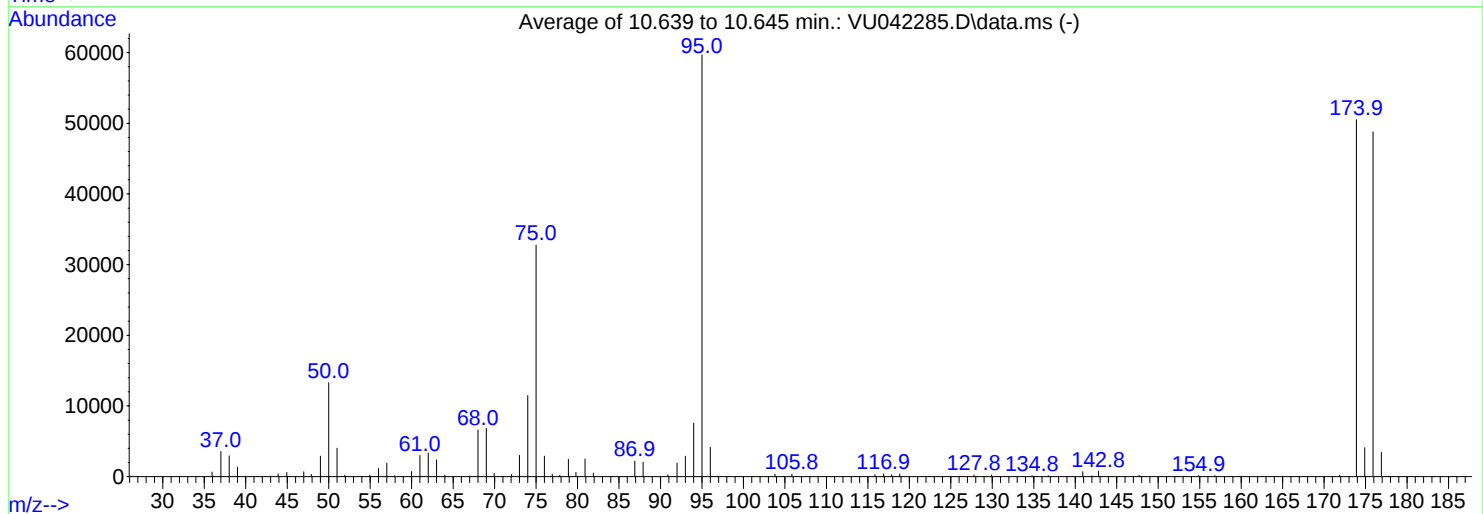


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020821\
Data File : VU042285.D
Acq On : 08 Feb 2021 09:34
Operator : SY/MD
Sample : BFB44
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB44

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR012021WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Feb 09 00:18:31 2021

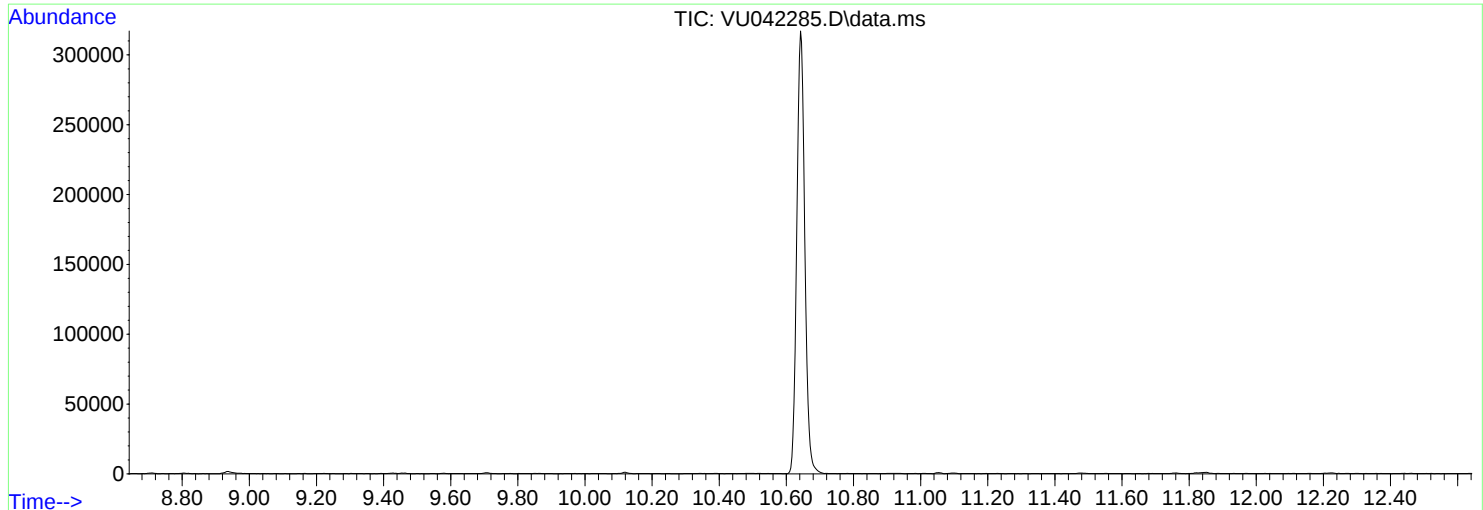

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	13298	PASS
75	95	30	80	54.9	32760	PASS
95	95	100	100	100.0	59688	PASS
96	95	5	9	7.0	4163	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.6	50509	PASS
175	174	5	9	8.1	4097	PASS
176	174	95	101	96.6	48797	PASS
177	176	5	9	7.0	3419	PASS

m/z	Abundance
35.90	614.0
37.00	3394.0
38.00	3012.0
39.00	1280.0
40.00	124.0
44.00	581.0
45.00	586.0
47.00	697.0
47.90	336.0
49.00	2816.0
50.00	13039.0
51.00	3934.0
51.90	217.0
55.00	196.0
56.00	1193.0
57.00	1899.0
57.90	104.0
60.00	696.0
61.00	2810.0
62.00	3375.0
63.00	2329.0
64.00	192.0
68.00	6356.0
69.00	6591.0
69.90	453.0
72.10	345.0
73.00	3007.0
74.00	11330.0
75.00	31960.0
76.00	2901.0
77.00	350.0
77.90	168.0
78.90	2400.0
79.80	595.0
80.90	2454.0
81.90	505.0
86.90	2087.0
87.90	1952.0
90.90	237.0
92.00	1848.0
93.00	2811.0
94.00	7369.0
95.00	58008.0
96.00	4246.0
96.90	109.0
103.80	309.0
105.90	370.0
115.80	291.0
116.90	390.0
117.90	287.0
118.80	368.0
127.80	280.0
129.90	278.0
134.80	118.0
136.70	140.0
140.90	642.0
142.00	108.0
142.80	745.0
147.70	201.0
154.90	161.0
156.80	153.0
171.80	161.0
173.90	48104.0
174.90	3934.0
175.90	46240.0
176.90	3353.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	673.0
37.00	3685.0
38.00	3014.0
39.00	1350.0
39.90	104.0
43.90	570.0
44.90	624.0
47.00	699.0
47.90	338.0
49.00	2988.0
50.00	13672.0
51.00	4170.0
52.00	205.0
55.00	207.0
56.00	1182.0
57.00	1935.0
58.00	107.0
60.00	762.0
61.00	3065.0
62.00	3511.0
63.00	2430.0
64.00	223.0
68.00	6802.0
69.00	7062.0
69.90	451.0
72.10	313.0
73.00	3062.0
74.00	11805.0
75.00	33728.0
76.00	2990.0
77.00	351.0
77.80	218.0
78.90	2523.0
79.80	642.0
80.90	2629.0
81.90	503.0
85.90	114.0
86.90	2286.0
87.90	2103.0
90.90	258.0
92.00	1972.0
93.00	3009.0
94.00	7774.0
95.00	61448.0
96.00	4285.0
96.90	115.0
103.80	353.0
105.80	352.0
115.80	307.0
116.90	389.0
117.90	279.0
118.80	381.0
127.80	269.0
129.90	272.0
134.80	133.0
136.70	130.0
140.90	739.0
142.00	123.0
142.80	768.0
147.70	204.0
154.90	170.0
156.80	162.0
171.90	179.0
173.90	51952.0
174.90	4201.0
175.90	50152.0
176.90	3510.0
177.80	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	678.0
37.00	3575.0
38.00	2822.0
39.00	1282.0
43.90	549.0
44.90	642.0
47.00	665.0
47.90	305.0
49.00	2883.0
50.00	13182.0
51.00	4023.0
52.00	187.0
54.90	230.0
56.00	1105.0
57.00	1879.0
58.00	102.0
60.00	728.0
61.00	3127.0
62.00	3202.0
63.00	2354.0
64.00	234.0
67.00	180.0
68.00	6661.0
69.00	6854.0
70.00	457.0
71.90	299.0
73.00	2954.0
74.00	11330.0
75.00	32592.0
76.00	2796.0
76.90	306.0
77.80	251.0
78.90	2425.0
79.80	609.0
80.90	2465.0
81.90	496.0
86.90	2229.0
87.90	2033.0
90.90	276.0
92.00	1937.0
93.00	2870.0
94.00	7611.0
95.00	59608.0
96.00	3958.0
103.80	350.0
104.80	109.0
105.80	334.0
115.90	275.0
116.90	378.0
117.80	248.0
118.90	343.0
127.80	215.0
129.90	215.0
134.80	126.0
136.80	123.0
140.90	740.0
142.00	122.0
142.80	723.0
147.70	184.0
154.90	167.0
156.90	127.0
171.90	198.0
173.90	51472.0
174.90	4157.0
175.90	50000.0
176.90	3393.0
177.80	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
43.90	178.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44