




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020823\
Data File : VU053008.D
Acq On : 08 Feb 2023 18:46
Operator : JC/MD
Sample : 01488-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Manual IntegrationsAPPROVED

Quant Time: Feb 09 01:49:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020823WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 09 01:09:47 2023
Response via : Initial Calibration

Reviewed By :
Supervised By :

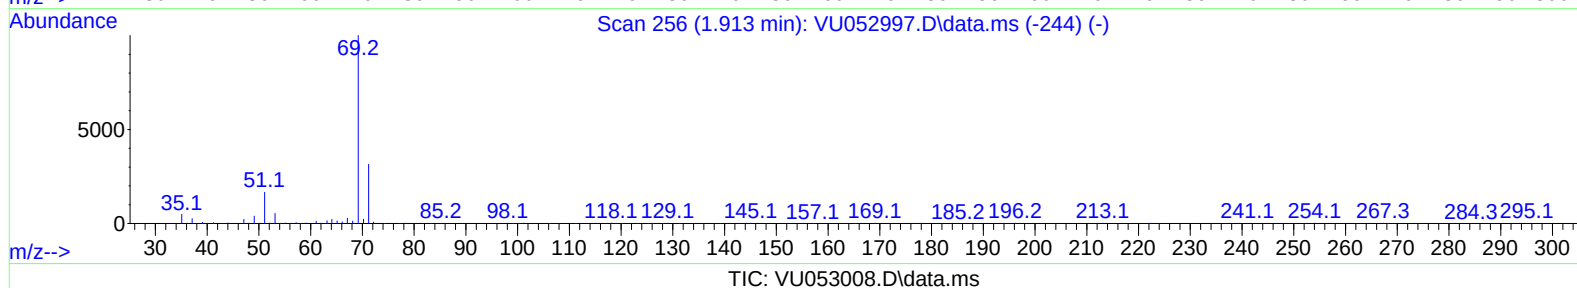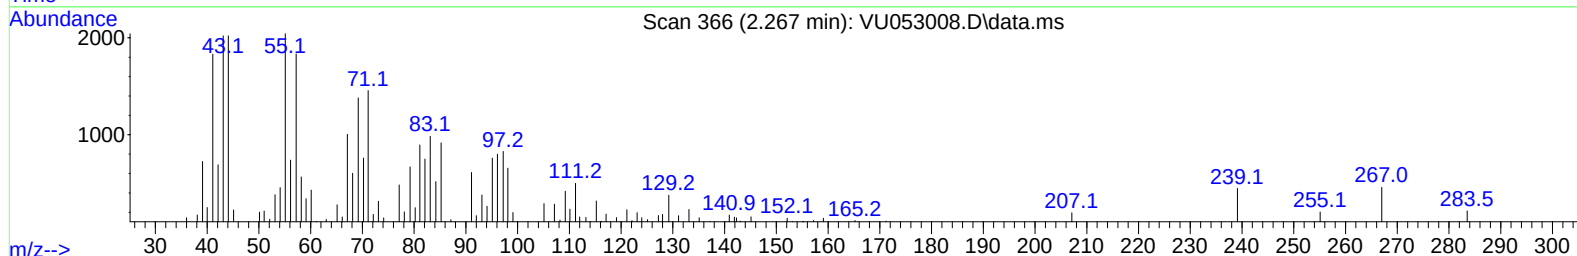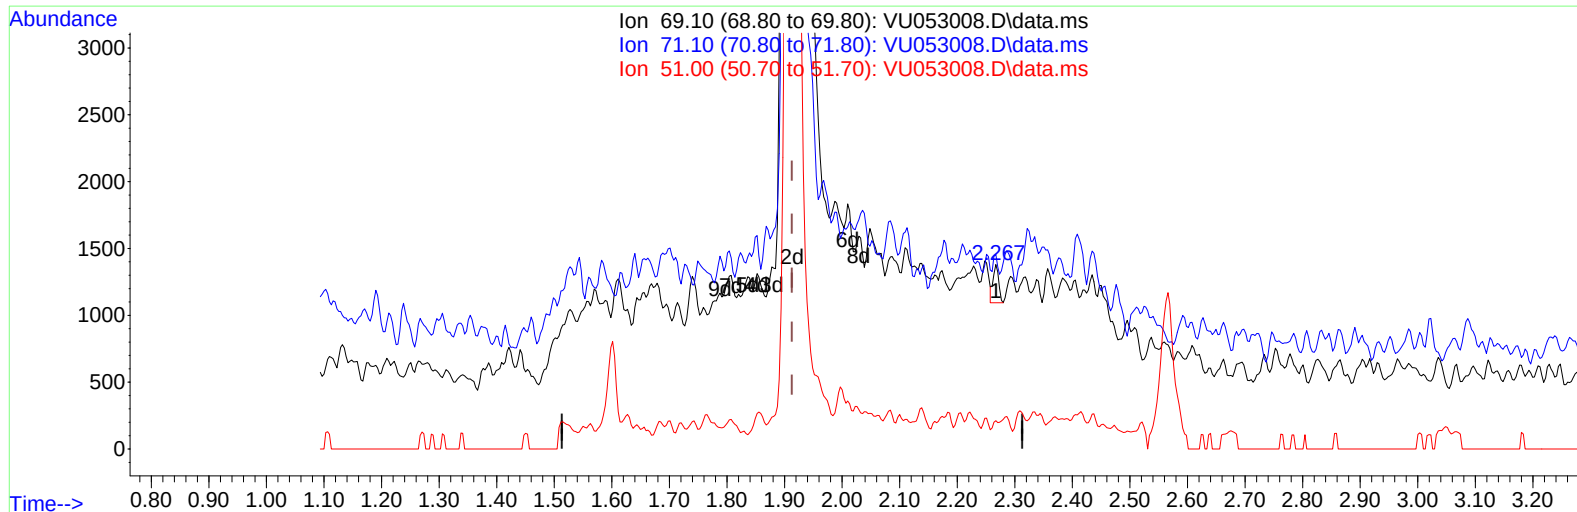

TIC: VU053008.D\data.ms

(7) Chloroethane-d5 (S)

2.267min (+ 0.354) 0.08 ug/L

response	190	
Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.90	40.53
51.00	24.20	23.16
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020823\
Data File : VU053008.D
Acq On : 08 Feb 2023 18:46
Operator : JC/MD
Sample : 01488-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Feb 09 01:49:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020823WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 09 01:09:47 2023
Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :
Supervised By :

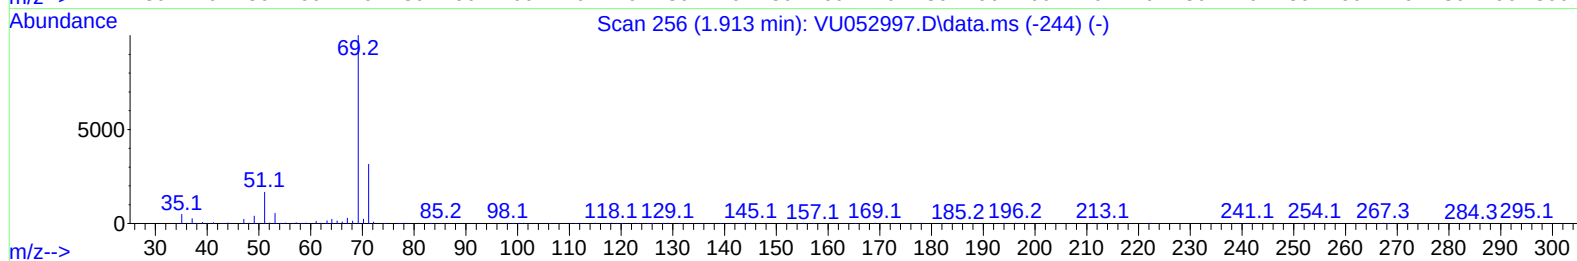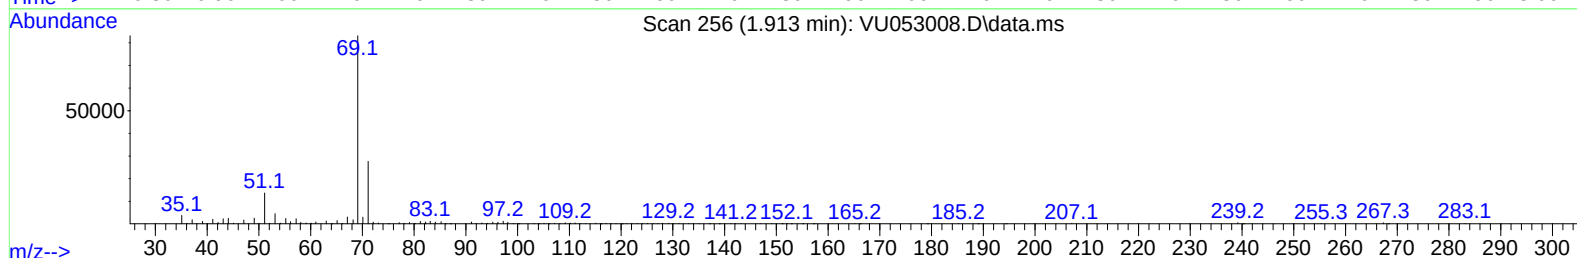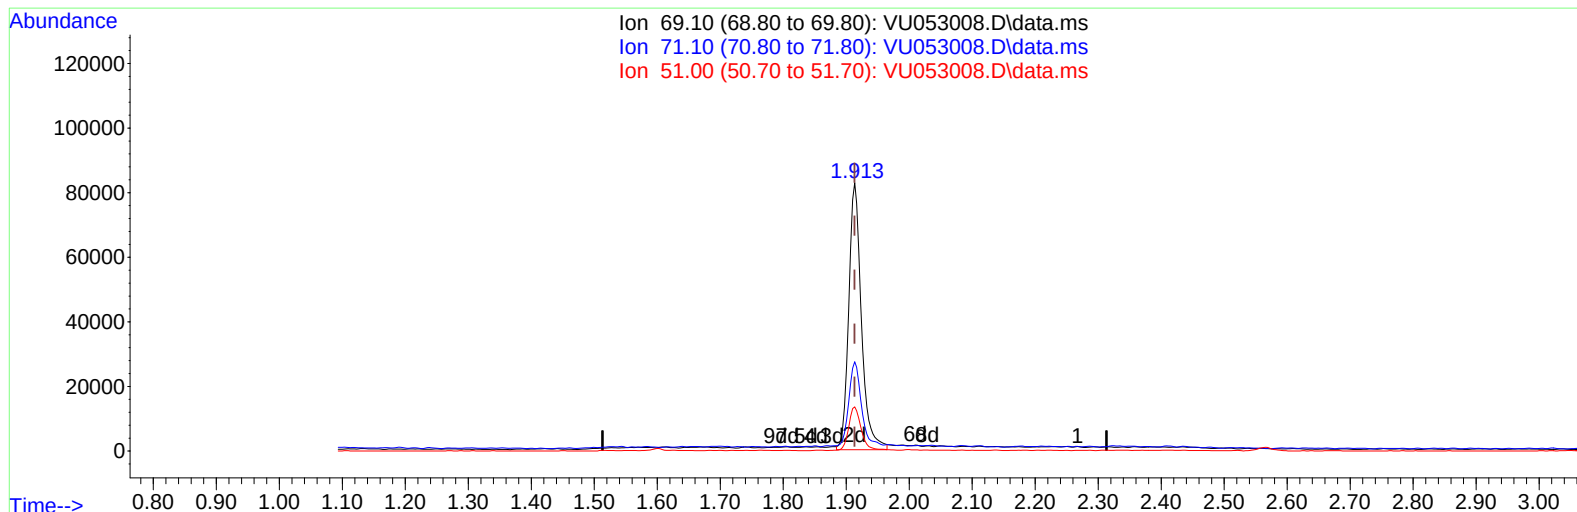

TIC: VU053008.D\data.ms

(7) Chloroethane-d5 (S)

1.913min (+ 0.000) 48.08 ug/L m

response 115749

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.90	0.07#
51.00	24.20	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020823\
 Data File : VU053008.D
 Acq On : 08 Feb 2023 18:46
 Operator : JC/MD
 Sample : 01488-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Manual IntegrationsAPPROVED

Quant Time: Feb 09 01:49:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 09 01:09:47 2023
 Response via : Initial Calibration

Reviewed By :
 Supervised By :

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.244	114	320302	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	299698	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	153670	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	131244	44.104	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.200%		
7) Chloroethane-d5	1.913	69	115749m	48.085	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.160%		
11) 1,1-Dichloroethene-d2	2.563	63	160100	35.109	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.220%		
21) 2-Butanone-d5	4.627	46	112258	97.263	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.260%		
24) Chloroform-d	5.058	84	225704	45.872	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.740%		
26) 1,2-Dichloroethane-d4	5.698	65	136826	46.526	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.060%		
32) Benzene-d6	5.723	84	472279	47.497	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.000%		
36) 1,2-Dichloropropane-d6	6.685	67	144612	47.138	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.280%		
41) Toluene-d8	7.894	98	450779	46.268	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.540%		
43) trans-1,3-Dichloroprop...	8.174	79	78644	46.774	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.540%		
47) 2-Hexanone-d5	8.627	63	94034	100.935	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	100.940%		
56) 1,1,2,2-Tetrachloroeth...	10.752	84	203334	47.877	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.760%		
66) 1,2-Dichlorobenzene-d4	12.186	152	165298	48.333	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.660%		
Target Compounds					Qvalue	
67) 1,2-Dichlorobenzene	12.209	146	4664	0.975	ug/L #	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020823\
Data File : VU053008.D
Acq On : 08 Feb 2023 18:46
Operator : JC/MD
Sample : 01488-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Manual IntegrationsAPPROVED

Quant Time: Feb 09 01:49:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020823WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 09 01:09:47 2023
Response via : Initial Calibration

Reviewed By :
Supervised By :

