

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057856.D
 Acq On : 08 Feb 2024 11:17
 Operator : MD/SY
 Sample : P1370-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M

Title : VOC Analysis

Signal : TIC: VU057856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	109	rVB	118177	143986	15.26%	2.024%
2	1.882	178	184	206	rVB	90498	131814	13.97%	1.853%
3	2.554	382	393	410	rBV	194723	318501	33.76%	4.476%
4	3.312	627	629	635	rBV	197	128	0.01%	0.002%
5	3.573	707	710	712	rBV2	198	123	0.01%	0.002%
6	3.682	740	744	746	rBV	216	154	0.02%	0.002%
7	4.120	877	880	881	rBV	183	103	0.01%	0.001%
8	4.361	949	955	958	rBV2	277	331	0.04%	0.005%
9	4.380	958	961	966	rVV2	200	197	0.02%	0.003%
10	4.415	970	972	978	rVB	110	106	0.01%	0.001%
11	4.611	1023	1033	1077	rBV	66572	180138	19.09%	2.532%
12	5.052	1156	1170	1197	rBV	162420	359228	38.08%	5.049%
13	5.258	1231	1234	1237	rBV2	106	63	0.01%	0.001%
14	5.306	1245	1249	1250	rBV	452	225	0.02%	0.003%
15	5.373	1268	1270	1271	rBV	78	35	0.00%	0.000%
16	5.418	1281	1284	1285	rBV	85	55	0.01%	0.001%
17	5.444	1290	1292	1295	rBV	85	38	0.00%	0.001%
18	5.518	1314	1315	1316	rBV	115	29	0.00%	0.000%
19	5.592	1330	1338	1341	rBV2	248	273	0.03%	0.004%
20	5.714	1356	1376	1409	rBV2	347146	943386	100.00%	13.258%
21	5.978	1456	1458	1459	rBV	426	164	0.02%	0.002%
22	6.023	1470	1472	1475	rVB2	190	118	0.01%	0.002%
23	6.049	1477	1480	1481	rBV2	186	94	0.01%	0.001%
24	6.174	1516	1519	1522	rBV	134	119	0.01%	0.002%
25	6.242	1527	1540	1566	rBV	290668	571118	60.54%	8.027%
26	6.457	1604	1607	1609	rBV2	212	151	0.02%	0.002%
27	6.525	1621	1628	1636	rVB5	1591	2689	0.29%	0.038%
28	6.560	1636	1639	1641	rVB	57	37	0.00%	0.001%
29	6.576	1641	1644	1645	rBV2	143	76	0.01%	0.001%
30	6.589	1645	1648	1650	rBV2	456	316	0.03%	0.004%
31	6.682	1662	1677	1696	rBV	211258	413631	43.85%	5.813%
32	6.836	1724	1725	1728	rVB	321	98	0.01%	0.001%
33	6.907	1744	1747	1752	rVB2	289	180	0.02%	0.003%
34	6.997	1772	1775	1778	rBV	120	90	0.01%	0.001%
35	7.126	1813	1815	1817	rBV2	96	53	0.01%	0.001%
36	7.335	1876	1880	1883	rVB2	208	179	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057856.D
 Acq On : 08 Feb 2024 11:17
 Operator : MD/SY
 Sample : P1370-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	7.393	1896	1898	1903	rVB	188	109	0.01%	0.002%
38	7.444	1911	1914	1918	rBV2	166	99	0.01%	0.001%
39	7.470	1918	1922	1928	rBV2	153	178	0.02%	0.003%
40	7.496	1928	1930	1932	rBV2	71	35	0.00%	0.000%
41	7.560	1938	1950	1971	rBV	111426	199161	21.11%	2.799%
42	7.750	2006	2009	2012	rBV2	207	120	0.01%	0.002%
43	7.769	2012	2015	2016	rBV	109	59	0.01%	0.001%
44	7.891	2040	2053	2072	rBV	415316	729291	77.31%	10.250%
45	8.174	2130	2141	2158	rBV	76670	129754	13.75%	1.824%
46	8.303	2178	2181	2182	rBV	246	119	0.01%	0.002%
47	8.351	2193	2196	2201	rVB2	243	198	0.02%	0.003%
48	8.386	2201	2207	2210	rBV2	163	150	0.02%	0.002%
49	8.457	2221	2229	2231	rBV3	497	519	0.06%	0.007%
50	8.515	2246	2247	2248	rBV3	140	40	0.00%	0.001%
51	8.569	2261	2264	2268	rBV2	182	165	0.02%	0.002%
52	8.631	2271	2283	2317	rBV	237098	467867	49.59%	6.575%
53	8.891	2362	2364	2368	rVB2	251	153	0.02%	0.002%
54	8.910	2368	2370	2371	rBV	154	84	0.01%	0.001%
55	8.942	2378	2380	2384	rVB	225	132	0.01%	0.002%
56	8.991	2390	2395	2398	rBV2	196	186	0.02%	0.003%
57	9.078	2414	2422	2424	rBV	210	299	0.03%	0.004%
58	9.235	2469	2471	2473	rBV	61	34	0.00%	0.000%
59	9.274	2481	2483	2485	rBV	147	63	0.01%	0.001%
60	9.322	2495	2498	2500	rBV	166	103	0.01%	0.001%
61	9.412	2514	2526	2557	rBV	411770	703137	74.53%	9.882%
62	9.688	2608	2612	2616	rBV3	557	687	0.07%	0.010%
63	9.798	2643	2646	2648	rBV	115	74	0.01%	0.001%
64	9.897	2673	2677	2679	rBV	363	241	0.03%	0.003%
65	10.039	2718	2721	2724	rBV2	168	146	0.02%	0.002%
66	10.251	2784	2787	2792	rVB	198	171	0.02%	0.002%
67	10.277	2792	2795	2800	rBV	138	133	0.01%	0.002%
68	10.325	2804	2810	2813	rBV2	214	204	0.02%	0.003%
69	10.373	2822	2825	2828	rBV2	145	127	0.01%	0.002%
70	10.512	2865	2868	2870	rBV	151	100	0.01%	0.001%
71	10.582	2887	2890	2893	rBV	218	154	0.02%	0.002%
72	10.614	2896	2900	2908	rVB	277	367	0.04%	0.005%
73	10.753	2930	2943	2961	rBV	285175	469980	49.82%	6.605%
74	10.891	2977	2986	2992	rBV3	884	1064	0.11%	0.015%
75	11.084	3043	3046	3049	rBV2	232	100	0.01%	0.001%
76	11.110	3049	3054	3055	rBV2	431	331	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057856.D
 Acq On : 08 Feb 2024 11:17
 Operator : MD/SY
 Sample : P1370-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M

Title : VOC Analysis

77	11.303	3111	3114	3115	rBB	36	35	0.00%	0.000%
78	11.630	3212	3216	3218	rBV	150	154	0.02%	0.002%
79	11.746	3246	3252	3259	rBV5	1466	2009	0.21%	0.028%
80	11.807	3259	3271	3293	rBV	404577	670231	71.05%	9.420%
81	12.190	3377	3390	3421	rBV	387143	659674	69.93%	9.271%
82	12.447	3467	3470	3475	rBV	239	189	0.02%	0.003%
83	12.476	3476	3479	3484	rVV3	226	173	0.02%	0.002%
84	12.640	3529	3530	3531	rBV3	150	50	0.01%	0.001%
85	12.855	3595	3597	3600	rBV2	220	92	0.01%	0.001%
86	13.129	3677	3682	3686	rBV2	273	346	0.04%	0.005%
87	13.852	3902	3907	3918	rVB6	2554	3632	0.38%	0.051%
88	14.103	3978	3985	3986	rBV2	1381	1254	0.13%	0.018%
89	14.341	4051	4059	4067	rVB4	2283	3534	0.37%	0.050%




Sum of corrected areas: 7115333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057856.D
Acq On : 08 Feb 2024 11:17
Operator : MD/SY
Sample : P1370-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

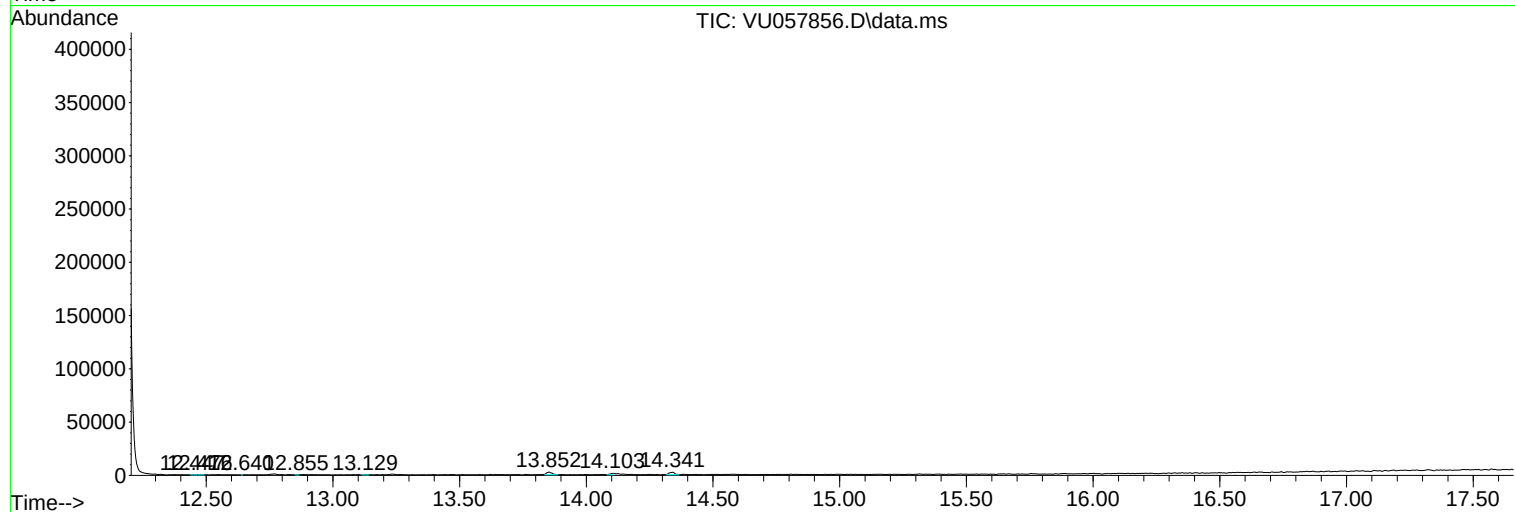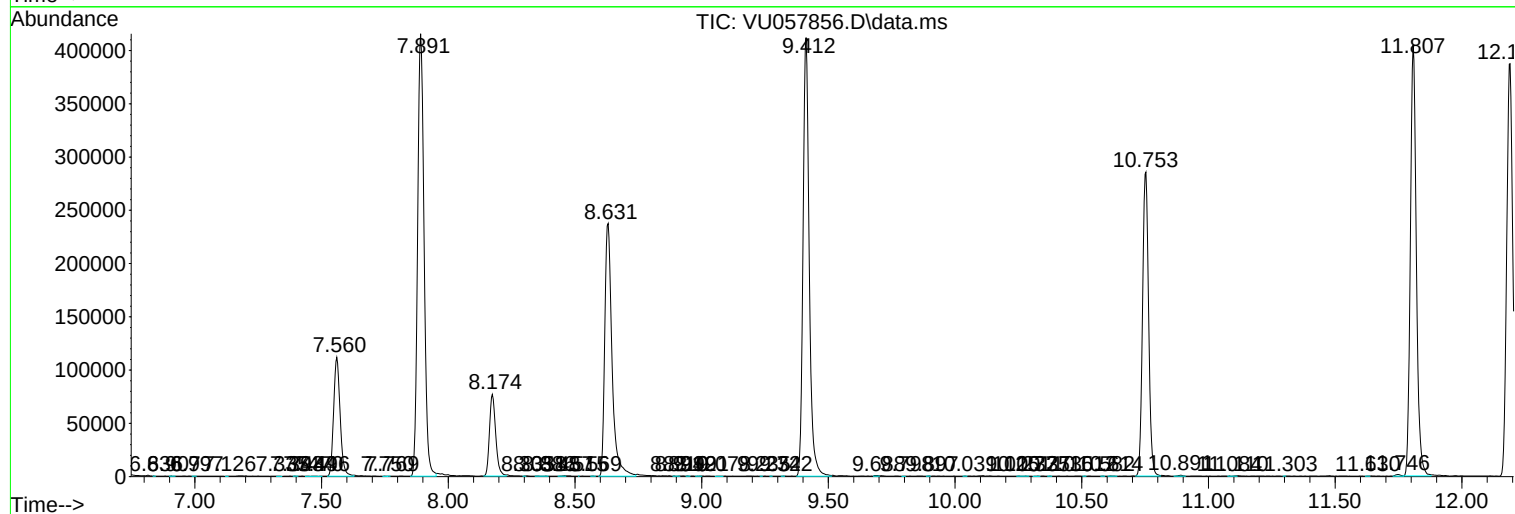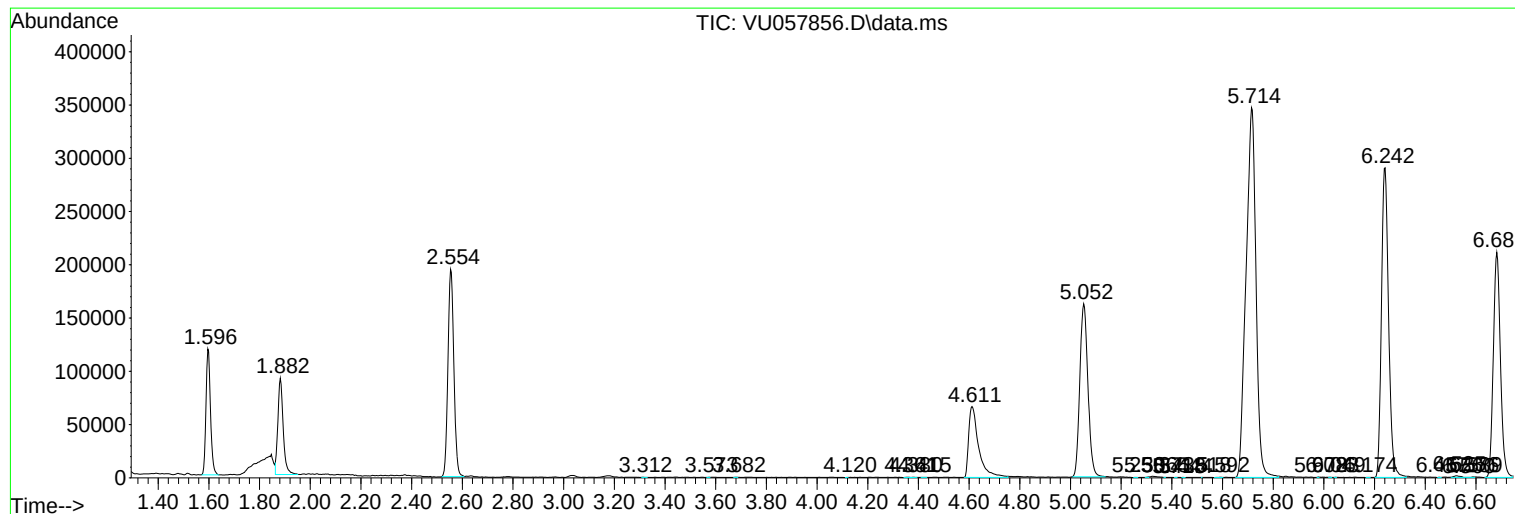

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057856.D
Acq On : 08 Feb 2024 11:17
Operator : MD/SY
Sample : P1370-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057856.D
Acq On : 08 Feb 2024 11:17
Operator : MD/SY
Sample : P1370-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc