

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057858.D
 Acq On : 08 Feb 2024 12:07
 Operator : MD/SY
 Sample : P1081-07DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

Signal : TIC: VU057858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rVB	123987	145073	9.27%	1.689%
2	1.888	178	186	203	rVB	93028	131332	8.39%	1.529%
3	2.557	381	394	410	rBV	195269	319248	20.40%	3.716%
4	2.663	424	427	430	rVB2	368	244	0.02%	0.003%
5	2.888	494	497	501	rBV	161	146	0.01%	0.002%
6	2.981	523	526	529	rBV	325	203	0.01%	0.002%
7	3.033	534	542	554	rVV4	2195	3886	0.25%	0.045%
8	3.168	574	584	586	rBV3	1889	2272	0.15%	0.026%
9	3.425	659	664	666	rBV2	201	175	0.01%	0.002%
10	3.641	728	731	736	rBV2	178	146	0.01%	0.002%
11	3.718	748	755	761	rBV2	209	324	0.02%	0.004%
12	4.213	907	909	913	rVV2	259	226	0.01%	0.003%
13	4.239	914	917	922	rVV2	258	221	0.01%	0.003%
14	4.280	926	930	937	rBV2	294	370	0.02%	0.004%
15	4.354	947	953	961	rVV2	183	301	0.02%	0.004%
16	4.608	1023	1032	1075	rBV	69568	186462	11.92%	2.171%
17	4.907	1123	1125	1128	rVB2	336	191	0.01%	0.002%
18	5.052	1154	1170	1203	rBV	168167	376464	24.06%	4.383%
19	5.242	1224	1229	1231	rBV	331	355	0.02%	0.004%
20	5.322	1245	1254	1264	rBV3	953	1902	0.12%	0.022%
21	5.419	1281	1284	1287	rBV	319	182	0.01%	0.002%
22	5.518	1307	1315	1329	rVB4	449	989	0.06%	0.012%
23	5.579	1329	1334	1338	rBV2	216	226	0.01%	0.003%
24	5.618	1342	1346	1350	rVB2	135	137	0.01%	0.002%
25	5.714	1356	1376	1386	rBV2	348934	968605	61.90%	11.276%
26	6.004	1463	1466	1467	rBV2	362	182	0.01%	0.002%
27	6.036	1473	1476	1478	rBV	247	165	0.01%	0.002%
28	6.100	1493	1496	1499	rVB2	229	152	0.01%	0.002%
29	6.184	1519	1522	1526	rBV	230	141	0.01%	0.002%
30	6.242	1527	1540	1560	rBV	294379	564048	36.05%	6.566%
31	6.393	1584	1587	1592	rBV2	420	316	0.02%	0.004%
32	6.531	1619	1630	1634	rBV6	570	943	0.06%	0.011%
33	6.554	1634	1637	1642	rVB2	164	149	0.01%	0.002%
34	6.611	1652	1655	1657	rVB2	223	136	0.01%	0.002%
35	6.682	1663	1677	1707	rBV	216801	425652	27.20%	4.955%
36	6.853	1726	1730	1733	rBV2	159	143	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057858.D
 Acq On : 08 Feb 2024 12:07
 Operator : MD/SY
 Sample : P1081-07DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	6.949	1757	1760	1766	rVB	272	216	0.01%	0.003%
38	7.010	1774	1779	1782	rVB2	193	204	0.01%	0.002%
39	7.187	1823	1834	1839	rBV3	440	807	0.05%	0.009%
40	7.364	1887	1889	1893	rVB2	271	187	0.01%	0.002%
41	7.409	1899	1903	1909	rBV2	170	183	0.01%	0.002%
42	7.460	1914	1919	1921	rBV2	164	147	0.01%	0.002%
43	7.560	1935	1950	1970	rBV	121230	218606	13.97%	2.545%
44	7.737	2001	2005	2009	rVB2	170	133	0.01%	0.002%
45	7.891	2040	2053	2073	rBV	430399	747355	47.76%	8.700%
46	8.174	2129	2141	2170	rBV	81302	143946	9.20%	1.676%
47	8.316	2183	2185	2187	rBV2	210	141	0.01%	0.002%
48	8.332	2187	2190	2197	rVB2	421	417	0.03%	0.005%
49	8.470	2220	2233	2242	rBV2	672	1516	0.10%	0.018%
50	8.627	2271	2282	2307	rBV	254281	475411	30.38%	5.534%
51	8.865	2351	2356	2359	rBV2	246	291	0.02%	0.003%
52	9.042	2408	2411	2419	rVB2	264	338	0.02%	0.004%
53	9.078	2419	2422	2426	rBV	239	198	0.01%	0.002%
54	9.119	2431	2435	2437	rBV2	160	134	0.01%	0.002%
55	9.148	2441	2444	2448	rBV	154	150	0.01%	0.002%
56	9.242	2464	2473	2476	rBV2	171	301	0.02%	0.004%
57	9.319	2494	2497	2501	rVB	205	149	0.01%	0.002%
58	9.412	2513	2526	2530	rBV	427663	680158	43.47%	7.918%
59	9.695	2603	2614	2624	rBV4	906	1403	0.09%	0.016%
60	9.914	2679	2682	2687	rVB2	215	197	0.01%	0.002%
61	9.955	2687	2695	2698	rBV2	197	244	0.02%	0.003%
62	10.107	2738	2742	2748	rVB2	428	514	0.03%	0.006%
63	10.139	2748	2752	2753	rBV	195	153	0.01%	0.002%
64	10.200	2764	2771	2774	rBV2	190	255	0.02%	0.003%
65	10.479	2852	2858	2860	rBV2	281	300	0.02%	0.003%
66	10.570	2882	2886	2888	rBV	218	153	0.01%	0.002%
67	10.621	2898	2902	2907	rBV2	204	252	0.02%	0.003%
68	10.750	2930	2942	2971	rVB	297215	479119	30.62%	5.578%
69	10.885	2978	2984	2988	rBV4	841	914	0.06%	0.011%
70	11.020	3022	3026	3030	rVV2	280	236	0.02%	0.003%
71	11.090	3044	3048	3052	rBV3	306	291	0.02%	0.003%
72	11.476	3164	3168	3172	rBV2	357	327	0.02%	0.004%
73	11.550	3189	3191	3199	rVB2	360	485	0.03%	0.006%
74	11.595	3199	3205	3207	rBV2	253	325	0.02%	0.004%
75	11.740	3240	3250	3260	rBV	135097	211591	13.52%	2.463%
76	11.811	3260	3272	3273	rBV	487831	592258	37.85%	6.895%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057858.D
 Acq On : 08 Feb 2024 12:07
 Operator : MD/SY
 Sample : P1081-07DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	12.007	3329	3333	3335	rBV	207	173	0.01%	0.002%
78	12.065	3345	3351	3353	rBV2	181	209	0.01%	0.002%
79	12.106	3357	3364	3370	rBV2	297	506	0.03%	0.006%
80	12.203	3377	3394	3413	rBV2	654039	1564695	100.00%	18.215%
81	12.332	3431	3434	3438	rVB3	354	231	0.01%	0.003%
82	12.589	3509	3514	3518	rBV	331	288	0.02%	0.003%
83	12.766	3562	3569	3577	rBV3	957	1510	0.10%	0.018%
84	12.926	3616	3619	3621	rBV2	231	142	0.01%	0.002%
85	13.187	3697	3700	3706	rVB2	202	192	0.01%	0.002%
86	13.229	3710	3713	3715	rBV2	463	317	0.02%	0.004%
87	13.553	3812	3814	3817	rVB	357	173	0.01%	0.002%
88	13.836	3891	3902	3925	rBV	132315	215145	13.75%	2.505%
89	14.013	3954	3957	3960	rBV3	184	152	0.01%	0.002%
90	14.200	4012	4015	4020	rBV2	226	257	0.02%	0.003%
91	14.325	4044	4054	4076	rVB	67215	110917	7.09%	1.291%
92	14.412	4076	4081	4082	rBV2	284	243	0.02%	0.003%
93	14.447	4088	4092	4097	rBV3	308	381	0.02%	0.004%
94	14.505	4105	4110	4113	rBV2	334	336	0.02%	0.004%
95	14.608	4138	4142	4146	rVB2	308	320	0.02%	0.004%
96	14.637	4146	4151	4153	rBV	293	294	0.02%	0.003%
97	14.675	4160	4163	4169	rBV2	446	405	0.03%	0.005%
98	15.437	4398	4400	4403	rVB3	407	219	0.01%	0.003%
99	16.003	4572	4576	4578	rBV4	645	576	0.04%	0.007%
100	16.087	4598	4602	4605	rBV5	829	676	0.04%	0.008%




Sum of corrected areas: 8590069

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057858.D
Acq On : 08 Feb 2024 12:07
Operator : MD/SY
Sample : P1081-07DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

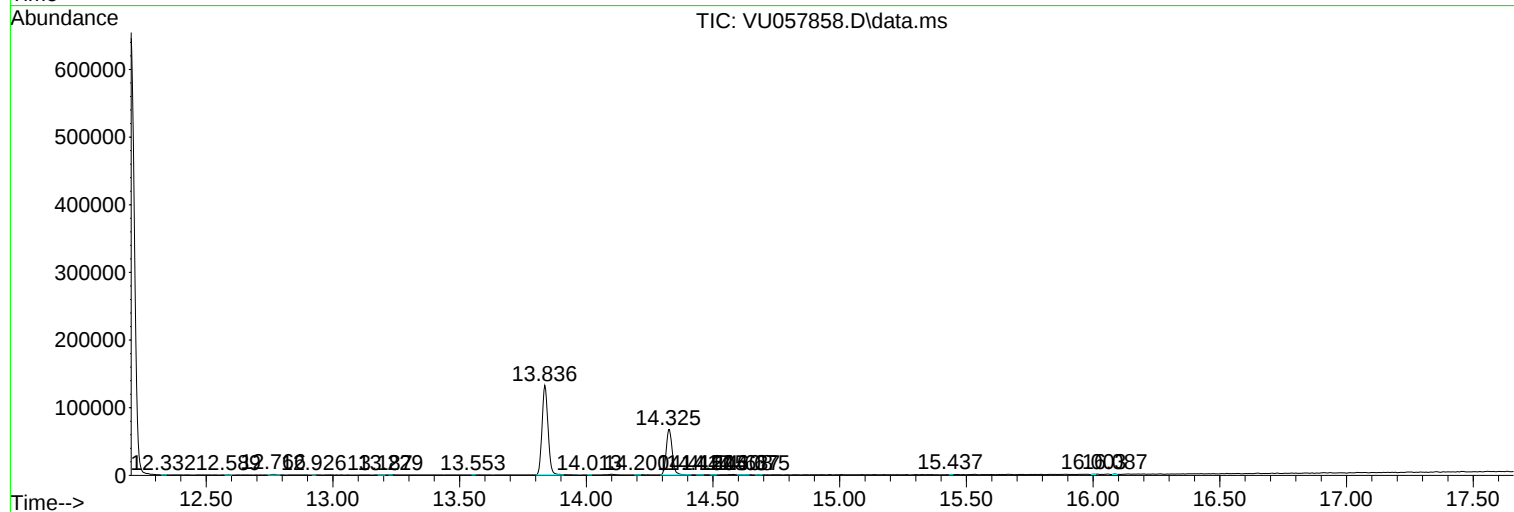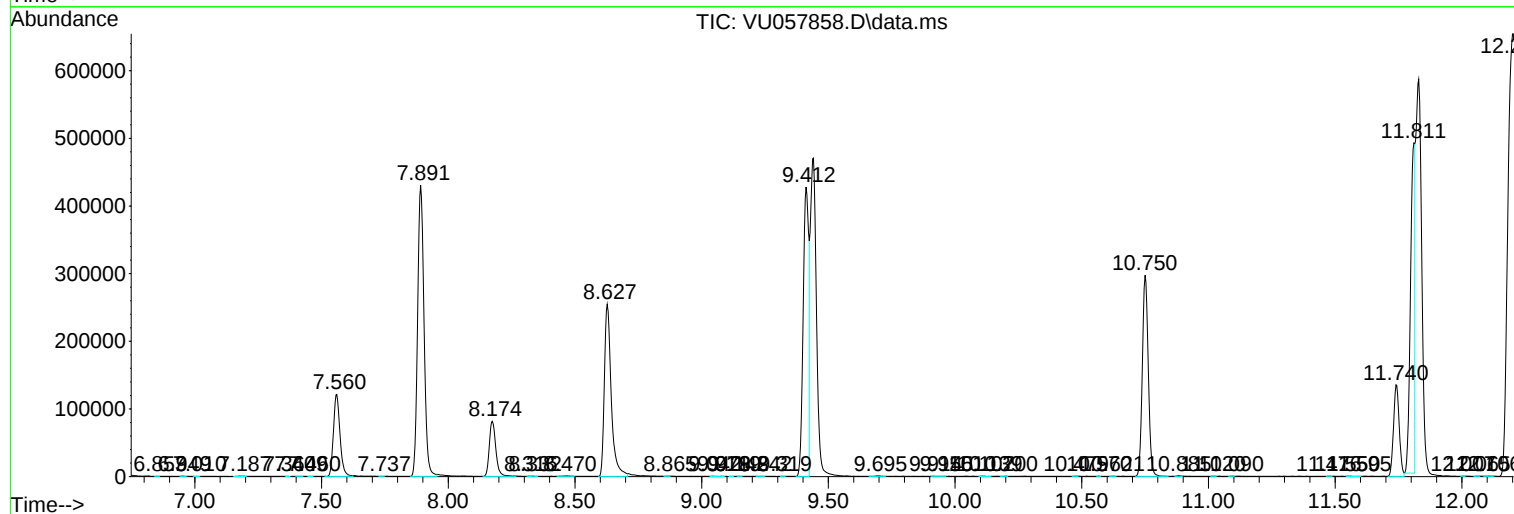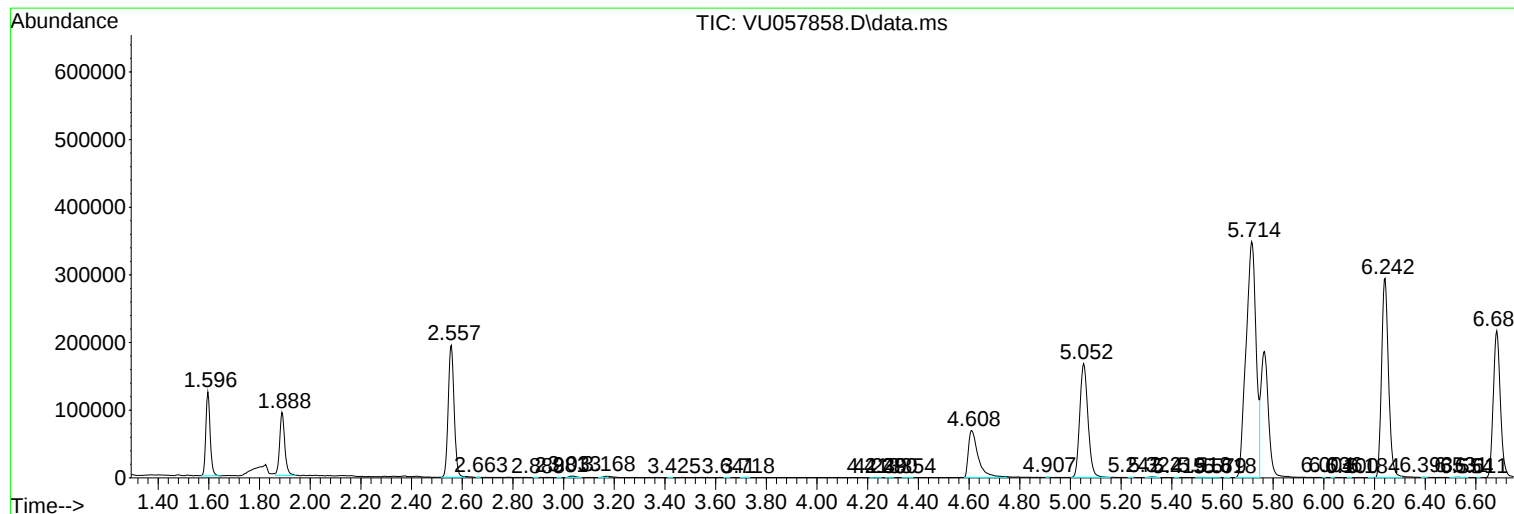

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057858.D
Acq On : 08 Feb 2024 12:07
Operator : MD/SY
Sample : P1081-07DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057858.D
Acq On : 08 Feb 2024 12:07
Operator : MD/SY
Sample : P1081-07DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------