

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057859.D
 Acq On : 08 Feb 2024 12:31
 Operator : MD/SY
 Sample : P1352-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

Signal : TIC: VU057859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rBV	118133	143402	15.12%	1.959%
2	1.801	137	159	160	rBV6	12363	33897	3.57%	0.463%
3	1.882	176	184	199	rVB	89595	130479	13.76%	1.783%
4	2.554	381	393	414	rBV	196684	321422	33.89%	4.392%
5	2.779	458	463	464	rBV2	384	336	0.04%	0.005%
6	2.840	479	482	485	rVB2	323	184	0.02%	0.003%
7	2.949	512	516	519	rBV3	295	272	0.03%	0.004%
8	3.033	535	542	551	rVB3	2633	4579	0.48%	0.063%
9	3.171	578	585	594	rVB4	913	1505	0.16%	0.021%
10	3.300	618	625	629	rVB	263	338	0.04%	0.005%
11	3.322	629	632	634	rBV	208	154	0.02%	0.002%
12	3.338	634	637	641	rVB	232	178	0.02%	0.002%
13	3.637	726	730	737	rBV2	265	373	0.04%	0.005%
14	3.872	800	803	813	rVB2	278	376	0.04%	0.005%
15	3.917	814	817	821	rBV2	306	209	0.02%	0.003%
16	4.030	847	852	857	rVB2	203	238	0.03%	0.003%
17	4.058	857	861	863	rBV	226	170	0.02%	0.002%
18	4.123	878	881	884	rVB	287	179	0.02%	0.002%
19	4.165	891	894	899	rVB2	250	209	0.02%	0.003%
20	4.219	906	911	915	rBV2	191	236	0.02%	0.003%
21	4.351	950	952	956	rVV2	225	166	0.02%	0.002%
22	4.612	1023	1033	1064	rBV2	67564	176792	18.64%	2.415%
23	4.962	1138	1142	1147	rVB	338	377	0.04%	0.005%
24	5.052	1153	1170	1195	rVV	166416	367852	38.79%	5.026%
25	5.193	1212	1214	1217	rBV2	326	183	0.02%	0.003%
26	5.287	1238	1243	1246	rBV2	170	168	0.02%	0.002%
27	5.322	1246	1254	1256	rBV3	736	986	0.10%	0.013%
28	5.528	1313	1318	1321	rBV	175	167	0.02%	0.002%
29	5.714	1356	1376	1409	rBV2	347579	948353	100.00%	12.957%
30	5.997	1462	1464	1470	rBV3	170	168	0.02%	0.002%
31	6.197	1517	1526	1527	rBV2	241	326	0.03%	0.004%
32	6.238	1527	1539	1570	rVV	305349	585608	61.75%	8.001%
33	6.521	1623	1627	1628	rBV2	1027	811	0.09%	0.011%
34	6.682	1664	1677	1702	rBV	214057	420278	44.32%	5.742%
35	6.801	1710	1714	1719	rVB5	546	565	0.06%	0.008%
36	6.904	1737	1746	1751	rVB2	189	285	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057859.D
 Acq On : 08 Feb 2024 12:31
 Operator : MD/SY
 Sample : P1352-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	6.991	1768	1773	1775	rBV	271	212	0.02%	0.003%
38	7.184	1824	1833	1837	rBV3	467	636	0.07%	0.009%
39	7.470	1917	1922	1926	rVB2	232	219	0.02%	0.003%
40	7.560	1937	1950	1968	rBV	120115	212379	22.39%	2.902%
41	7.669	1983	1984	1987	rVB2	339	159	0.02%	0.002%
42	7.698	1988	1993	1994	rBV2	219	155	0.02%	0.002%
43	7.711	1994	1997	2002	rVV	249	250	0.03%	0.003%
44	7.891	2039	2053	2077	rBV	427610	737590	77.78%	10.078%
45	8.132	2124	2128	2129	rBV2	267	212	0.02%	0.003%
46	8.174	2130	2141	2159	rBV	81931	139682	14.73%	1.908%
47	8.280	2172	2174	2182	rVB2	529	470	0.05%	0.006%
48	8.377	2202	2204	2209	rVB	275	240	0.03%	0.003%
49	8.457	2225	2229	2231	rBV	339	317	0.03%	0.004%
50	8.627	2266	2282	2317	rBV	243885	475813	50.17%	6.501%
51	9.242	2468	2473	2476	rVB2	423	349	0.04%	0.005%
52	9.258	2476	2478	2481	rBV2	217	158	0.02%	0.002%
53	9.412	2514	2526	2553	rBV	414944	714072	75.30%	9.756%
54	9.695	2609	2614	2625	rVB2	786	1267	0.13%	0.017%
55	9.962	2694	2697	2700	rBV2	231	173	0.02%	0.002%
56	10.078	2730	2733	2736	rBV2	231	147	0.02%	0.002%
57	10.106	2736	2742	2747	rVV2	545	535	0.06%	0.007%
58	10.190	2760	2768	2771	rBV2	252	330	0.03%	0.005%
59	10.277	2791	2795	2799	rVB2	183	157	0.02%	0.002%
60	10.547	2872	2879	2881	rBV2	197	243	0.03%	0.003%
61	10.692	2921	2924	2928	rBV2	177	148	0.02%	0.002%
62	10.753	2929	2943	2962	rBV	287181	474934	50.08%	6.489%
63	10.888	2978	2985	2996	rBV3	969	1327	0.14%	0.018%
64	11.106	3050	3053	3054	rBV	255	165	0.02%	0.002%
65	11.222	3083	3089	3093	rBV	186	246	0.03%	0.003%
66	11.377	3131	3137	3140	rBV2	180	219	0.02%	0.003%
67	11.473	3164	3167	3170	rVB3	259	177	0.02%	0.002%
68	11.524	3180	3183	3187	rVB2	264	172	0.02%	0.002%
69	11.557	3190	3193	3197	rBV	187	159	0.02%	0.002%
70	11.634	3213	3217	3219	rBV2	209	170	0.02%	0.002%
71	11.688	3230	3234	3238	rBV2	242	265	0.03%	0.004%
72	11.746	3245	3252	3260	rVV2	2943	3582	0.38%	0.049%
73	11.807	3260	3271	3296	rBV	423614	699440	73.75%	9.556%
74	12.190	3377	3390	3411	rBV	399563	682207	71.94%	9.321%
75	12.357	3439	3442	3446	rBV2	241	175	0.02%	0.002%
76	12.396	3451	3454	3457	rBV	334	201	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
 Data File : VU057859.D
 Acq On : 08 Feb 2024 12:31
 Operator : MD/SY
 Sample : P1352-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	12.766	3561	3569	3576	rVB	1123	1569	0.17%	0.021%
78	12.875	3598	3603	3606	rBV2	217	211	0.02%	0.003%
79	12.946	3619	3625	3631	rVB2	386	367	0.04%	0.005%
80	13.052	3655	3658	3666	rVB2	311	378	0.04%	0.005%
81	13.097	3667	3672	3676	rVV3	330	298	0.03%	0.004%
82	13.193	3698	3702	3704	rBV	269	151	0.02%	0.002%
83	13.389	3760	3763	3770	rVB2	227	261	0.03%	0.004%
84	13.425	3771	3774	3777	rVV	245	196	0.02%	0.003%
85	13.444	3777	3780	3782	rVV2	289	192	0.02%	0.003%
86	13.457	3782	3784	3788	rVB2	256	152	0.02%	0.002%
87	13.576	3818	3821	3825	rBV	235	210	0.02%	0.003%
88	13.647	3841	3843	3848	rVB2	263	154	0.02%	0.002%
89	13.794	3886	3889	3896	rVB2	358	271	0.03%	0.004%
90	13.846	3896	3905	3917	rBV5	6896	12358	1.30%	0.169%
91	14.103	3983	3985	3988	rBV2	379	319	0.03%	0.004%
92	14.267	4033	4036	4039	rBV2	305	260	0.03%	0.004%
93	14.335	4049	4057	4070	rBV4	4857	7623	0.80%	0.104%
94	14.508	4108	4111	4116	rBV3	280	288	0.03%	0.004%
95	14.531	4116	4118	4123	rBV2	399	302	0.03%	0.004%
96	14.569	4124	4130	4132	rBV2	633	641	0.07%	0.009%
97	14.666	4156	4160	4163	rBV	237	211	0.02%	0.003%
98	14.724	4171	4178	4180	rBV3	387	447	0.05%	0.006%
99	15.280	4345	4351	4357	rBV4	384	685	0.07%	0.009%
100	15.656	4466	4468	4476	rVB3	482	427	0.05%	0.006%




Sum of corrected areas: 7319144

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057859.D
Acq On : 08 Feb 2024 12:31
Operator : MD/SY
Sample : P1352-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

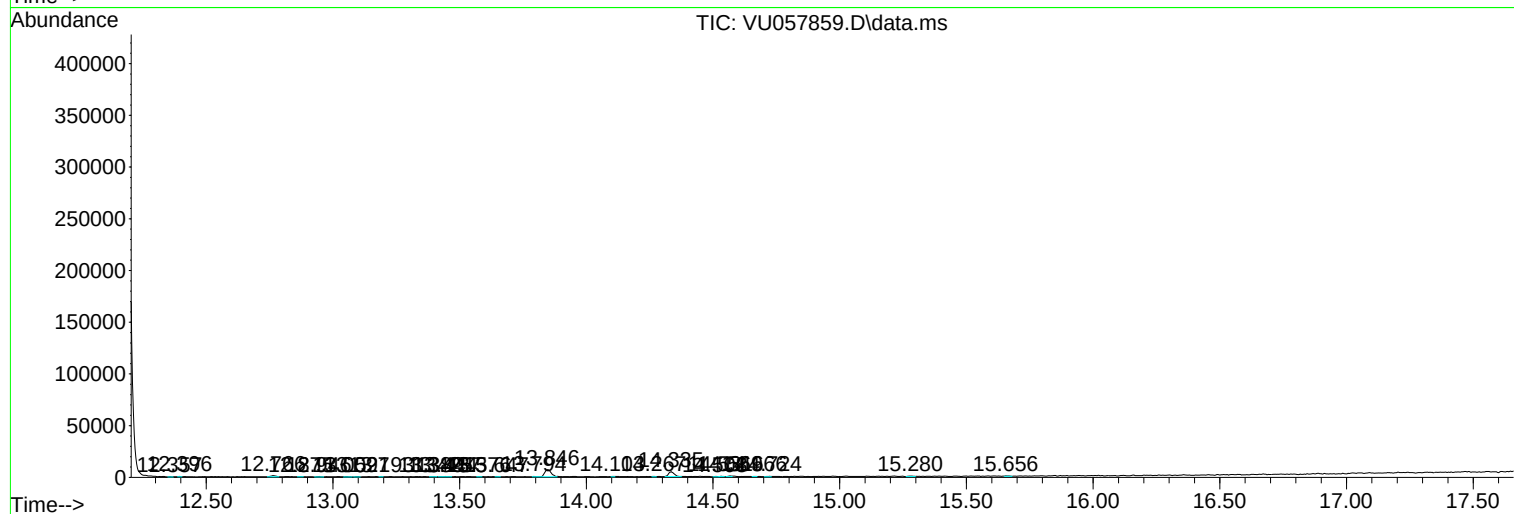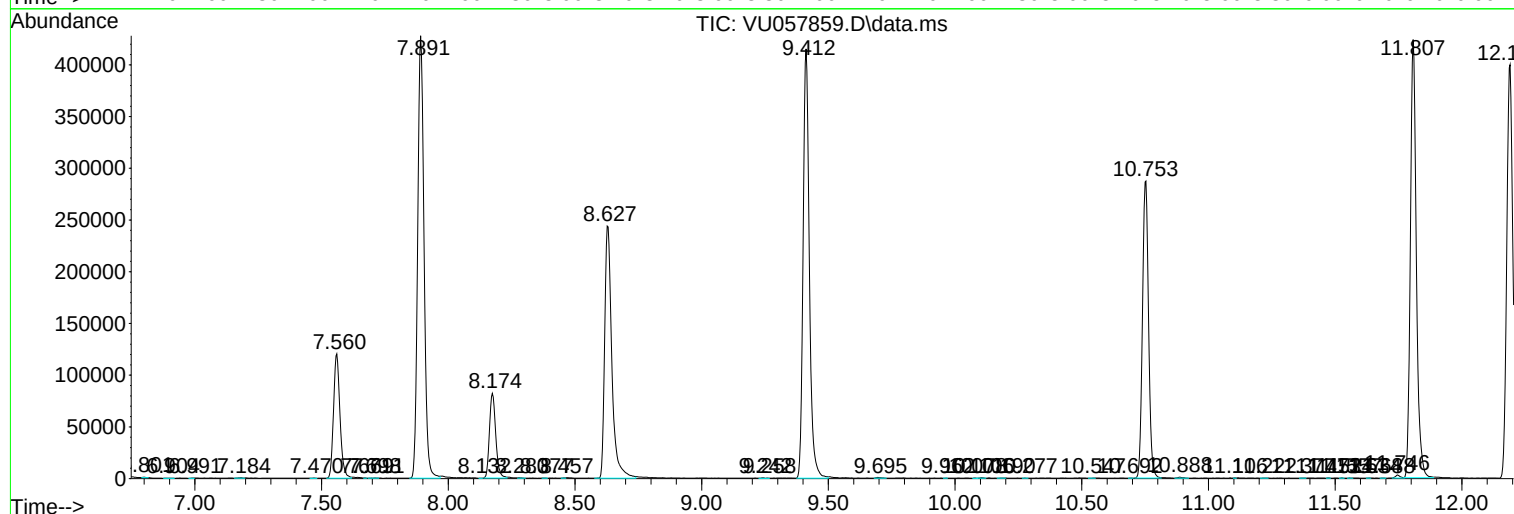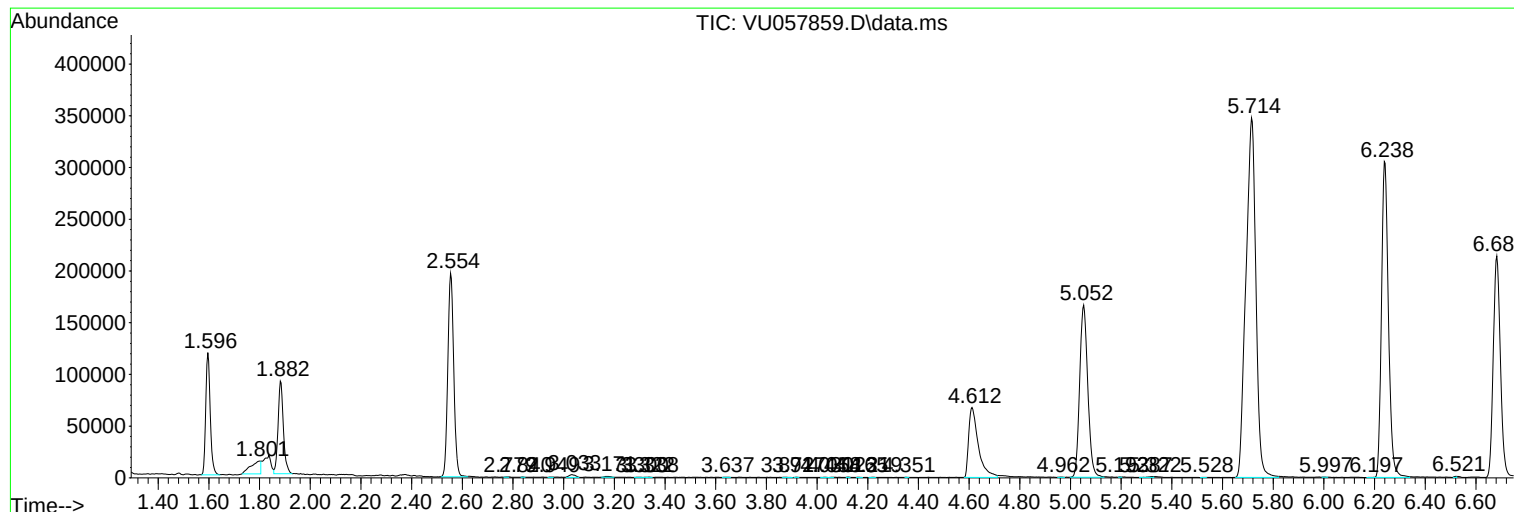

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057859.D
Acq On : 08 Feb 2024 12:31
Operator : MD/SY
Sample : P1352-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020824\
Data File : VU057859.D
Acq On : 08 Feb 2024 12:31
Operator : MD/SY
Sample : P1352-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc