
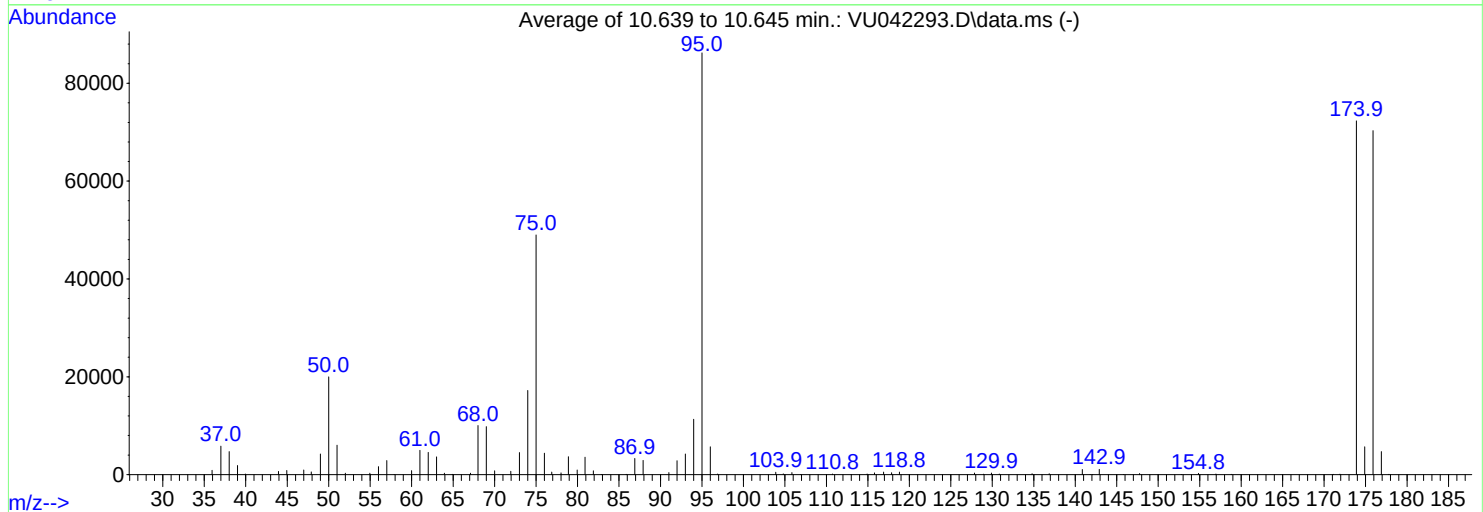


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020921\
 Data File : VU042293.D
 Acq On : 09 Feb 2021 13:06
 Operator : SY/MD
 Sample : BFB45
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB45

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR012021WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Feb 10 02:29:25 2021

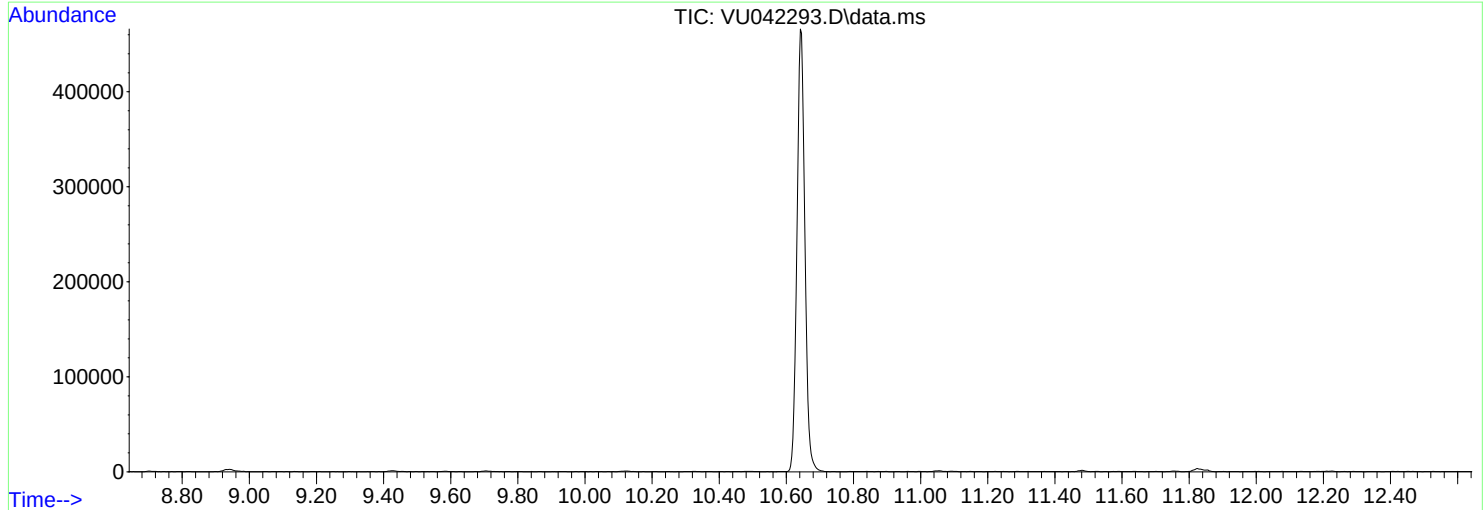

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	19989	PASS
75	95	30	80	56.8	48992	PASS
95	95	100	100	100.0	86219	PASS
96	95	5	9	6.6	5684	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.9	72331	PASS
175	174	5	9	7.9	5709	PASS
176	174	95	101	97.2	70323	PASS
177	176	5	9	6.7	4707	PASS

m/z	Abundance
36.00	844.0
37.00	5510.0
38.00	4587.0
39.00	1816.0
40.00	161.0
44.00	980.0
45.00	905.0
47.00	921.0
47.90	545.0
49.00	4037.0
50.00	19296.0
51.00	5850.0
52.00	302.0
54.90	289.0
56.00	1645.0
57.00	2729.0
57.90	104.0
60.00	743.0
61.00	4772.0
62.00	4341.0
63.00	3505.0
64.00	290.0
64.90	125.0
67.00	255.0
68.00	9790.0
69.00	9300.0
70.00	752.0
72.00	603.0
73.00	4337.0
74.00	16648.0
75.00	46552.0
76.00	4295.0
76.90	524.0
78.00	302.0
78.90	3334.0
79.90	896.0
80.90	3470.0
81.90	742.0
82.90	112.0
86.90	3058.0
87.90	2825.0
91.00	396.0
92.00	2780.0
93.00	3821.0
94.00	10838.0
95.00	82040.0
96.00	5569.0
96.90	138.0
103.90	447.0
104.80	107.0
105.80	388.0
110.80	105.0
114.90	114.0
115.80	300.0
116.90	477.0
117.90	306.0
118.80	524.0
127.80	339.0
129.90	312.0
130.80	108.0
134.80	204.0
136.90	172.0
140.90	1050.0
142.90	1001.0
147.70	205.0
154.90	240.0
157.00	139.0
158.80	119.0
173.90	66520.0
174.90	5497.0
175.90	64568.0
176.90	4415.0
177.80	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
35.90	912.0
37.00	6005.0
38.00	4835.0
39.00	1938.0
40.00	142.0
44.00	980.0
45.00	892.0
47.00	981.0
47.90	589.0
49.00	4366.0
50.00	20760.0
51.00	6224.0
52.00	293.0
54.90	319.0
56.00	1684.0
57.00	3007.0
60.00	837.0
61.00	5201.0
62.00	4652.0
63.00	3745.0
63.90	283.0
64.90	115.0
67.10	296.0
68.00	10381.0
69.00	10124.0
70.00	811.0
72.00	705.0
73.00	4681.0
74.00	17728.0
75.00	50656.0
76.00	4584.0
76.90	539.0
78.00	383.0
78.90	3767.0
79.90	984.0
80.90	3664.0
81.90	810.0
85.90	108.0
86.90	3467.0
87.90	3032.0
91.00	442.0
92.00	3001.0
93.00	4403.0
94.00	11724.0
95.00	88704.0
96.00	5851.0
96.90	111.0
103.90	512.0
104.80	175.0
105.90	433.0
106.90	107.0
110.70	121.0
114.90	137.0
115.80	363.0
116.90	512.0
117.90	401.0
118.80	548.0
127.90	332.0
128.90	127.0
129.90	343.0
130.80	124.0
134.80	216.0
136.90	188.0
140.90	1076.0
142.10	110.0
142.90	1144.0
147.80	237.0
152.80	112.0
154.80	264.0
157.00	129.0
158.80	103.0
171.10	106.0
171.90	252.0
173.90	74744.0
174.90	5882.0
175.90	72512.0
176.90	4888.0
177.80	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
35.90	897.0
37.00	5926.0
38.00	4701.0
39.00	1841.0
39.90	123.0
44.00	913.0
44.90	789.0
47.00	980.0
47.90	573.0
49.00	4267.0
50.00	19912.0
51.00	5991.0
52.00	249.0
55.00	293.0
56.00	1535.0
57.00	2911.0
60.00	876.0
61.00	4940.0
62.00	4690.0
63.00	3688.0
63.90	284.0
67.20	323.0
68.00	9928.0
69.00	10055.0
70.00	789.0
71.90	707.0
73.00	4536.0
74.00	17248.0
75.00	49768.0
76.00	4260.0
76.90	566.0
78.00	392.0
78.90	3868.0
80.00	1007.0
80.90	3580.0
81.90	776.0
85.80	120.0
86.90	3399.0
87.90	2841.0
91.00	452.0
92.00	2798.0
93.00	4406.0
94.00	11381.0
95.00	87912.0
96.00	5633.0
96.90	112.0
103.90	557.0
104.80	216.0
105.90	474.0
110.80	131.0
113.00	121.0
114.90	137.0
115.80	382.0
116.90	538.0
117.80	455.0
118.80	498.0
127.90	305.0
129.00	167.0
129.90	333.0
130.90	122.0
134.80	218.0
136.80	214.0
140.80	1028.0
141.80	120.0
142.90	1127.0
145.80	108.0
147.80	228.0
154.90	248.0
156.80	131.0
171.10	133.0
173.90	75728.0
174.90	5747.0
175.90	73888.0
176.90	4819.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
43.90	311.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45