

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020923\
 Data File : VU053018.D
 Acq On : 09 Feb 2023 14:55
 Operator : JC/MD
 Sample : 01480-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L57-020723-FD

Quant Time: Feb 09 15:15:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jan 24 05:16:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.112	96	32508	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	11885	1.099	ug/l	0.00
Spiked Amount 1.000			Recovery	=	110.000%	
68) 1,2-Dichlorobenzene-d4	12.189	152	9692	0.871	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020923\
Data File : VU053018.D
Acq On : 09 Feb 2023 14:55
Operator : JC/MD
Sample : 01480-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L57-020723-FD

Quant Time: Feb 09 15:15:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jan 24 05:16:59 2023
Response via : Initial Calibration




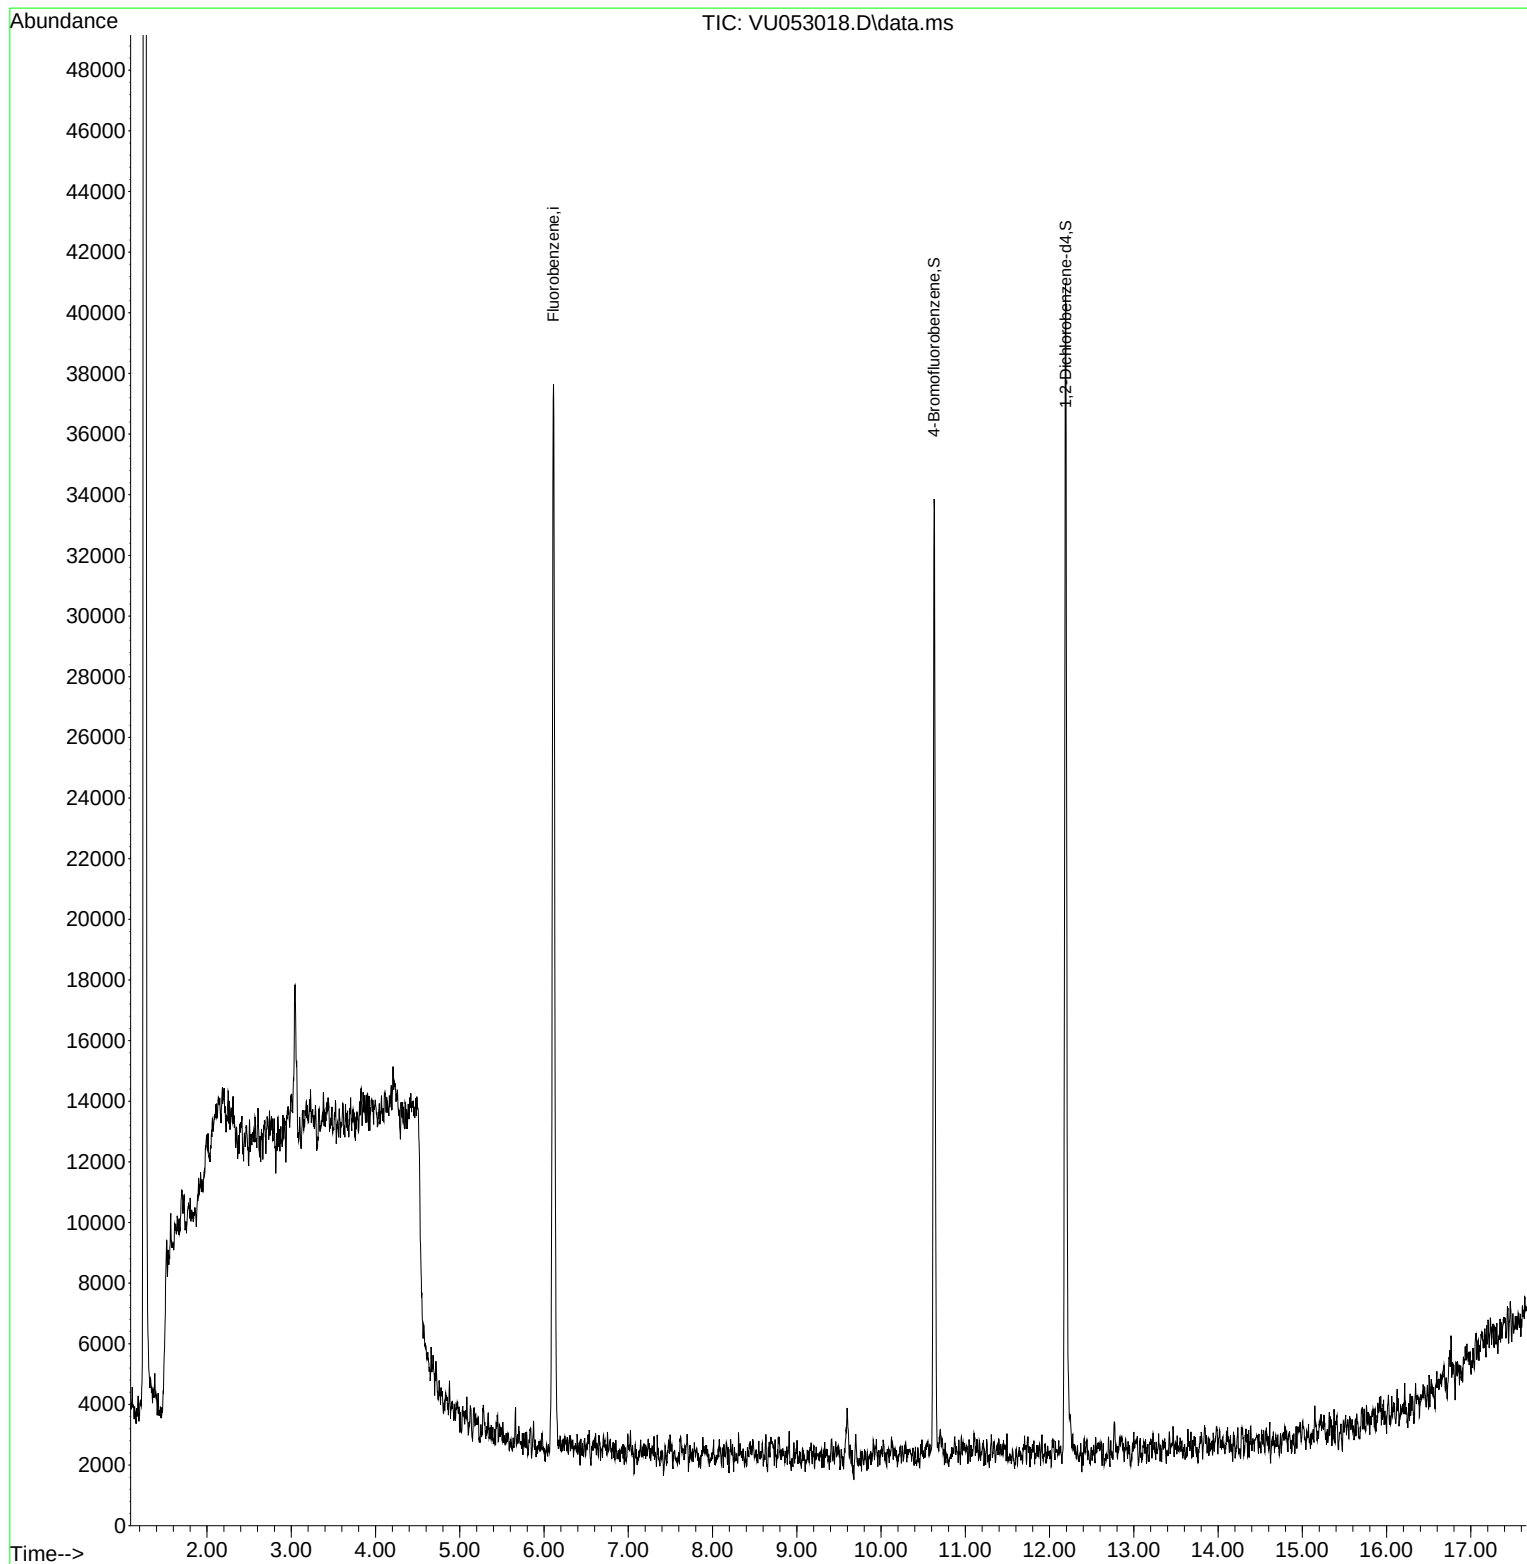


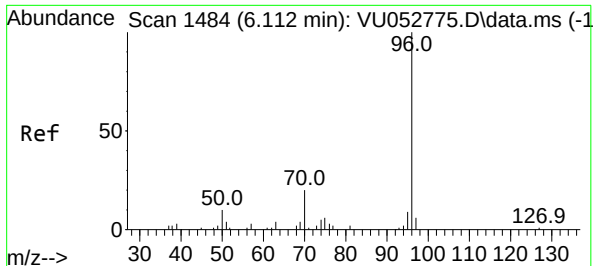

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU053018.D
Acq: 09 Feb 2023 14:55




Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L57-020723-FD


Tgt Ion: 96	Resp: 32508
Ion Ratio	Lower Upper
96 100	
70 20.8	16.2 24.4
95 9.9	7.4 11.0
97 7.6	0.0 0.0#

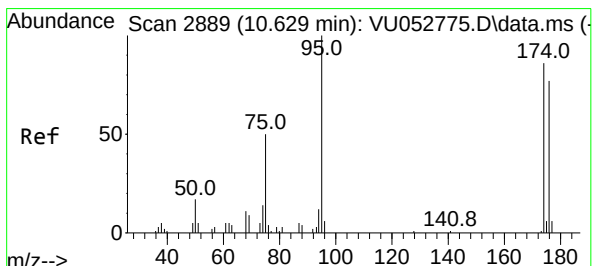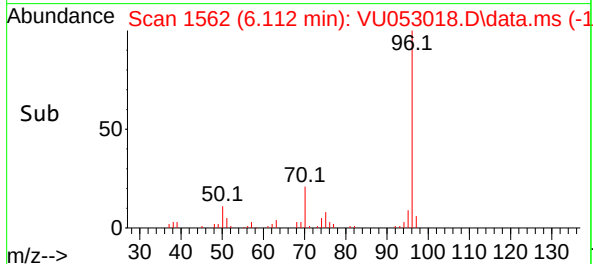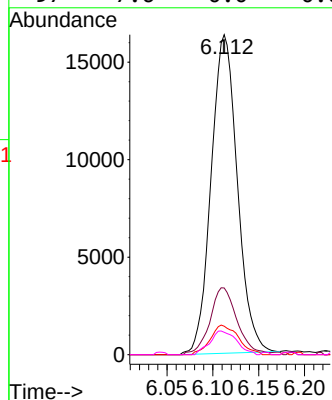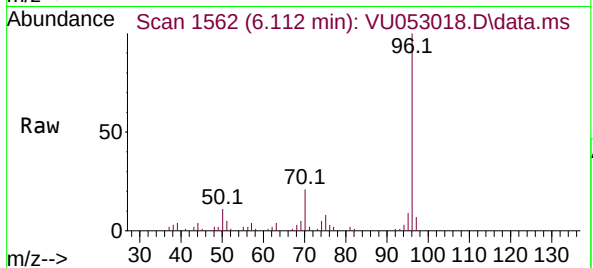

#57
4-Bromofluorobenzene
Concen: 1.099 ug/l
RT: 10.630 min Scan# 2967
Delta R.T. 0.001 min
Lab File: VU053018.D
Acq: 09 Feb 2023 14:55

Tgt Ion: 95	Resp: 11885
Ion Ratio	Lower Upper
95 100	
174 61.5	66.9 100.3#
176 59.2	61.9 92.9#

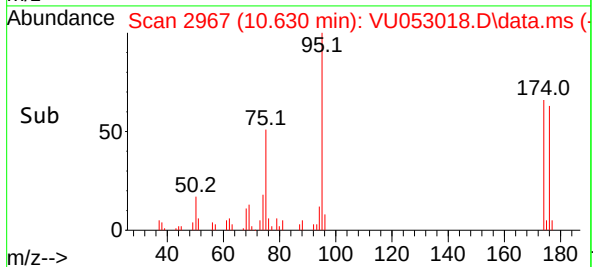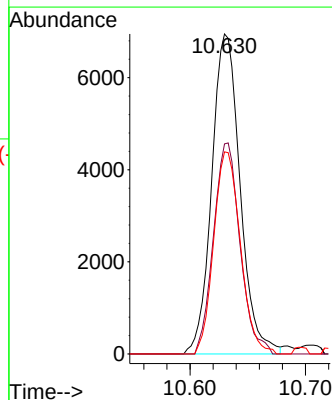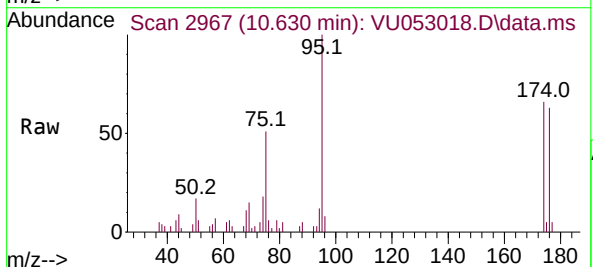

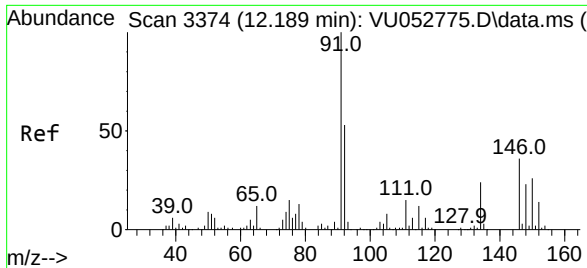

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.871 ug/l
 RT: 12.189 min Scan# 34
 Delta R.T. 0.001 min
 Lab File: VU053018.D
 Acq: 09 Feb 2023 14:55

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L57-020723-FD

Tgt Ion:	152	Resp:	9692
Ion Ratio	Lower	Upper	
152	100		
115	73.9	0.0	262.6
150	156.8	0.0	638.0

