

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020923\
 Data File : VU053023.D
 Acq On : 09 Feb 2023 17:51
 Operator : JC/MD
 Sample : 01479-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L10-D-020723

Quant Time: Feb 10 01:22:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jan 24 05:16:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.109	96	33475	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	11300	1.015	ug/l	0.00
Spiked Amount 1.000			Recovery	=	101.000%	
68) 1,2-Dichlorobenzene-d4	12.189	152	9571	0.836	ug/l	0.00
Spiked Amount 1.000			Recovery	=	84.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020923\
Data File : VU053023.D
Acq On : 09 Feb 2023 17:51
Operator : JC/MD
Sample : 01479-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-020723

Quant Time: Feb 10 01:22:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jan 24 05:16:59 2023
Response via : Initial Calibration




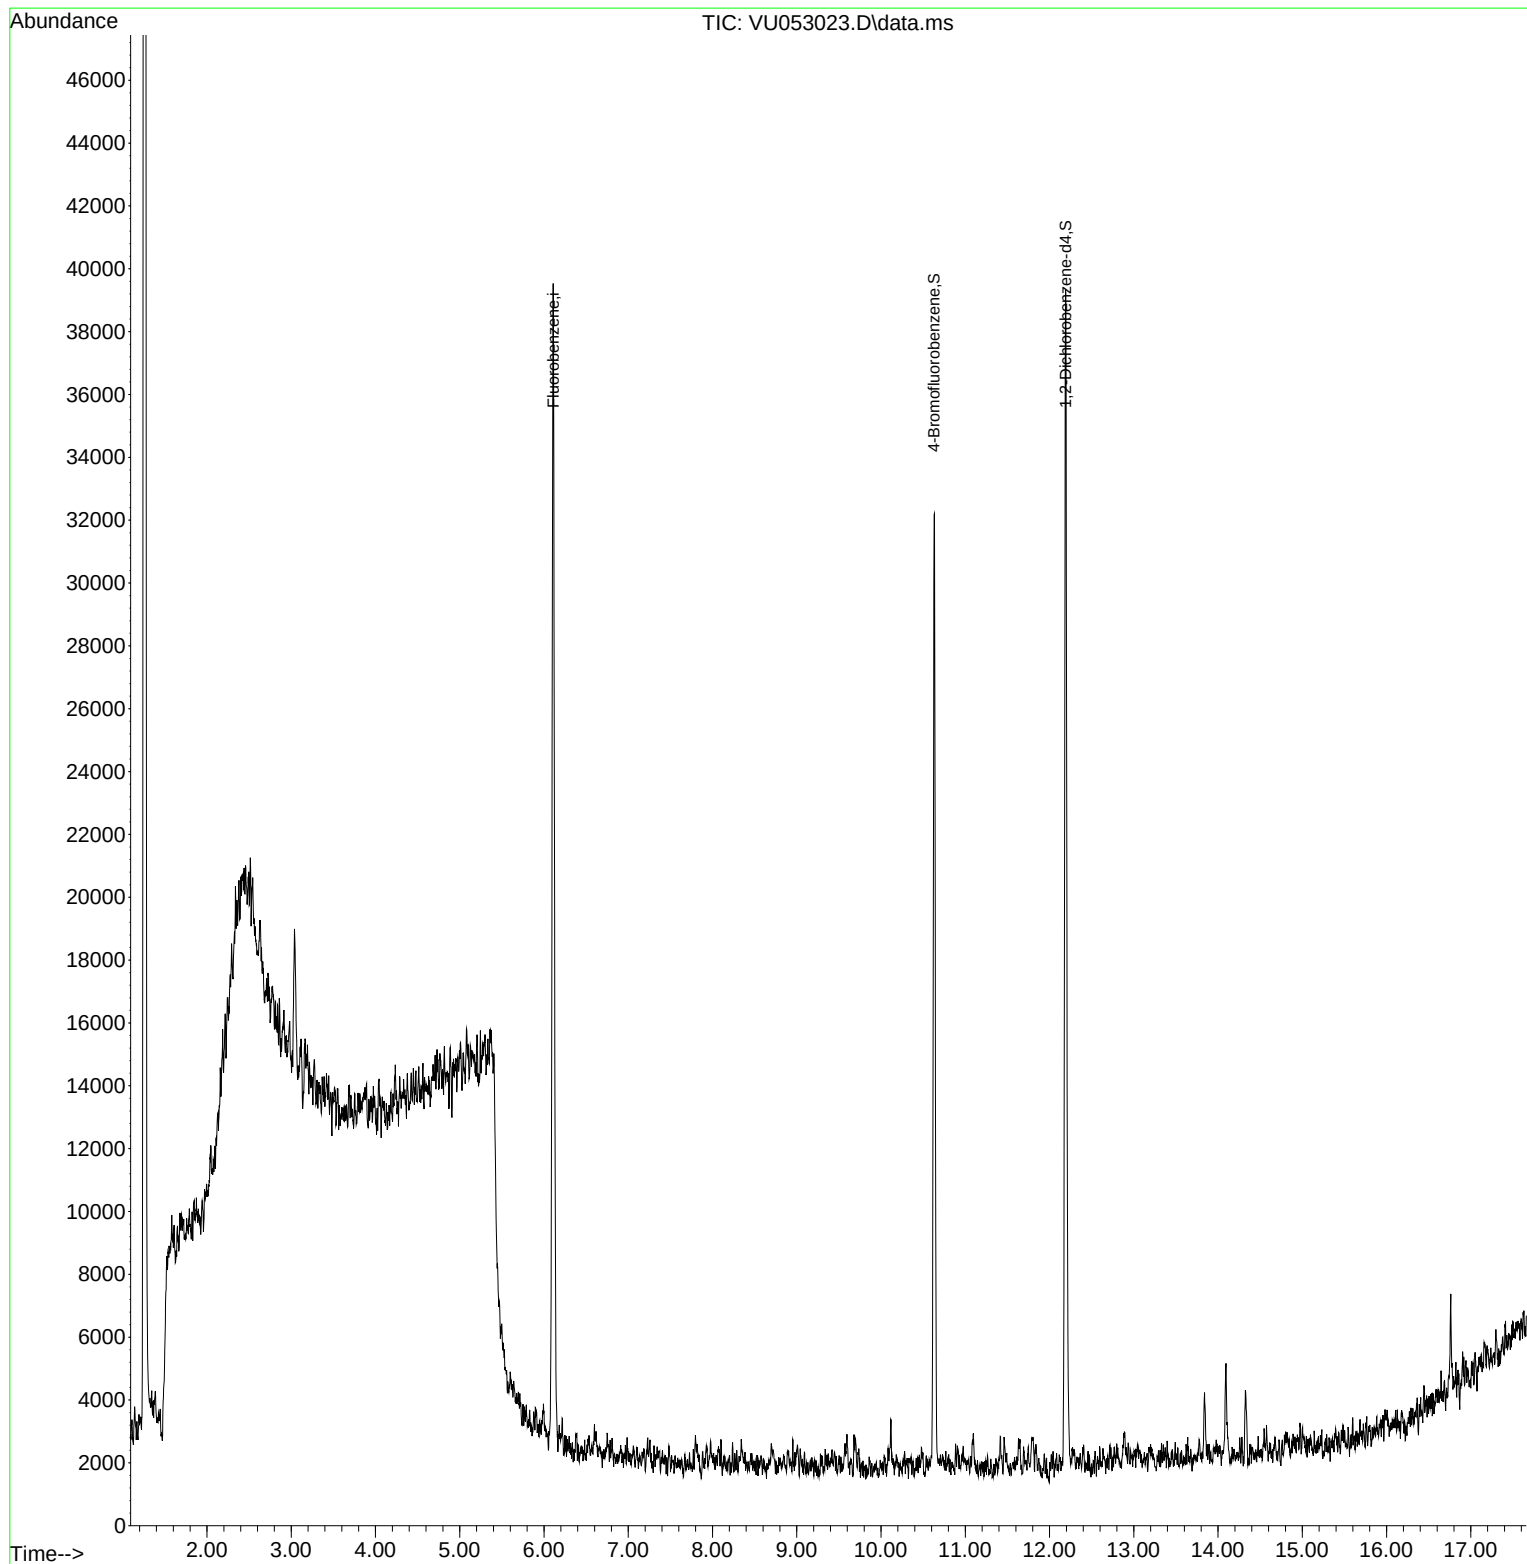


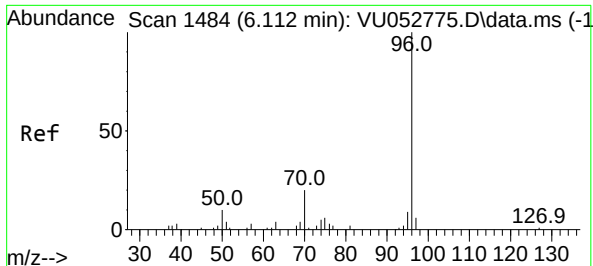

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.109 min Scan# 11
Delta R.T. -0.003 min
Lab File: VU053023.D
Acq: 09 Feb 2023 17:51




Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-020723


Tgt Ion: 96	Resp: 33475
Ion Ratio	Lower Upper
96 100	
70 20.2	16.2 24.4
95 9.1	7.4 11.0
97 7.6	0.0 0.0

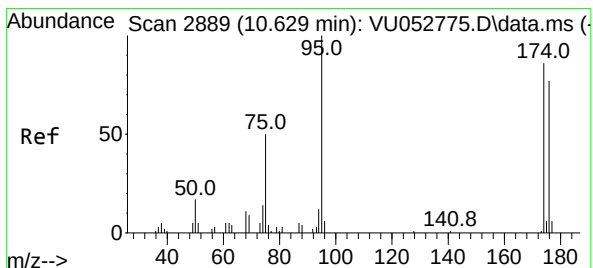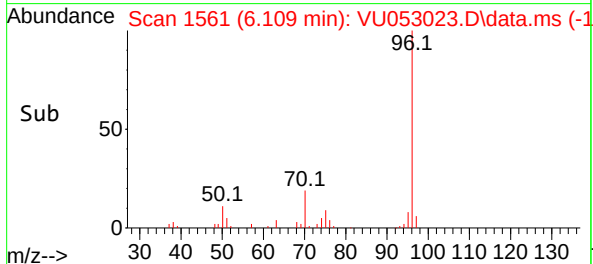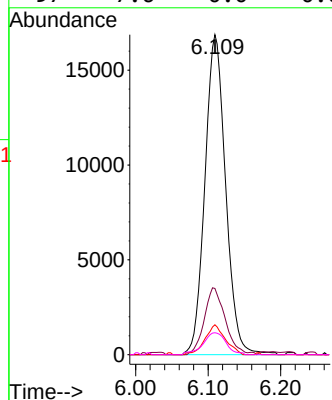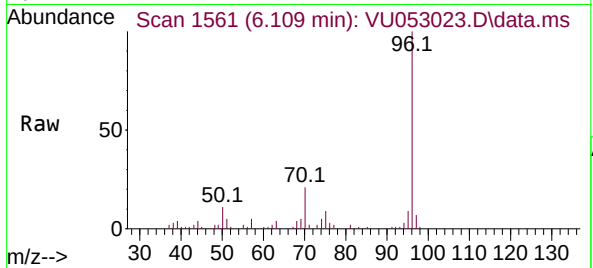

#57
4-Bromofluorobenzene
Concen: 1.015 ug/l
RT: 10.630 min Scan# 2967
Delta R.T. 0.001 min
Lab File: VU053023.D
Acq: 09 Feb 2023 17:51

Tgt Ion: 95	Resp: 11300
Ion Ratio	Lower Upper
95 100	
174 62.4	66.9 100.3
176 62.0	61.9 92.9

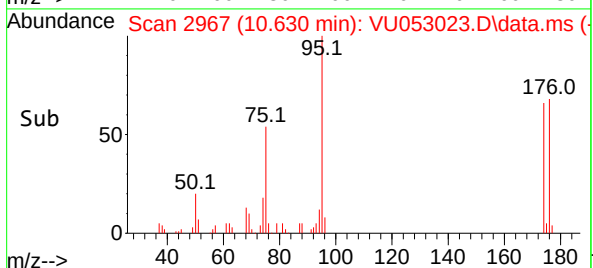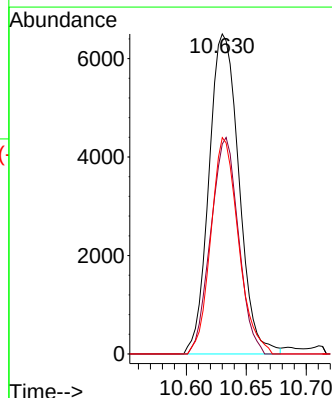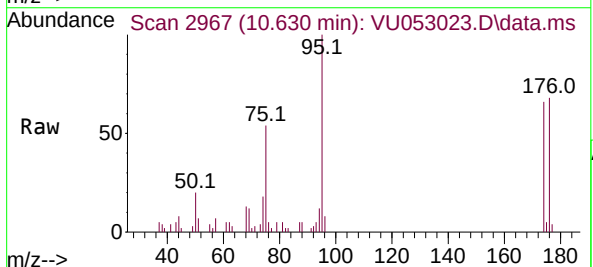

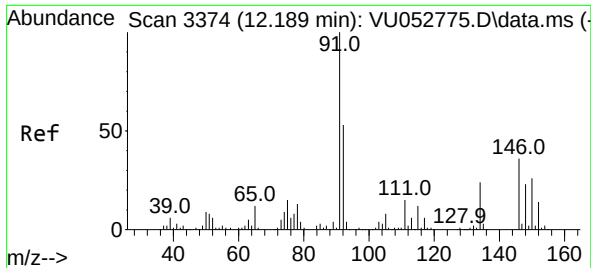

#68

1,2-Dichlorobenzene-d4

Concen: 0.836 ug/l

RT: 12.189 min Scan# 34

Delta R.T. 0.001 min

Lab File: VU053023.D


Acq: 09 Feb 2023 17:51

Instrument :

MSVOA_U

ClientSampleId :

PW-B6-L10-D-020723

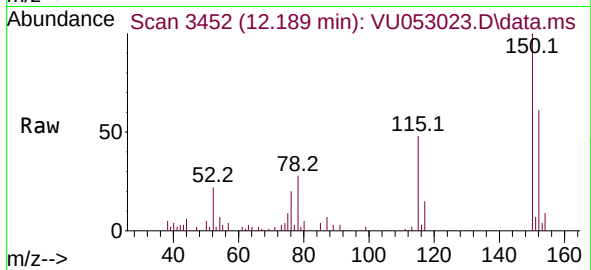

Tgt Ion:152 Resp: 9571

Ion Ratio Lower Upper

152 100

115 76.0 0.0 262.6

150 158.3 0.0 638.0

