

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020923\
 Data File : VU053024.D
 Acq On : 09 Feb 2023 18:22
 Operator : JC/MD
 Sample : 01479-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L10-D-020723-FD

Quant Time: Feb 10 01:23:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jan 24 05:16:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.109	96	33018	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	11366	1.035	ug/l	0.00
Spiked Amount	1.000		Recovery	=	103.000%	
68) 1,2-Dichlorobenzene-d4	12.189	152	9699	0.858	ug/l	0.00
Spiked Amount	1.000		Recovery	=	86.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020923\
Data File : VU053024.D
Acq On : 09 Feb 2023 18:22
Operator : JC/MD
Sample : 01479-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-020723-FD

Quant Time: Feb 10 01:23:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jan 24 05:16:59 2023
Response via : Initial Calibration




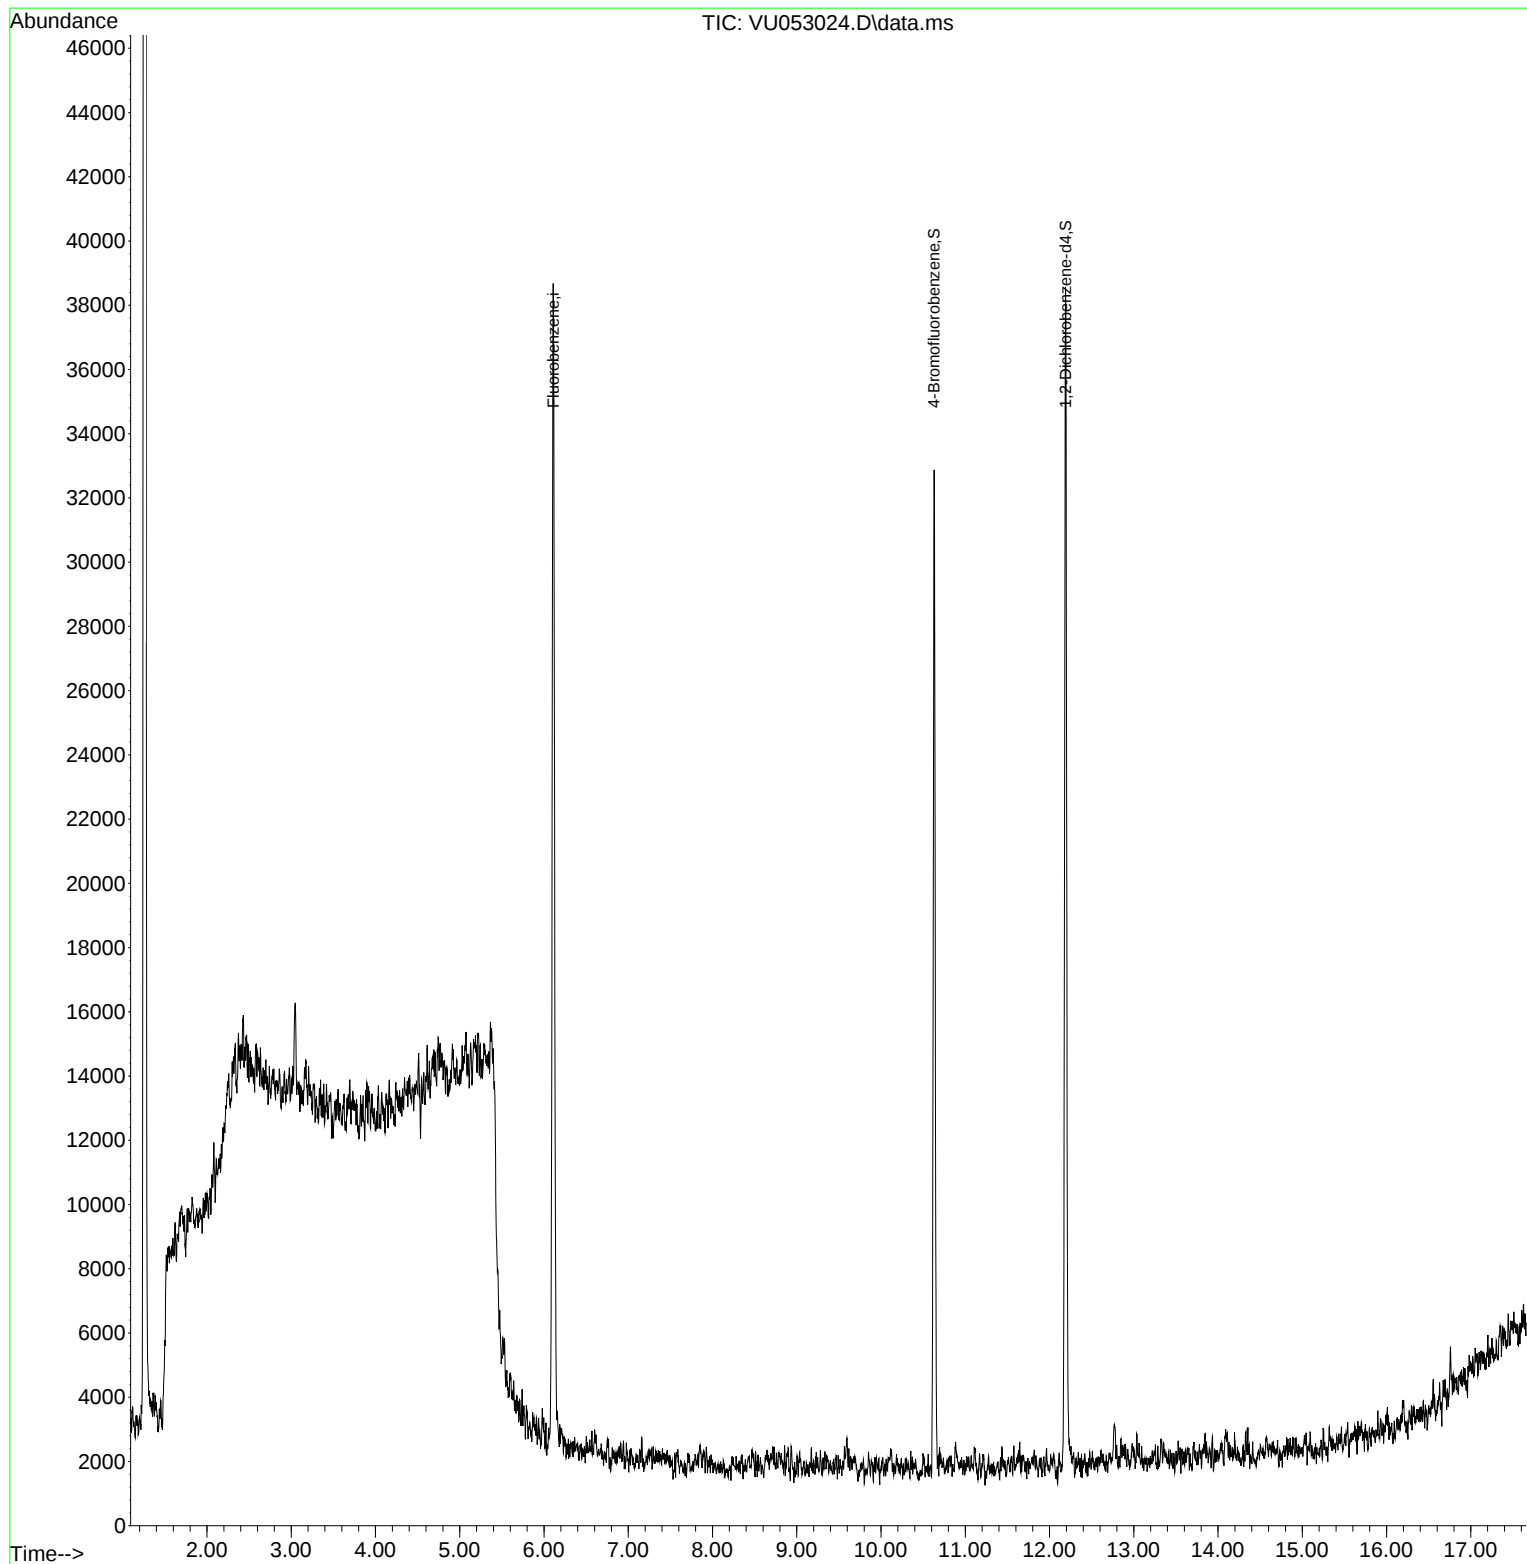


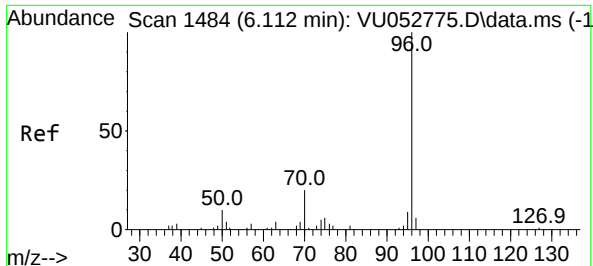

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.109 min Scan# 11
Delta R.T. -0.003 min
Lab File: VU053024.D
Acq: 09 Feb 2023 18:22




Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-020723-FD


Tgt Ion: 96	Resp: 33018
Ion Ratio	Lower Upper
96 100	
70 22.5	16.2 24.4
95 9.2	7.4 11.0
97 6.2	0.0 0.0#

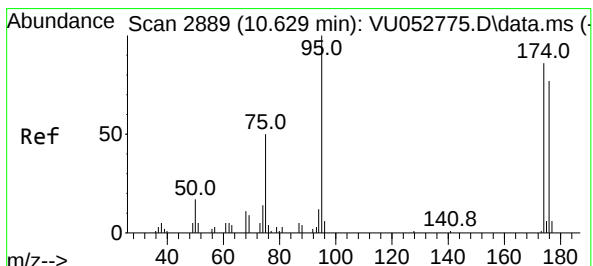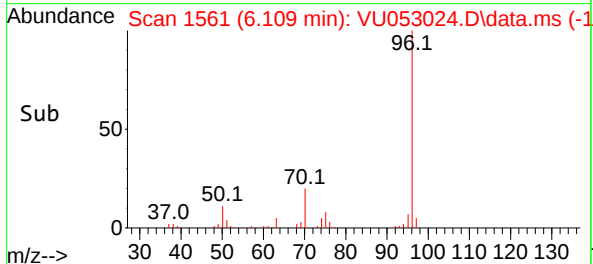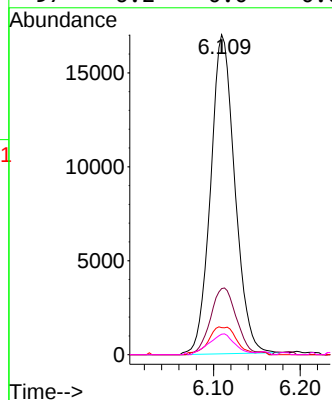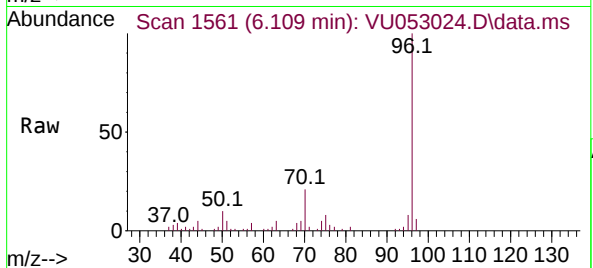

#57
4-Bromofluorobenzene
Concen: 1.035 ug/l
RT: 10.630 min Scan# 2967
Delta R.T. 0.001 min
Lab File: VU053024.D
Acq: 09 Feb 2023 18:22


Tgt Ion: 95	Resp: 11366
Ion Ratio	Lower Upper
95 100	
174 64.9	66.9 100.3#
176 61.0	61.9 92.9#

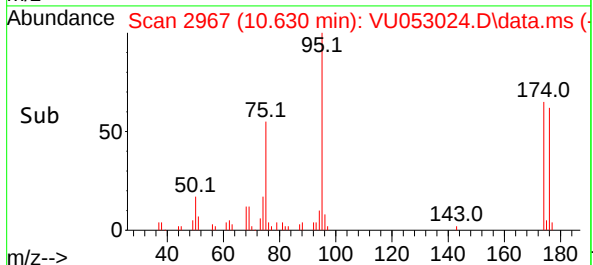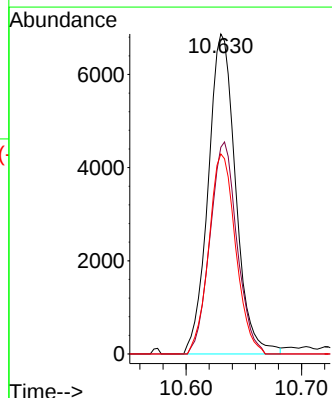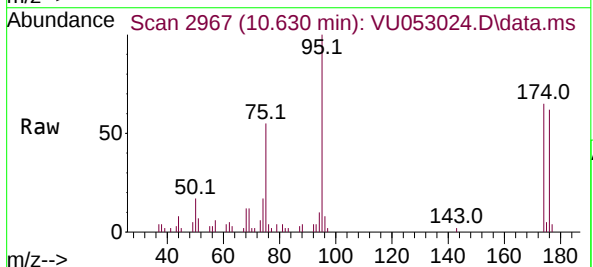

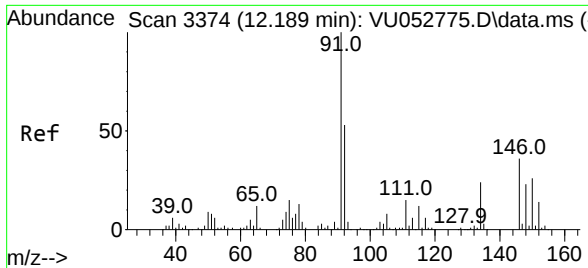

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.858 ug/l
 RT: 12.189 min Scan# 34
 Delta R.T. 0.001 min
 Lab File: VU053024.D
 Acq: 09 Feb 2023 18:22

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L10-D-020723-FD

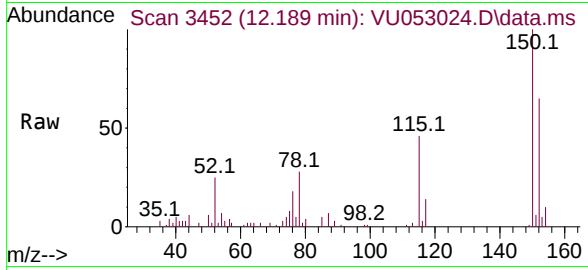

Tgt Ion:	152	Resp:	9699
Ion Ratio	Lower	Upper	
152	100		
115	70.2	0.0	262.6
150	155.7	0.0	638.0

