


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020923\
 Data File : VU053012.D
 Acq On : 09 Feb 2023 09:24
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Tue Jan 24 05:16:59 2023

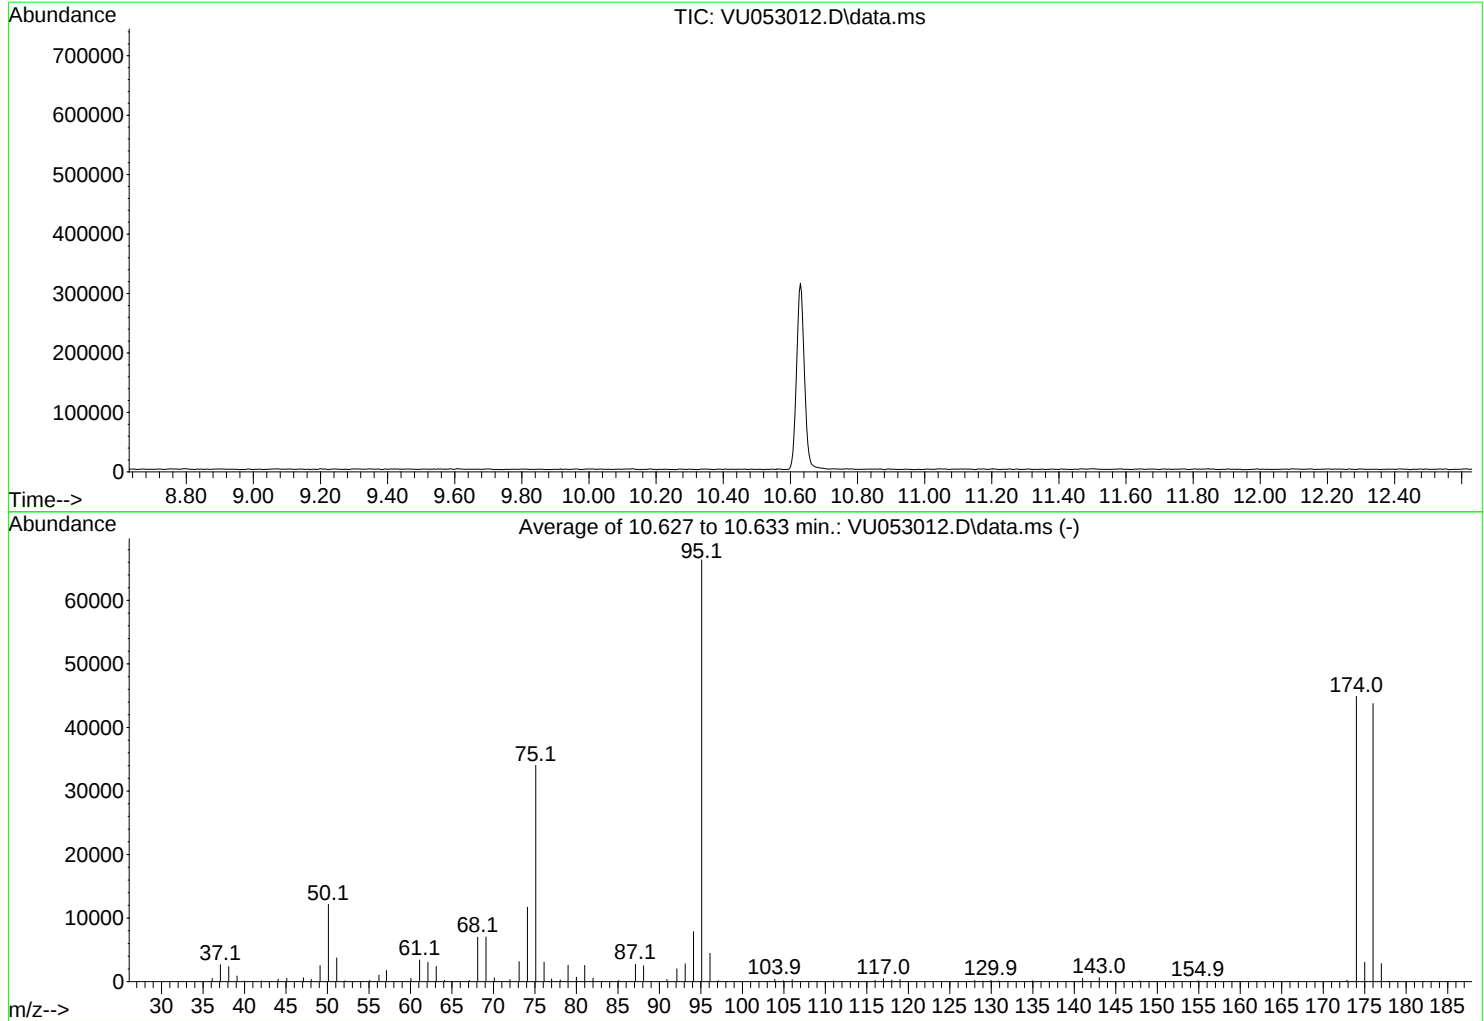

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2952

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	12156	PASS
75	95	30	60	51.3	34043	PASS
95	95	100	100	100.0	66384	PASS
96	95	5	9	6.7	4451	PASS
173	174	0.00	2	0.5	220	PASS
174	95	50	100	67.6	44896	PASS
175	174	5	9	6.8	3063	PASS
176	174	95	101	97.5	43757	PASS
177	176	5	9	6.4	2812	PASS