

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036705.D
 Acq On : 10 Feb 2020 12:05
 Operator : JC/MD
 Sample : VU0210WBL05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK109

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	99	rBV	119341	128365	13.29%	1.657%
2	1.932	176	184	200	rVB	106987	141321	14.63%	1.825%
3	2.594	378	390	404	rBV	188438	308637	31.95%	3.985%
4	2.748	436	438	444	rVB	181	87	0.01%	0.001%
5	2.993	512	514	516	rVB	183	59	0.01%	0.001%
6	3.083	535	542	549	rBV3	1148	1737	0.18%	0.022%
7	3.224	576	586	602	rVB2	2514	5362	0.56%	0.069%
8	3.288	602	606	612	rBV	159	138	0.01%	0.002%
9	3.372	630	632	634	rVB	173	68	0.01%	0.001%
10	3.385	634	636	645	rVB	201	118	0.01%	0.002%
11	3.546	683	686	689	rBV	97	77	0.01%	0.001%
12	3.620	705	709	711	rBV3	415	395	0.04%	0.005%
13	3.806	765	767	772	rVB	205	119	0.01%	0.002%
14	3.915	798	801	803	rBV	88	64	0.01%	0.001%
15	4.034	836	838	842	rVB	179	84	0.01%	0.001%
16	4.057	842	845	847	rBV	109	65	0.01%	0.001%
17	4.153	872	875	880	rVB2	211	192	0.02%	0.002%
18	4.243	900	903	904	rBV	116	69	0.01%	0.001%
19	4.269	909	911	916	rVB	261	175	0.02%	0.002%
20	4.301	916	921	924	rBV	149	158	0.02%	0.002%
21	4.321	925	927	929	rBV	131	54	0.01%	0.001%
22	4.359	936	939	944	rVB	223	144	0.01%	0.002%
23	4.449	966	967	970	rVB2	144	74	0.01%	0.001%
24	4.481	975	977	980	rVB	123	69	0.01%	0.001%
25	4.610	1013	1017	1019	rBV	98	79	0.01%	0.001%
26	4.626	1019	1022	1023	rBV	122	62	0.01%	0.001%
27	4.677	1023	1038	1060	rBV	115324	267555	27.70%	3.455%
28	5.028	1144	1147	1149	rBV2	111	79	0.01%	0.001%
29	5.041	1150	1151	1154	rVB	179	91	0.01%	0.001%
30	5.112	1157	1173	1192	rBV	173277	373087	38.62%	4.817%
31	5.420	1266	1269	1272	rBV2	341	304	0.03%	0.004%
32	5.456	1277	1280	1283	rBV	72	72	0.01%	0.001%
33	5.517	1295	1299	1302	rBV	175	138	0.01%	0.002%
34	5.546	1306	1308	1309	rBV	179	69	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036705.D
 Acq On : 10 Feb 2020 12:05
 Operator : JC/MD
 Sample : VU0210WBL05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK109

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

35	5.665	1342	1345	1348	rBV	98	61	0.01%	0.001%
36	5.767	1356	1377	1398	rBV2	367513	966013	100.00%	12.473%
37	6.134	1489	1491	1492	rBV2	271	111	0.01%	0.001%
38	6.147	1492	1495	1497	rBV	341	228	0.02%	0.003%
39	6.195	1503	1510	1514	rBV3	325	395	0.04%	0.005%
40	6.292	1525	1540	1557	rBV	344850	644145	66.68%	8.317%
41	6.526	1611	1613	1618	rVB	209	136	0.01%	0.002%
42	6.565	1618	1625	1635	rBV3	2444	3894	0.40%	0.050%
43	6.648	1649	1651	1655	rVB	158	82	0.01%	0.001%
44	6.732	1662	1677	1699	rBV	235859	454130	47.01%	5.864%
45	6.838	1706	1710	1711	rBV	395	269	0.03%	0.003%
46	6.883	1722	1724	1727	rBV2	231	90	0.01%	0.001%
47	6.935	1737	1740	1743	rBV	124	100	0.01%	0.001%
48	7.015	1761	1765	1768	rBV	98	81	0.01%	0.001%
49	7.060	1776	1779	1783	rBV	70	63	0.01%	0.001%
50	7.163	1807	1811	1812	rBV	145	86	0.01%	0.001%
51	7.218	1821	1828	1834	rBV4	1101	1189	0.12%	0.015%
52	7.259	1840	1841	1843	rBV4	138	59	0.01%	0.001%
53	7.398	1882	1884	1888	rVB2	140	93	0.01%	0.001%
54	7.497	1912	1915	1918	rBV	118	80	0.01%	0.001%
55	7.600	1934	1947	1968	rBV	134663	235556	24.38%	3.042%
56	7.758	1993	1996	1999	rBV2	265	164	0.02%	0.002%
57	7.780	2001	2003	2006	rBV	160	67	0.01%	0.001%
58	7.796	2006	2008	2011	rVB	178	64	0.01%	0.001%
59	7.812	2011	2013	2014	rBV	405	156	0.02%	0.002%
60	7.828	2015	2018	2019	rBV2	685	409	0.04%	0.005%
61	7.931	2036	2050	2065	rBV	450750	766053	79.30%	9.891%
62	8.211	2125	2137	2160	rBV	94529	158544	16.41%	2.047%
63	8.353	2179	2181	2185	rBV2	331	255	0.03%	0.003%
64	8.430	2201	2205	2208	rBV	173	116	0.01%	0.001%
65	8.500	2222	2227	2230	rBV	210	201	0.02%	0.003%
66	8.581	2243	2252	2259	rBV4	2790	3637	0.38%	0.047%
67	8.668	2266	2279	2310	rBV	345036	611358	63.29%	7.894%
68	8.870	2340	2342	2345	rVB2	192	107	0.01%	0.001%
69	8.893	2345	2349	2354	rBV	97	135	0.01%	0.002%
70	8.973	2367	2374	2380	rBV3	645	929	0.10%	0.012%
71	9.111	2414	2417	2419	rBV	98	59	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036705.D
 Acq On : 10 Feb 2020 12:05
 Operator : JC/MD
 Sample : VU0210WBL05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK109

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

72	9.192	2439	2442	2447	rVB2	160	160	0.02%	0.002%
73	9.288	2470	2472	2475	rVB	152	66	0.01%	0.001%
74	9.446	2508	2521	2545	rBV	482714	795281	82.33%	10.269%
75	9.597	2563	2568	2572	rVV2	295	326	0.03%	0.004%
76	9.619	2572	2575	2578	rVB	145	88	0.01%	0.001%
77	9.658	2584	2587	2589	rBV	140	93	0.01%	0.001%
78	9.716	2602	2605	2612	rBV3	431	494	0.05%	0.006%
79	9.767	2619	2621	2623	rBV	145	54	0.01%	0.001%
80	9.812	2633	2635	2640	rBV2	210	131	0.01%	0.002%
81	9.880	2653	2656	2661	rVB	215	155	0.02%	0.002%
82	9.906	2661	2664	2667	rVB2	146	107	0.01%	0.001%
83	9.925	2667	2670	2673	rBV	189	142	0.01%	0.002%
84	9.983	2684	2688	2690	rBV	156	132	0.01%	0.002%
85	10.034	2702	2704	2711	rBV	170	158	0.02%	0.002%
86	10.111	2723	2728	2729	rBV	163	149	0.02%	0.002%
87	10.279	2776	2780	2783	rVB	292	196	0.02%	0.003%
88	10.298	2783	2786	2788	rBV	192	142	0.01%	0.002%
89	10.372	2806	2809	2814	rBV	122	80	0.01%	0.001%
90	10.783	2924	2937	2955	rBV	317067	510398	52.84%	6.590%
91	10.906	2972	2975	2981	rVB	273	293	0.03%	0.004%
92	11.111	3036	3039	3043	rVB2	413	263	0.03%	0.003%
93	11.462	3145	3148	3150	rBV	151	107	0.01%	0.001%
94	11.835	3251	3264	3281	rBV	439220	702202	72.69%	9.067%
95	12.214	3370	3382	3397	rVB	398622	654263	67.73%	8.448%
96	12.500	3468	3471	3474	rBV	288	181	0.02%	0.002%
97	12.999	3623	3626	3629	rBV2	257	212	0.02%	0.003%
98	13.555	3797	3799	3803	rBV	237	131	0.01%	0.002%
99	13.803	3873	3876	3878	rBV	349	218	0.02%	0.003%
100	13.915	3909	3911	3913	rBV	328	110	0.01%	0.001%


Sum of corrected areas: 7744614

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU021020\
Data File : VU036705.D
Acq On : 10 Feb 2020 12:05
Operator : JC/MD
Sample : VU0210WBL05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK109

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

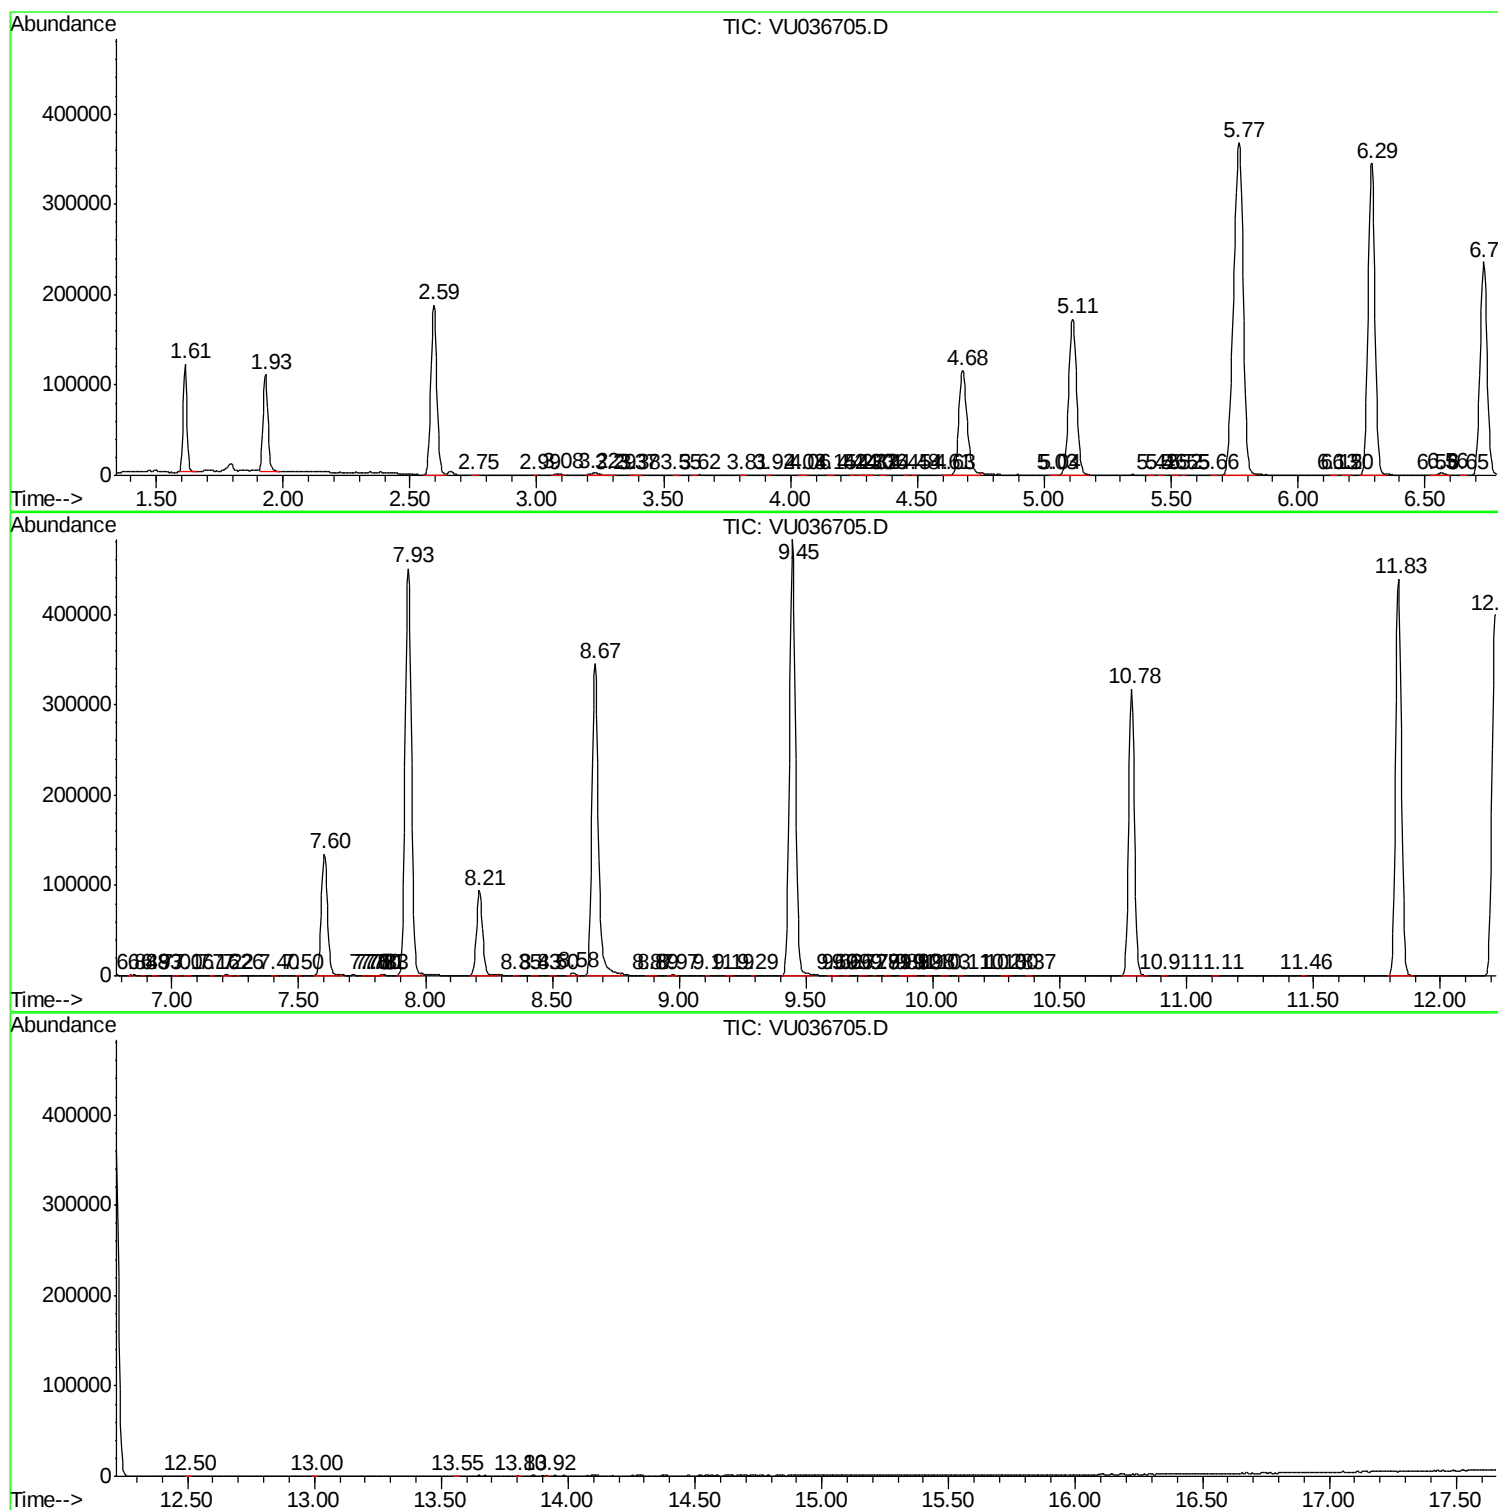

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU021020\
Data File : VU036705.D
Acq On : 10 Feb 2020 12:05
Operator : JC/MD
Sample : VU0210WBL05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK109

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU021020\
Data File : VU036705.D
Acq On : 10 Feb 2020 12:05
Operator : JC/MD
Sample : VU0210WBL05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK109

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc