

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036706.D
 Acq On : 10 Feb 2020 12:28
 Operator : JC/MD
 Sample : VU0210WBL06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK110

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	96	rVB	118484	123311	13.05%	1.632%
2	1.928	176	183	202	rVB	104267	137634	14.57%	1.821%
3	2.594	378	390	403	rBV	181535	296890	31.42%	3.928%
4	2.970	505	507	509	rVB	180	48	0.01%	0.001%
5	3.086	535	543	548	rBV3	1038	1441	0.15%	0.019%
6	3.227	579	587	599	rVB2	1613	3408	0.36%	0.045%
7	3.395	637	639	640	rBV2	143	41	0.00%	0.001%
8	3.620	705	709	710	rBV2	458	306	0.03%	0.004%
9	3.690	730	731	735	rVB2	140	88	0.01%	0.001%
10	3.755	750	751	754	rVB2	151	40	0.00%	0.001%
11	3.777	754	758	760	rBV	146	121	0.01%	0.002%
12	3.822	770	772	776	rVB	203	79	0.01%	0.001%
13	3.870	786	787	789	rVB	129	30	0.00%	0.000%
14	3.880	789	790	792	rVB	124	43	0.00%	0.001%
15	3.893	792	794	797	rBV	45	27	0.00%	0.000%
16	4.002	826	828	829	rBV	121	48	0.01%	0.001%
17	4.025	833	835	836	rBV	133	36	0.00%	0.000%
18	4.195	882	888	892	rBV2	227	211	0.02%	0.003%
19	4.279	912	914	915	rVB	114	27	0.00%	0.000%
20	4.333	928	931	934	rVB	200	104	0.01%	0.001%
21	4.362	938	940	941	rBV	141	61	0.01%	0.001%
22	4.443	960	965	968	rBV	97	107	0.01%	0.001%
23	4.468	971	973	978	rVB	161	100	0.01%	0.001%
24	4.530	990	992	995	rVB	186	65	0.01%	0.001%
25	4.565	1000	1003	1006	rBV	294	172	0.02%	0.002%
26	4.681	1023	1039	1064	rBV	114707	269154	28.49%	3.561%
27	5.021	1141	1145	1150	rBV2	207	243	0.03%	0.003%
28	5.050	1152	1154	1156	rVB	278	147	0.02%	0.002%
29	5.111	1156	1173	1193	rBV	167558	363111	38.43%	4.805%
30	5.272	1222	1223	1227	rVB	256	82	0.01%	0.001%
31	5.398	1260	1262	1264	rBV	150	42	0.00%	0.001%
32	5.414	1264	1267	1270	rVV2	372	285	0.03%	0.004%
33	5.446	1274	1277	1280	rVB	247	109	0.01%	0.001%
34	5.462	1280	1282	1284	rBV	178	86	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036706.D
 Acq On : 10 Feb 2020 12:28
 Operator : JC/MD
 Sample : VU0210WBL06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK110

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

35	5.568	1313	1315	1317	rBV	72	43	0.00%	0.001%
36	5.681	1348	1350	1352	rVB	129	36	0.00%	0.000%
37	5.767	1355	1377	1399	rBV2	361586	944821	100.00%	12.502%
38	6.060	1466	1468	1471	rBV	246	140	0.01%	0.002%
39	6.086	1471	1476	1480	rVV2	332	308	0.03%	0.004%
40	6.134	1490	1491	1494	rBV	187	74	0.01%	0.001%
41	6.150	1494	1496	1499	rVV	204	148	0.02%	0.002%
42	6.176	1502	1504	1506	rBV	56	29	0.00%	0.000%
43	6.195	1506	1510	1512	rBV2	198	150	0.02%	0.002%
44	6.288	1524	1539	1560	rBV	337913	630436	66.73%	8.342%
45	6.565	1617	1625	1633	rVB6	2116	3463	0.37%	0.046%
46	6.603	1635	1637	1639	rVV	138	58	0.01%	0.001%
47	6.626	1643	1644	1650	rVB	142	98	0.01%	0.001%
48	6.664	1654	1656	1661	rVB	152	46	0.00%	0.001%
49	6.732	1662	1677	1700	rBV	227274	439813	46.55%	5.820%
50	6.886	1723	1725	1730	rVB	201	134	0.01%	0.002%
51	6.909	1730	1732	1735	rBV	162	68	0.01%	0.001%
52	6.928	1735	1738	1740	rBV	94	61	0.01%	0.001%
53	6.992	1754	1758	1760	rBV	118	91	0.01%	0.001%
54	7.054	1773	1777	1780	rBV	92	75	0.01%	0.001%
55	7.073	1780	1783	1785	rBV	99	71	0.01%	0.001%
56	7.124	1796	1799	1802	rBV	67	55	0.01%	0.001%
57	7.221	1822	1829	1835	rBV2	869	1055	0.11%	0.014%
58	7.343	1860	1867	1870	rBV	159	215	0.02%	0.003%
59	7.372	1875	1876	1878	rBV	169	67	0.01%	0.001%
60	7.385	1878	1880	1882	rBV	65	35	0.00%	0.000%
61	7.420	1889	1891	1892	rBV	123	27	0.00%	0.000%
62	7.542	1924	1929	1932	rBV	108	130	0.01%	0.002%
63	7.600	1934	1947	1969	rBV	130230	227424	24.07%	3.009%
64	7.742	1990	1991	1992	rBV	230	55	0.01%	0.001%
65	7.835	2010	2020	2026	rBV3	1503	1775	0.19%	0.023%
66	7.931	2036	2050	2066	rBV	435188	737358	78.04%	9.757%
67	8.211	2125	2137	2159	rBV	90942	153187	16.21%	2.027%
68	8.343	2176	2178	2183	rBV2	242	136	0.01%	0.002%
69	8.394	2191	2194	2197	rVB	102	62	0.01%	0.001%
70	8.481	2217	2221	2224	rBV	119	100	0.01%	0.001%
71	8.504	2224	2228	2231	rBV2	181	198	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036706.D
 Acq On : 10 Feb 2020 12:28
 Operator : JC/MD
 Sample : VU0210WBL06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK110

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

72	8.584	2247	2253	2260	rVB6	2340	3367	0.36%	0.045%
73	8.668	2267	2279	2307	rBV	350692	603552	63.88%	7.986%
74	8.851	2334	2336	2339	rVB	178	116	0.01%	0.002%
75	8.893	2344	2349	2352	rBV	144	134	0.01%	0.002%
76	8.947	2359	2366	2370	rBV3	820	1064	0.11%	0.014%
77	9.082	2405	2408	2411	rBV	96	79	0.01%	0.001%
78	9.201	2442	2445	2447	rBV	121	73	0.01%	0.001%
79	9.317	2475	2481	2487	rBV	121	205	0.02%	0.003%
80	9.385	2499	2502	2505	rBV	103	97	0.01%	0.001%
81	9.446	2508	2521	2541	rBV	469688	768285	81.32%	10.166%
82	9.594	2564	2567	2571	rBV	293	270	0.03%	0.004%
83	9.722	2603	2607	2612	rBV2	422	416	0.04%	0.006%
84	9.938	2671	2674	2676	rBV	139	82	0.01%	0.001%
85	10.163	2740	2744	2747	rBV	200	152	0.02%	0.002%
86	10.221	2759	2762	2765	rBV	123	79	0.01%	0.001%
87	10.314	2786	2791	2795	rBV2	505	618	0.07%	0.008%
88	10.433	2823	2828	2830	rBV	258	251	0.03%	0.003%
89	10.513	2850	2853	2859	rVB2	327	290	0.03%	0.004%
90	10.606	2880	2882	2885	rVB	164	50	0.01%	0.001%
91	10.626	2885	2888	2892	rBV	215	131	0.01%	0.002%
92	10.783	2924	2937	2956	rBV	313650	500113	52.93%	6.618%
93	10.864	2959	2962	2965	rBV	301	206	0.02%	0.003%
94	11.114	3038	3040	3044	rBV	213	119	0.01%	0.002%
95	11.471	3149	3151	3152	rBV	151	40	0.00%	0.001%
96	11.487	3152	3156	3158	rBV2	227	189	0.02%	0.003%
97	11.835	3251	3264	3280	rVB	430300	692820	73.33%	9.167%
98	12.214	3370	3382	3400	rVB	401848	644516	68.22%	8.528%
99	12.307	3408	3411	3413	rBV	212	135	0.01%	0.002%
100	13.233	3697	3699	3704	rVB	415	171	0.02%	0.002%


Sum of corrected areas: 7557359

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU021020\
Data File : VU036706.D
Acq On : 10 Feb 2020 12:28
Operator : JC/MD
Sample : VU0210WBL06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

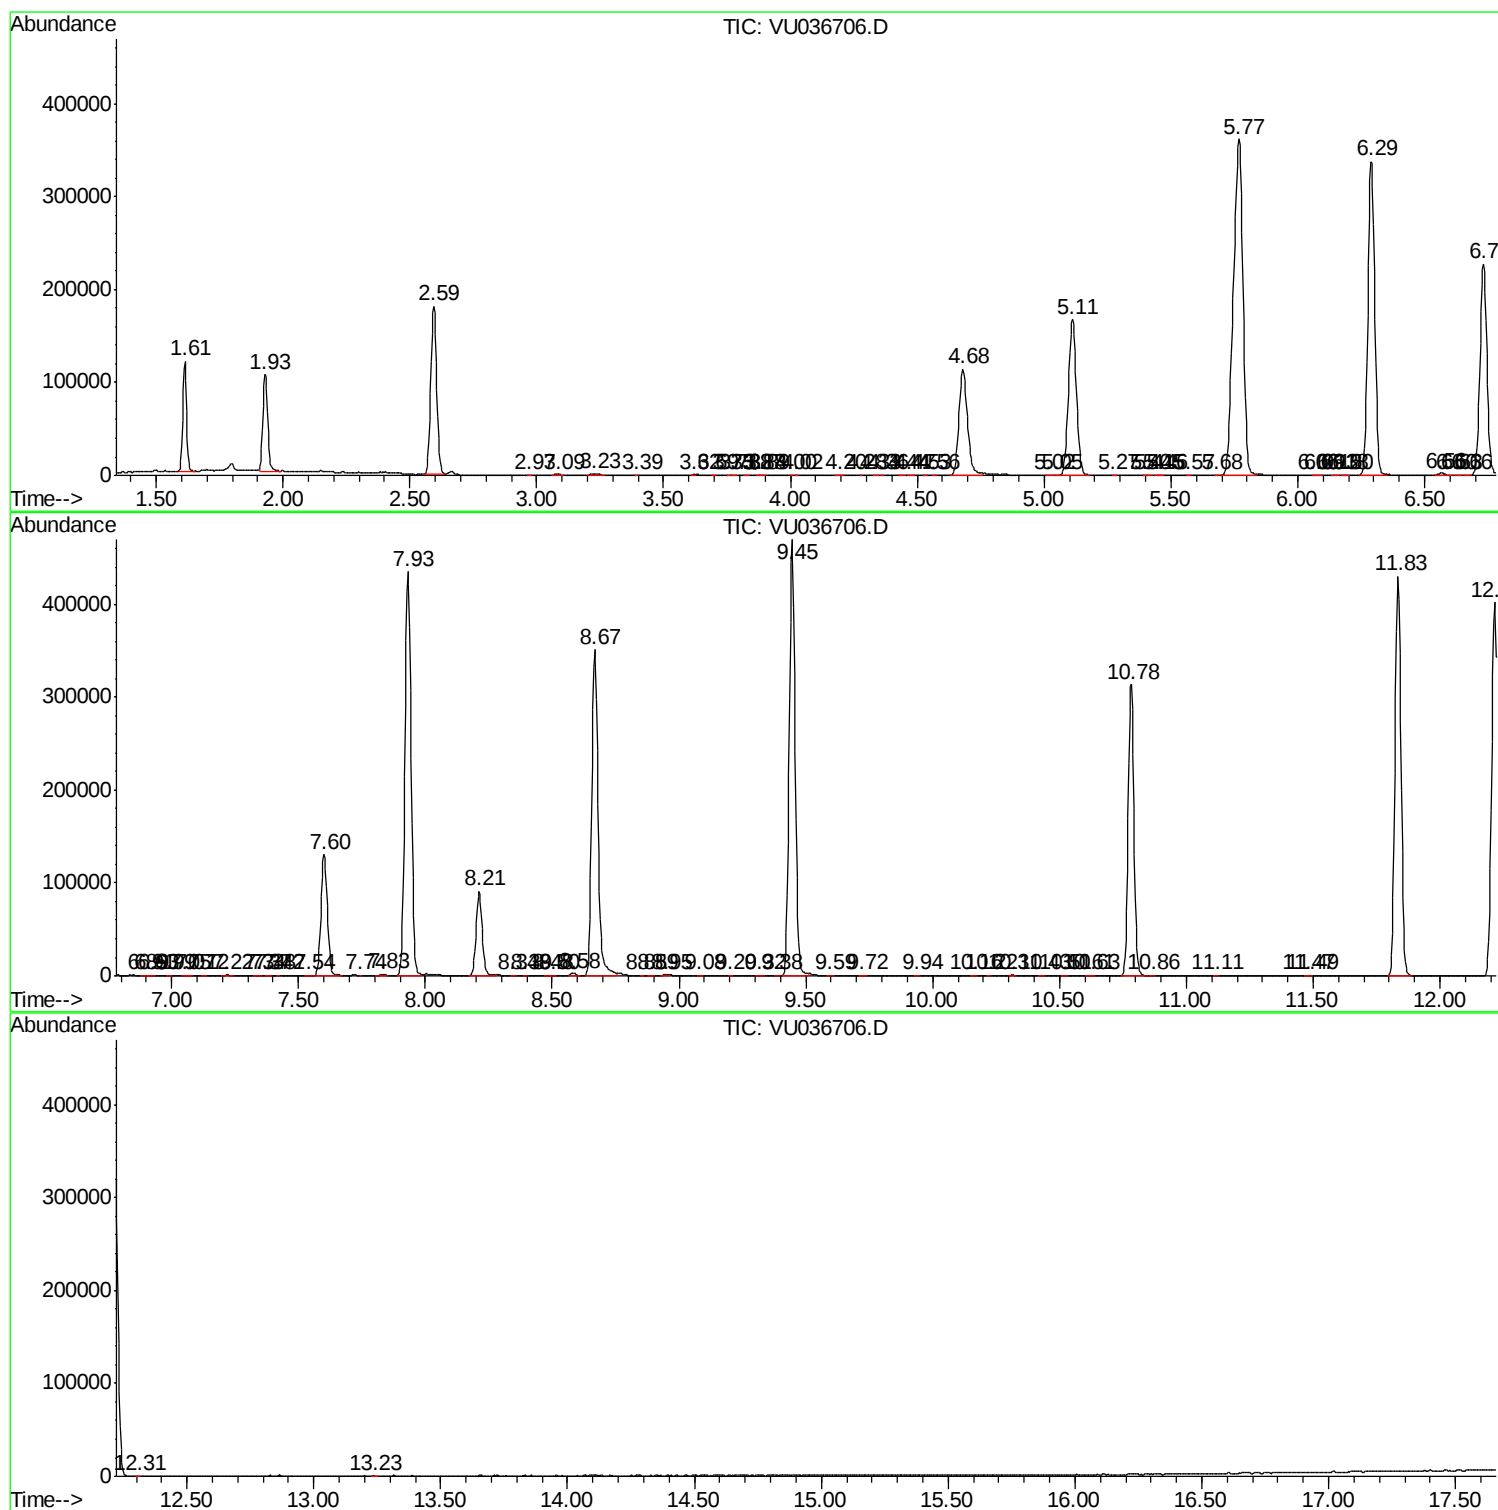

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU021020\
Data File : VU036706.D
Acq On : 10 Feb 2020 12:28
Operator : JC/MD
Sample : VU0210WBL06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU021020\
Data File : VU036706.D
Acq On : 10 Feb 2020 12:28
Operator : JC/MD
Sample : VU0210WBL06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc