

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036707.D
 Acq On : 10 Feb 2020 12:51
 Operator : JC/MD
 Sample : VU0210WBL07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.614	78	85	99	rBV	122522	131497	13.48%	1.708%
2	1.929	176	183	199	rVB	107977	142456	14.61%	1.851%
3	2.594	378	390	405	rBV	192825	313884	32.18%	4.078%
4	2.819	453	460	466	rBV2	455	685	0.07%	0.009%
5	2.925	490	493	496	rVB	213	145	0.01%	0.002%
6	3.083	535	542	549	rVB4	1186	1752	0.18%	0.023%
7	3.224	576	586	598	rBV2	2364	5124	0.53%	0.067%
8	3.334	616	620	624	rBV	208	175	0.02%	0.002%
9	3.482	663	666	670	rBV	105	77	0.01%	0.001%
10	3.565	690	692	694	rBV	147	60	0.01%	0.001%
11	3.626	703	711	713	rBV3	346	433	0.04%	0.006%
12	3.729	741	743	745	rVB	132	54	0.01%	0.001%
13	3.884	787	791	794	rBV	237	183	0.02%	0.002%
14	3.948	807	811	812	rBV	106	67	0.01%	0.001%
15	4.083	850	853	856	rVB	89	52	0.01%	0.001%
16	4.147	870	873	876	rVB	152	91	0.01%	0.001%
17	4.163	876	878	879	rBV	226	57	0.01%	0.001%
18	4.237	896	901	906	rBV	82	84	0.01%	0.001%
19	4.260	906	908	911	rVV	118	67	0.01%	0.001%
20	4.279	911	914	919	rVB	223	137	0.01%	0.002%
21	4.308	919	923	926	rBV	128	102	0.01%	0.001%
22	4.369	940	942	946	rVB	179	82	0.01%	0.001%
23	4.392	946	949	955	rVB	146	130	0.01%	0.002%
24	4.427	955	960	963	rBV	136	100	0.01%	0.001%
25	4.591	1007	1011	1013	rBV	120	83	0.01%	0.001%
26	4.678	1023	1038	1066	rBV	114809	269601	27.64%	3.502%
27	4.874	1097	1099	1101	rVB	306	125	0.01%	0.002%
28	5.112	1157	1173	1195	rVB	173540	372164	38.16%	4.835%
29	5.221	1204	1207	1209	rBV2	294	225	0.02%	0.003%
30	5.273	1220	1223	1226	rVB2	301	171	0.02%	0.002%
31	5.311	1231	1235	1238	rVB	113	91	0.01%	0.001%
32	5.337	1238	1243	1250	rVB3	620	820	0.08%	0.011%
33	5.392	1258	1260	1264	rVB2	157	140	0.01%	0.002%
34	5.414	1265	1267	1271	rVB2	129	85	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036707.D
 Acq On : 10 Feb 2020 12:51
 Operator : JC/MD
 Sample : VU0210WBL07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

35	5.520	1298	1300	1302	rBV	148	54	0.01%	0.001%
36	5.617	1328	1330	1334	rVB	213	116	0.01%	0.002%
37	5.649	1334	1340	1343	rBV	111	106	0.01%	0.001%
38	5.668	1344	1346	1349	rVB	170	57	0.01%	0.001%
39	5.768	1354	1377	1401	rBV2	372679	975307	100.00%	12.670%
40	5.954	1432	1435	1437	rBV	337	208	0.02%	0.003%
41	6.035	1457	1460	1463	rVB2	205	151	0.02%	0.002%
42	6.083	1473	1475	1482	rVB2	356	302	0.03%	0.004%
43	6.128	1485	1489	1492	rBV	83	70	0.01%	0.001%
44	6.150	1492	1496	1497	rBV	332	226	0.02%	0.003%
45	6.189	1505	1508	1511	rBV2	340	252	0.03%	0.003%
46	6.208	1512	1514	1518	rVB	436	246	0.03%	0.003%
47	6.289	1521	1539	1560	rBV	340523	629992	64.59%	8.184%
48	6.462	1591	1593	1594	rBV	164	51	0.01%	0.001%
49	6.536	1614	1616	1617	rBV	141	74	0.01%	0.001%
50	6.568	1618	1626	1640	rVB4	2588	4297	0.44%	0.056%
51	6.623	1640	1643	1647	rVB	117	103	0.01%	0.001%
52	6.646	1647	1650	1654	rBV	126	116	0.01%	0.002%
53	6.732	1662	1677	1695	rBV	236675	452087	46.35%	5.873%
54	6.909	1730	1732	1737	rVB	182	95	0.01%	0.001%
55	6.964	1747	1749	1752	rVB	206	74	0.01%	0.001%
56	6.993	1752	1758	1759	rBV	93	86	0.01%	0.001%
57	7.067	1777	1781	1784	rVB2	175	108	0.01%	0.001%
58	7.086	1784	1787	1792	rBV	67	68	0.01%	0.001%
59	7.141	1800	1804	1807	rBV	101	95	0.01%	0.001%
60	7.189	1815	1819	1821	rBV	112	87	0.01%	0.001%
61	7.221	1823	1829	1839	rVB3	958	1163	0.12%	0.015%
62	7.273	1843	1845	1849	rVB	219	124	0.01%	0.002%
63	7.295	1849	1852	1854	rBV	72	53	0.01%	0.001%
64	7.398	1880	1884	1887	rBV	141	91	0.01%	0.001%
65	7.536	1924	1927	1931	rVB	96	59	0.01%	0.001%
66	7.601	1931	1947	1964	rBV	134261	232041	23.79%	3.014%
67	7.790	2001	2006	2010	rVV2	377	342	0.04%	0.004%
68	7.829	2011	2018	2028	rVB2	1105	1533	0.16%	0.020%
69	7.932	2036	2050	2069	rBV	451673	766451	78.59%	9.957%
70	8.211	2124	2137	2155	rBV	92751	156335	16.03%	2.031%
71	8.379	2185	2189	2191	rBV	84	68	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021020\
 Data File : VU036707.D
 Acq On : 10 Feb 2020 12:51
 Operator : JC/MD
 Sample : VU0210WBL07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

72	8.478	2218	2220	2221	rBV	113	47	0.00%	0.001%
73	8.501	2224	2227	2230	rVB2	276	171	0.02%	0.002%
74	8.584	2245	2253	2259	rVB6	2308	3224	0.33%	0.042%
75	8.668	2264	2279	2324	rBV	347924	611526	62.70%	7.944%
76	8.880	2342	2345	2346	rBV	160	74	0.01%	0.001%
77	8.919	2355	2357	2359	rBV	132	80	0.01%	0.001%
78	8.967	2366	2372	2375	rBV2	487	596	0.06%	0.008%
79	9.006	2383	2384	2387	rVB	230	73	0.01%	0.001%
80	9.108	2414	2416	2419	rVB	170	67	0.01%	0.001%
81	9.163	2430	2433	2437	rBV2	220	149	0.02%	0.002%
82	9.250	2458	2460	2462	rBV	82	54	0.01%	0.001%
83	9.359	2491	2494	2497	rBV	142	74	0.01%	0.001%
84	9.446	2507	2521	2554	rVB	467471	775041	79.47%	10.069%
85	9.584	2561	2564	2566	rBV	160	114	0.01%	0.001%
86	9.604	2566	2570	2575	rVV2	246	320	0.03%	0.004%
87	9.642	2580	2582	2586	rVV	180	74	0.01%	0.001%
88	9.726	2601	2608	2610	rBV2	490	443	0.05%	0.006%
89	9.742	2610	2613	2617	rVB	215	146	0.01%	0.002%
90	9.771	2619	2622	2627	rBV	170	98	0.01%	0.001%
91	10.124	2730	2732	2735	rBV2	205	103	0.01%	0.001%
92	10.288	2780	2783	2785	rVB	185	85	0.01%	0.001%
93	10.353	2800	2803	2807	rBV	291	210	0.02%	0.003%
94	10.449	2830	2833	2836	rBV	170	106	0.01%	0.001%
95	10.784	2924	2937	2954	rVB	315278	509601	52.25%	6.620%
96	11.385	3121	3124	3125	rBV	150	92	0.01%	0.001%
97	11.481	3152	3154	3156	rBV2	166	87	0.01%	0.001%
98	11.835	3251	3264	3281	rVB	425653	678769	69.60%	8.818%
99	12.214	3368	3382	3400	rBV	402305	652174	66.87%	8.472%
100	12.324	3414	3416	3423	rBV	270	265	0.03%	0.003%


Sum of corrected areas: 7697550

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU021020\
Data File : VU036707.D
Acq On : 10 Feb 2020 12:51
Operator : JC/MD
Sample : VU0210WBL07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

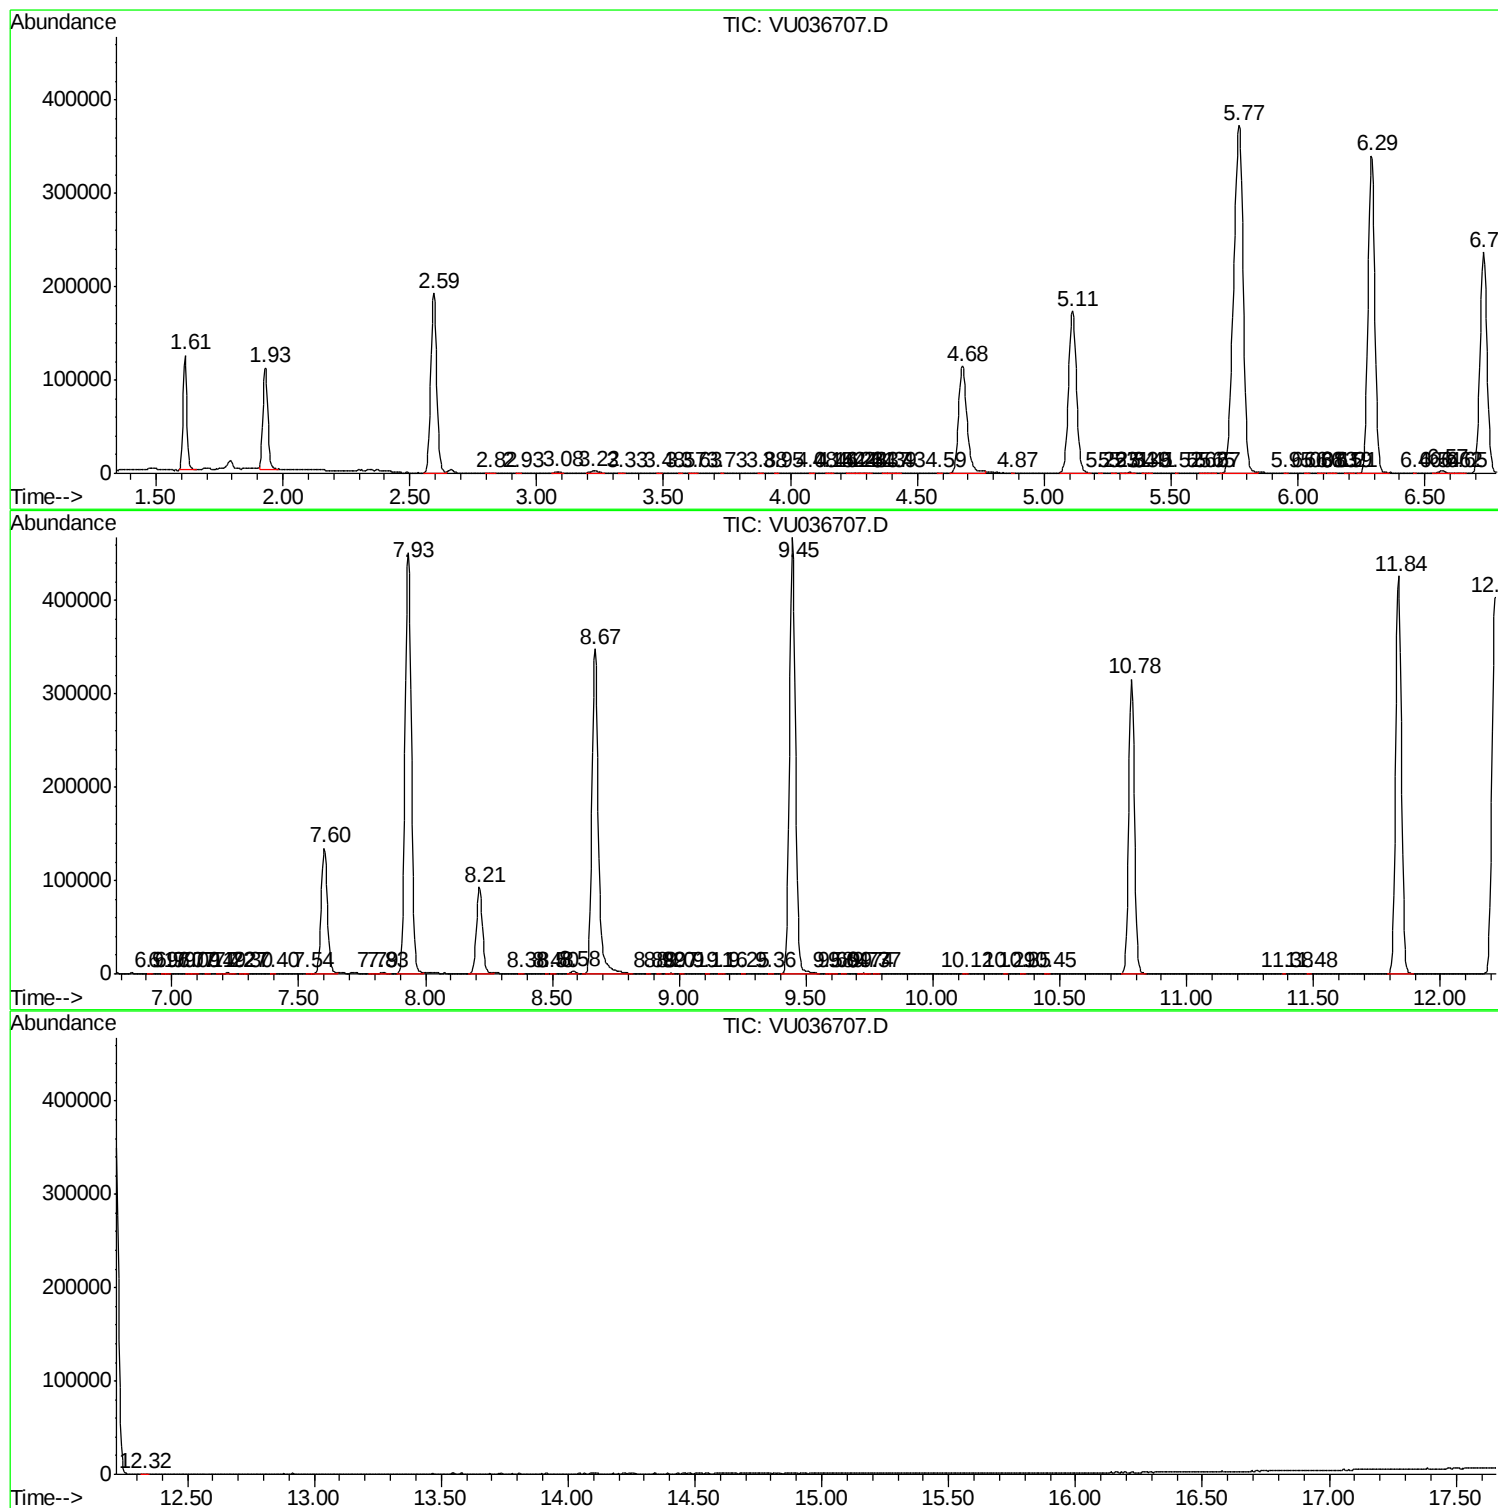

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU021020\
Data File : VU036707.D
Acq On : 10 Feb 2020 12:51
Operator : JC/MD
Sample : VU0210WBL07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU021020\
Data File : VU036707.D
Acq On : 10 Feb 2020 12:51
Operator : JC/MD
Sample : VU0210WBL07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc