


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021020\
 Data File : VU036701.D
 Acq On : 10 Feb 2020 09:34
 Operator : JC/MD
 Sample : BFB50
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB103

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis
 Last Update : Wed Feb 12 16:17:26 2020

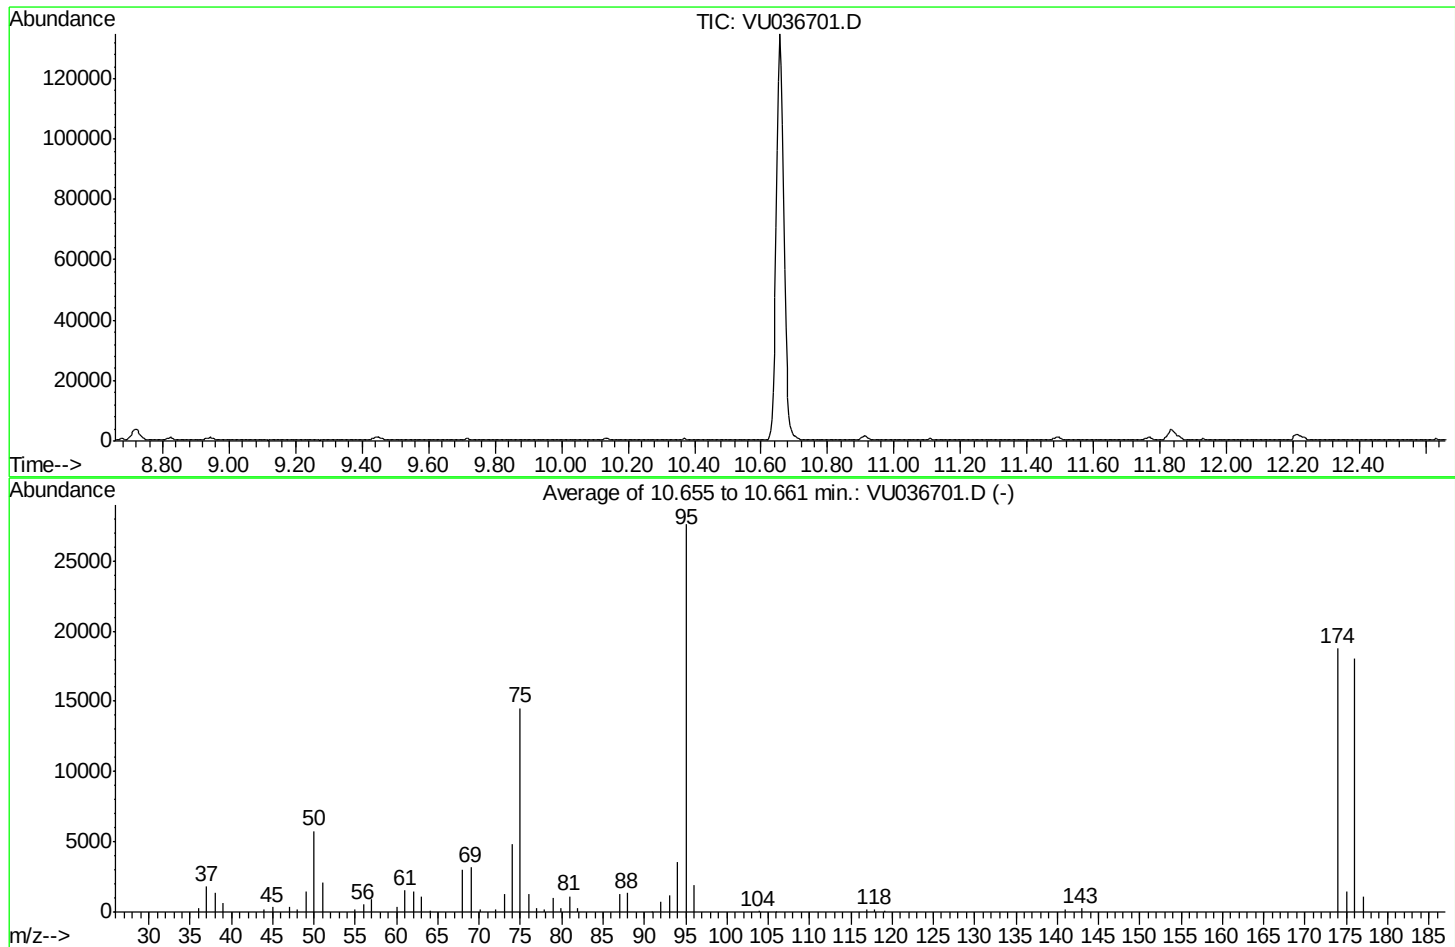

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	5767	PASS
75	95	30	80	52.5	14499	PASS
95	95	100	100	100.0	27602	PASS
96	95	5	9	7.0	1927	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.9	18744	PASS
175	174	5	9	8.0	1493	PASS
176	174	95	101	96.3	18045	PASS
177	176	5	9	6.2	1116	PASS

m/z	Abundance
35.00	275.0
37.00	1857.0
38.00	1443.0
39.00	723.0
43.00	570.0
45.00	342.0
47.00	412.0
48.00	217.0
49.00	1529.0
50.00	5920.0
51.00	2081.0
55.00	226.0
56.00	537.0
57.00	1056.0
60.00	356.0
61.00	1574.0
62.00	1482.0
63.00	1234.0
64.10	106.0
68.00	3121.0
69.00	3340.0
70.10	213.0
72.00	190.0
73.00	1289.0
74.00	5010.0
75.00	14973.0
76.10	1302.0
76.90	257.0
77.90	170.0
78.90	1027.0
79.90	316.0
80.90	1157.0
81.90	286.0
87.00	1219.0
88.00	1505.0
90.90	105.0
92.00	714.0
93.00	1181.0
94.00	3608.0
95.10	28064.0
96.00	2022.0
103.90	104.0
117.00	154.0
117.90	188.0
119.10	104.0
141.00	219.0
143.00	231.0
174.00	18616.0
175.00	1546.0
176.00	17808.0
177.00	1143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	268.0
37.00	1906.0
38.00	1427.0
39.00	648.0
44.00	606.0
45.00	330.0
47.00	401.0
48.00	202.0
49.00	1565.0
50.00	5925.0
51.00	2135.0
55.00	230.0
56.00	537.0
57.00	1007.0
60.00	341.0
61.00	1599.0
62.00	1489.0
63.00	1187.0
64.10	113.0
68.00	3073.0
69.00	3264.0
70.10	198.0
72.00	186.0
73.00	1301.0
74.00	5000.0
75.00	14908.0
76.00	1286.0
76.90	219.0
77.90	159.0
78.90	1012.0
79.90	302.0
81.00	1161.0
81.90	290.0
87.00	1301.0
87.90	1408.0
92.00	757.0
93.00	1247.0
94.00	3660.0
95.10	28504.0
96.00	1990.0
103.90	101.0
116.90	170.0
117.90	196.0
119.00	133.0
141.00	188.0
143.00	255.0
174.00	19352.0
175.00	1547.0
176.00	18544.0
177.00	1157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
36.00	268.0
37.00	1697.0
38.00	1319.0
38.90	564.0
44.00	629.0
45.00	298.0
47.00	313.0
47.90	178.0
49.00	1402.0
50.00	5458.0
51.00	1948.0
55.00	158.0
55.90	463.0
57.00	816.0
60.00	305.0
61.00	1448.0
62.00	1374.0
63.00	998.0
68.00	2797.0
69.00	2910.0
70.10	161.0
72.00	173.0
73.00	1236.0
74.00	4532.0
75.00	13618.0
76.00	1228.0
77.00	229.0
77.90	162.0
78.90	936.0
79.90	286.0
81.00	1074.0
81.90	286.0
87.00	1221.0
87.90	1187.0
92.00	719.0
93.00	1213.0
94.00	3290.0
95.10	26240.0
96.00	1771.0
105.90	105.0
116.90	155.0
117.90	152.0
119.00	137.0
140.90	169.0
142.90	231.0
174.00	18264.0
175.00	1387.0
176.00	17784.0
177.00	1049.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
43.90	391.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103