
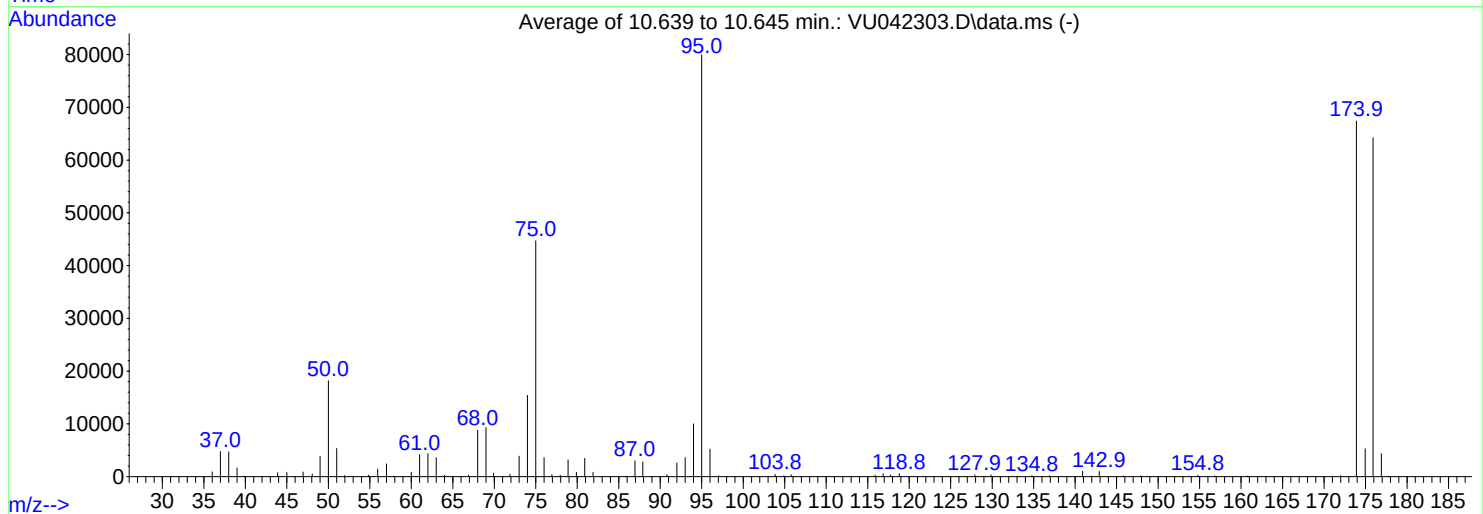


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021021\
 Data File : VU042303.D
 Acq On : 10 Feb 2021 08:46
 Operator : SY/MD
 Sample : BFB46
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB46

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR012021WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Feb 11 00:32:01 2021

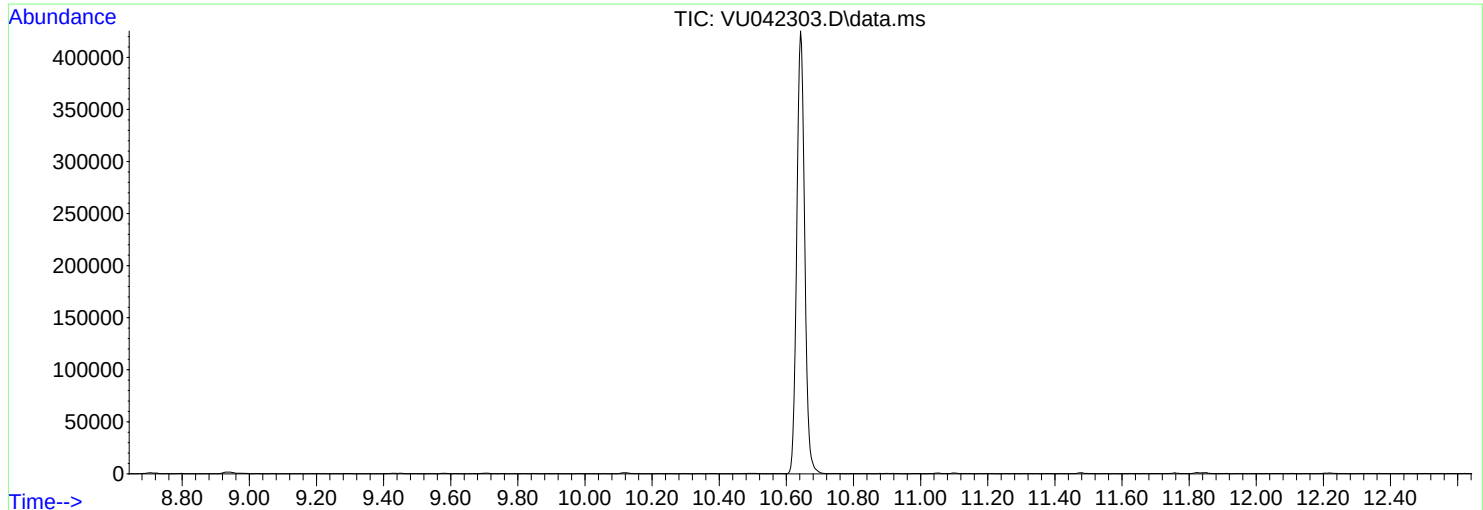

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	18152	PASS
75	95	30	80	55.9	44701	PASS
95	95	100	100	100.0	79949	PASS
96	95	5	9	6.5	5207	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.3	67403	PASS
175	174	5	9	7.8	5286	PASS
176	174	95	101	95.3	64245	PASS
177	176	5	9	6.8	4337	PASS

m/z	Abundance
36.00	888.0
37.00	4788.0
38.00	4644.0
39.00	1632.0
39.90	109.0
44.00	951.0
45.00	837.0
45.90	141.0
47.00	757.0
48.00	498.0
49.00	3816.0
50.00	17624.0
51.00	5188.0
52.00	218.0
54.90	300.0
55.90	1462.0
57.00	2260.0
57.90	147.0
60.00	840.0
61.00	4157.0
62.00	4268.0
63.00	3408.0
64.00	268.0
65.00	173.0
66.90	276.0
68.00	8733.0
69.00	9258.0
69.90	617.0
71.90	424.0
73.00	3865.0
74.00	15220.0
75.00	43712.0
76.00	3636.0
76.90	409.0
77.90	296.0
78.90	2982.0
79.90	850.0
80.90	3549.0
81.90	787.0
86.90	2953.0
87.90	2594.0
90.80	372.0
92.00	2525.0
93.00	3406.0
94.00	9400.0
95.00	78200.0
96.00	5197.0
97.00	128.0
103.80	413.0
104.90	137.0
105.80	396.0
115.90	256.0
116.90	502.0
117.80	353.0
118.80	511.0
127.90	321.0
129.00	100.0
129.80	302.0
134.80	176.0
136.90	167.0
140.90	942.0
142.00	146.0
142.90	963.0
145.80	108.0
147.90	146.0
154.80	285.0
156.80	127.0
160.70	104.0
173.90	64448.0
175.00	5125.0
175.90	61200.0
176.90	4190.0
177.80	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	924.0
37.00	4875.0
38.00	4863.0
39.00	1660.0
39.90	107.0
43.90	1010.0
45.00	857.0
45.90	130.0
46.90	914.0
48.10	505.0
49.00	3944.0
50.00	18760.0
51.00	5482.0
51.90	226.0
54.80	284.0
55.90	1432.0
57.00	2462.0
57.90	113.0
60.00	851.0
61.00	4275.0
62.00	4466.0
63.00	3733.0
64.00	289.0
65.00	128.0
66.90	281.0
68.00	9021.0
69.00	9518.0
69.90	691.0
71.90	451.0
73.00	3969.0
74.00	15917.0
75.00	46168.0
76.00	3731.0
77.00	393.0
77.90	284.0
78.90	3285.0
79.90	836.0
80.90	3549.0
81.90	856.0
85.80	114.0
86.90	3033.0
87.90	2904.0
90.80	401.0
92.00	2634.0
93.00	3727.0
94.00	10281.0
95.00	82544.0
96.00	5316.0
97.10	185.0
103.90	430.0
104.90	146.0
105.80	374.0
115.90	252.0
116.90	578.0
117.80	298.0
118.80	620.0
127.90	359.0
129.00	100.0
129.90	356.0
134.80	220.0
136.90	192.0
140.90	1012.0
141.90	138.0
142.90	1035.0
145.80	117.0
147.90	192.0
154.80	269.0
156.80	144.0
160.70	112.0
171.00	143.0
172.00	337.0
173.90	69464.0
174.90	5410.0
175.90	66056.0
176.90	4472.0
177.80	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	880.0
37.00	4586.0
38.00	4597.0
39.00	1613.0
39.80	106.0
43.90	920.0
45.00	808.0
47.00	940.0
48.00	476.0
49.00	3796.0
50.00	18072.0
51.00	5336.0
51.90	212.0
54.90	270.0
56.00	1346.0
57.00	2528.0
60.00	777.0
61.00	4115.0
62.00	4343.0
63.00	3592.0
64.00	292.0
66.90	246.0
68.00	8631.0
69.00	9108.0
69.90	714.0
71.90	445.0
73.00	3776.0
74.00	15131.0
75.00	44224.0
76.00	3482.0
77.00	414.0
78.00	263.0
78.90	3307.0
79.90	765.0
80.90	3311.0
81.90	781.0
85.90	132.0
87.00	2977.0
87.90	2906.0
90.80	403.0
92.00	2599.0
93.00	3713.0
94.00	10336.0
95.00	79104.0
96.00	5107.0
97.10	217.0
103.80	453.0
104.90	143.0
105.80	373.0
115.90	286.0
116.80	610.0
117.70	241.0
118.80	636.0
127.90	340.0
129.90	333.0
130.90	120.0
134.80	218.0
136.90	188.0
140.90	1025.0
141.90	125.0
142.90	997.0
145.80	112.0
147.90	226.0
154.80	250.0
156.80	149.0
160.80	108.0
171.00	159.0
172.00	355.0
173.90	68296.0
174.90	5324.0
175.90	65480.0
176.90	4348.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
43.80	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46