




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
 Data File : VU053036.D
 Acq On : 10 Feb 2023 14:28
 Operator : JC/MD
 Sample : 01422-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B79

Manual IntegrationsAPPROVED

Quant Time: Feb 10 23:31:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 10 23:20:41 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/13/2023
 Supervised By :Mahesh Dadoda 02/13/2023

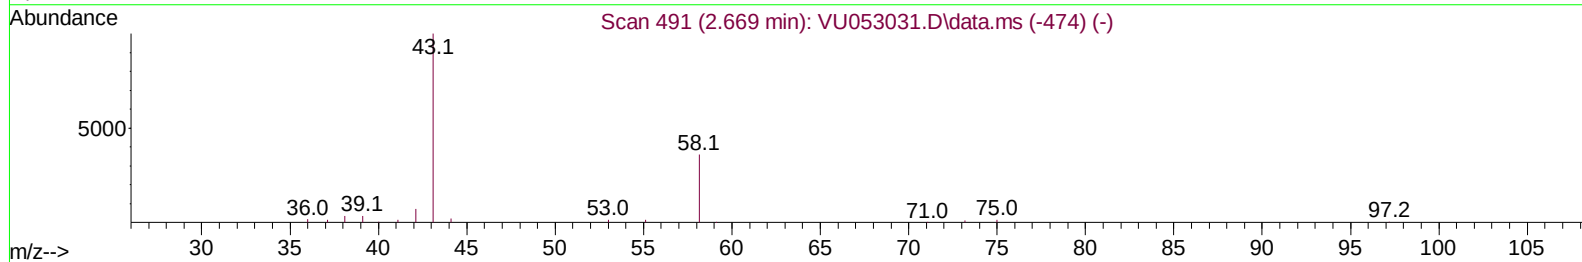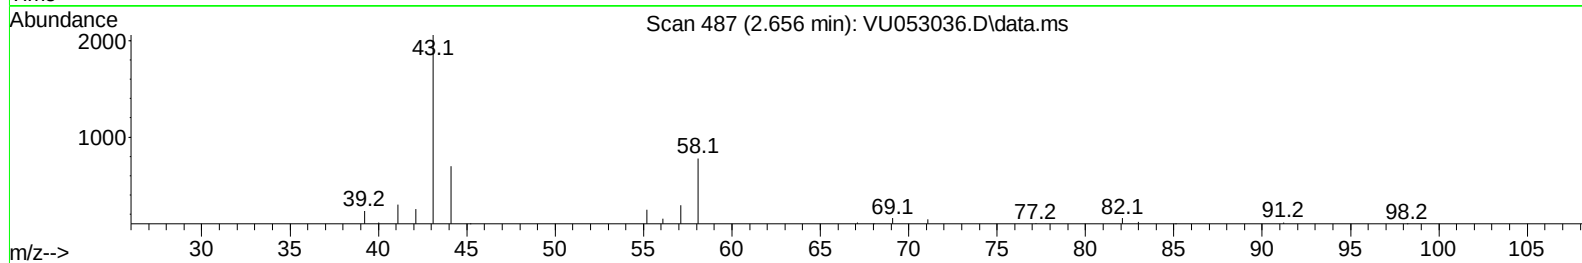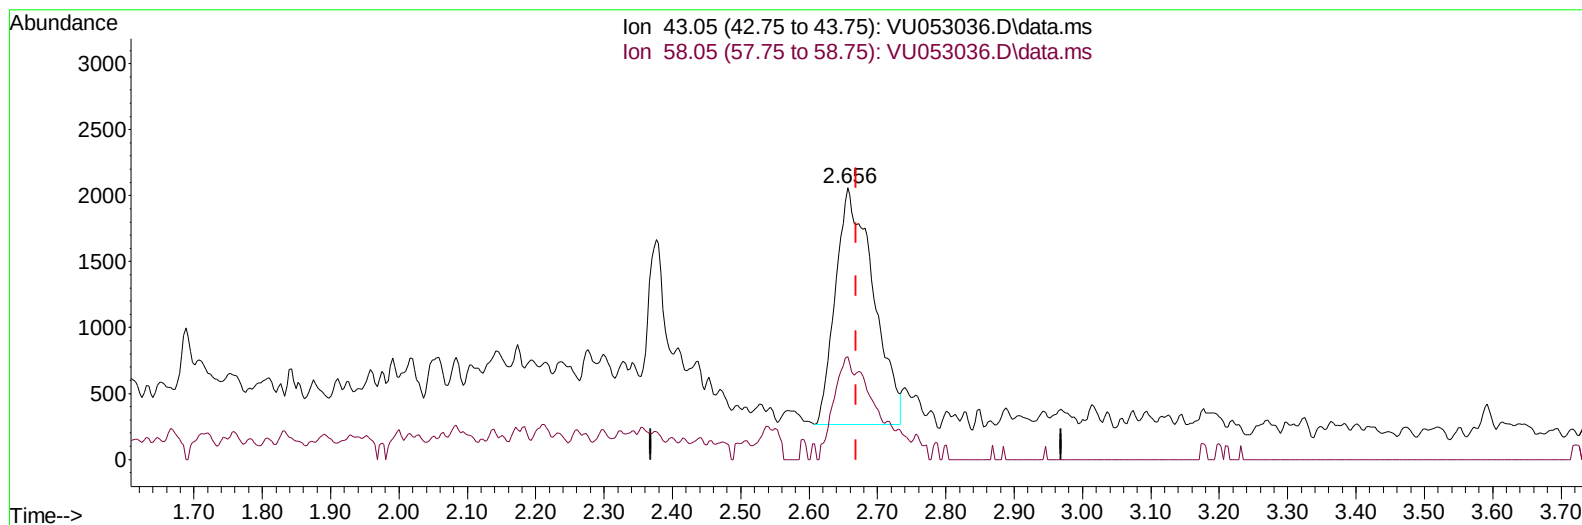

TIC: VU053036.D\data.ms

(13) Acetone (T)

2.656min (-0.013) 5.13 ug/L

response 6872

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.80	22.35#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
 Data File : VU053036.D
 Acq On : 10 Feb 2023 14:28
 Operator : JC/MD
 Sample : 01422-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B79

Manual IntegrationsAPPROVED

Quant Time: Feb 10 23:31:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 10 23:20:41 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/13/2023
 Supervised By :Mahesh Dadoda 02/13/2023

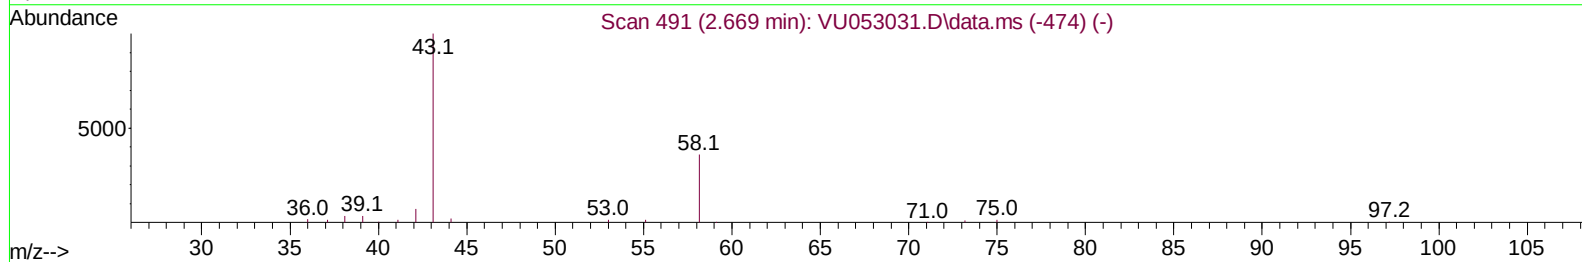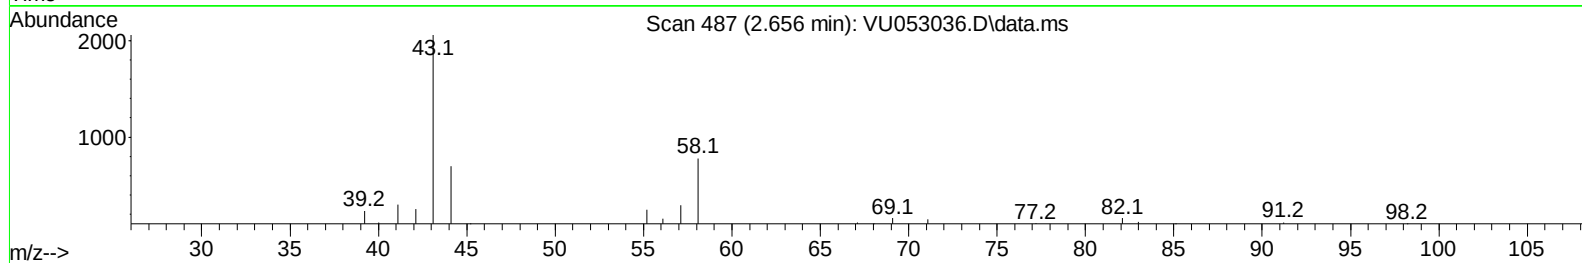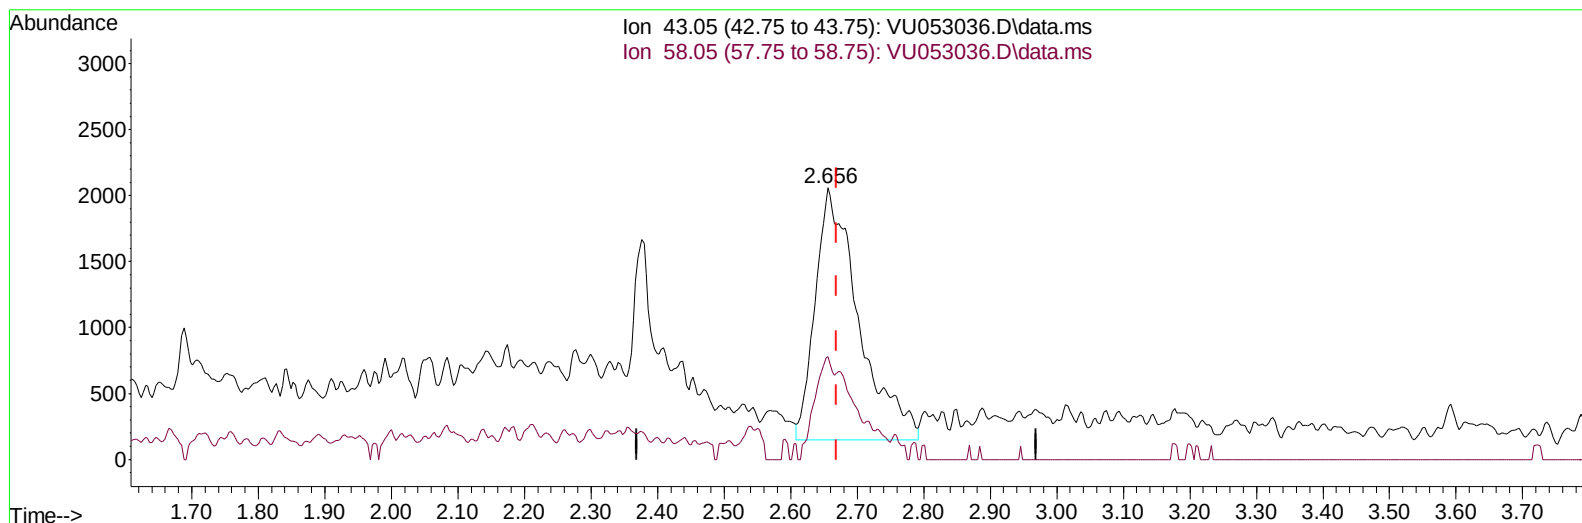

TIC: VU053036.D\data.ms

(13) Acetone (T)

2.656min (-0.013) 6.46 ug/L m

response 8661

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.80	17.73
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
 Data File : VU053036.D
 Acq On : 10 Feb 2023 14:28
 Operator : JC/MD
 Sample : 01422-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B79

Manual IntegrationsAPPROVED

Quant Time: Feb 10 23:31:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 10 23:20:41 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/13/2023
 Supervised By :Mahesh Dadoda 02/13/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.244	114		127295	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117		114188	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		52708	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.598	65		28921	4.743	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.800%	
7) Chloroethane-d5	1.913	69		28672	5.002	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.000%	
11) 1,1-Dichloroethene-d2	2.563	65		12859	4.597	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.000%	
20) 2-Butanone-d5	4.640	46		95586	51.179	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.360%	
24) Chloroform-d	5.058	84		65548	4.671	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	5.698	65		33519	4.740	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%	
32) Benzene-d6	5.724	84		122711	4.782	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.688	67		43920	4.914	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.200%	
41) Toluene-d8	7.894	98		108038	4.661	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%	
43) trans-1,3-Dichloroprop...	8.177	79		17919	4.953	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.000%	
46) 2-Hexanone-d5	8.630	63		80439	50.078	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.160%	
56) 1,1,2,2-Tetrachloroeth...	10.752	84		36765	4.790	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152		39396	5.003	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.000%	
Target Compounds							
13) Acetone	2.656	43		8661m	6.460	ug/L	
16) Methylene chloride	3.042	84		13872	1.592	ug/L	95
42) Toluene	7.965	91		6545	0.183	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
Data File : VU053036.D
Acq On : 10 Feb 2023 14:28
Operator : JC/MD
Sample : 01422-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B79

Manual IntegrationsAPPROVED

Quant Time: Feb 10 23:31:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 10 23:20:41 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 02/13/2023
Supervised By :Mahesh Dadoda 02/13/2023

