

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
 Data File : VU053046.D
 Acq On : 10 Feb 2023 18:25
 Operator : JC/MD
 Sample : 01422-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B80

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	41	52	66	rBV	125836	167515	39.78%	5.083%
2	1.518	119	133	134	rBV8	5185	7859	1.87%	0.238%
3	1.595	151	157	166	rBV	35640	40706	9.67%	1.235%
4	1.910	248	255	265	rBV	33810	43744	10.39%	1.327%
5	2.563	448	458	471	rVB	62058	101299	24.05%	3.074%
6	3.132	624	635	646	rBV4	6775	14309	3.40%	0.434%
7	4.650	1090	1107	1150	rBV	32079	159193	37.80%	4.831%
8	5.061	1220	1235	1257	rBV2	65882	149368	35.47%	4.533%
9	5.720	1419	1440	1466	rBV3	118861	320894	76.19%	9.738%
10	6.244	1590	1603	1626	rBV	147098	282068	66.98%	8.559%
11	6.688	1727	1741	1763	rVB	79358	159042	37.76%	4.826%
12	7.563	2000	2013	2026	rBV2	43154	75969	18.04%	2.305%
13	7.894	2103	2116	2135	rBV	145900	255576	60.69%	7.755%
14	8.177	2193	2204	2218	rBV2	26942	45966	10.91%	1.395%
15	8.550	2310	2320	2331	rVB2	33496	56276	13.36%	1.708%
16	8.633	2331	2346	2374	rBV3	197040	421150	100.00%	12.780%
17	9.415	2576	2589	2610	rBV	195932	326196	77.45%	9.898%
18	10.752	2991	3005	3018	rBV	70311	114393	27.16%	3.471%
19	11.807	3322	3333	3352	rBV	193616	307072	72.91%	9.318%
20	12.189	3440	3452	3472	rBV	145816	241309	57.30%	7.323%
21	14.549	4176	4186	4189	rBV7	3803	5527	1.31%	0.168%




Sum of corrected areas: 3295431

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
Data File : VU053046.D
Acq On : 10 Feb 2023 18:25
Operator : JC/MD
Sample : 01422-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

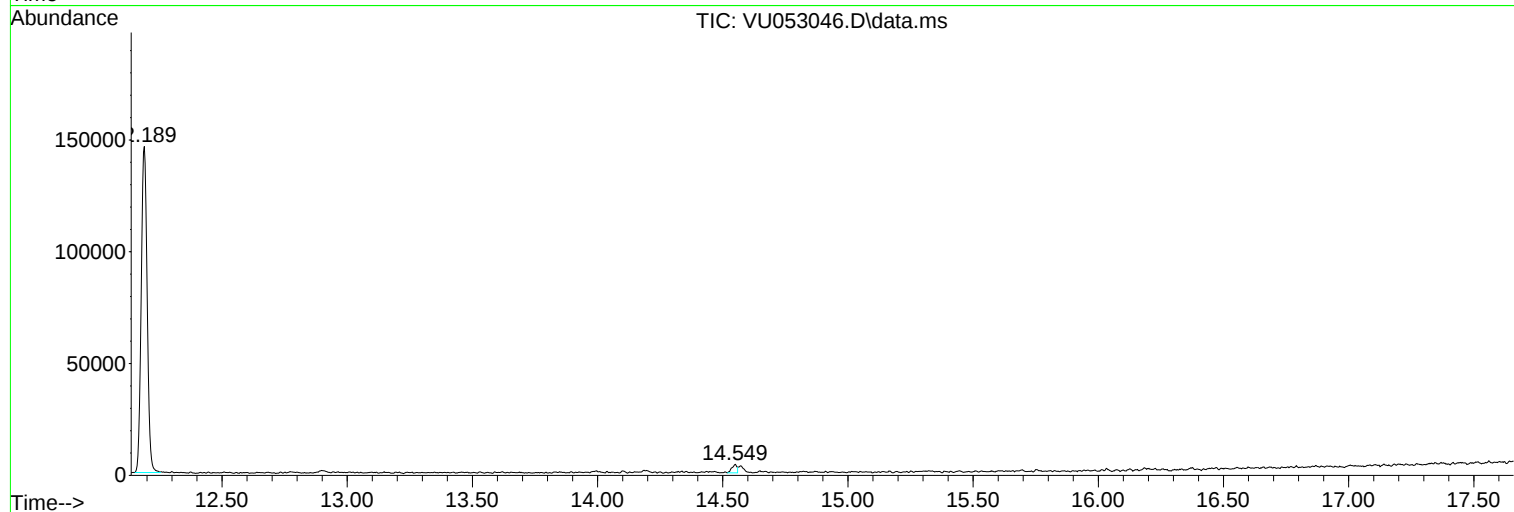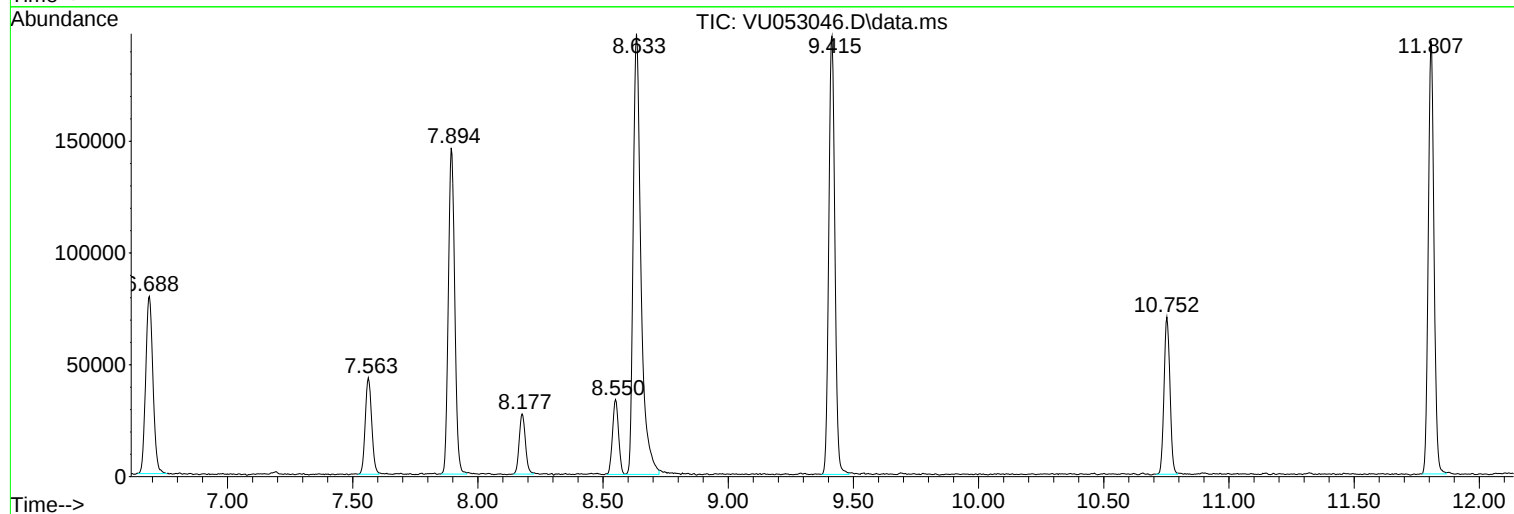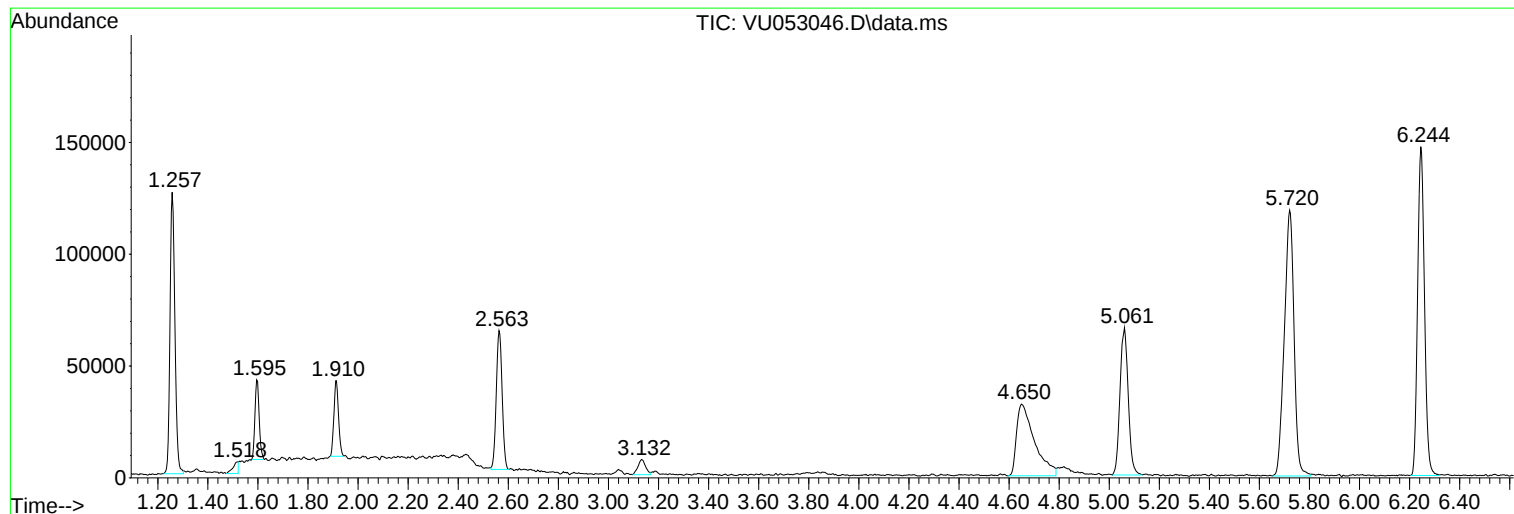

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
Data File : VU053046.D
Acq On : 10 Feb 2023 18:25
Operator : JC/MD
Sample : 01422-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
Data File : VU053046.D
Acq On : 10 Feb 2023 18:25
Operator : JC/MD
Sample : 01422-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------