

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
 Data File : VU053047.D
 Acq On : 10 Feb 2023 18:50
 Operator : JC/MD
 Sample : 01512-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B81

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	39	52	67	rBV	134905	178709	42.97%	5.442%
2	1.518	127	133	136	rBV6	4246	4955	1.19%	0.151%
3	1.595	151	157	168	rBV	34311	39836	9.58%	1.213%
4	1.910	248	255	271	rVB	35359	47821	11.50%	1.456%
5	2.563	448	458	471	rBV	61252	97835	23.52%	2.979%
6	3.129	627	634	646	rBV2	4495	7572	1.82%	0.231%
7	4.653	1091	1108	1149	rBV	31732	157796	37.94%	4.805%
8	5.058	1219	1234	1253	rBV2	66775	147609	35.49%	4.495%
9	5.720	1418	1440	1461	rBV2	122121	321807	77.37%	9.800%
10	6.244	1590	1603	1621	rBV	150373	284496	68.40%	8.664%
11	6.688	1727	1741	1759	rBV	79787	161798	38.90%	4.927%
12	7.563	1999	2013	2026	rBV	43708	78487	18.87%	2.390%
13	7.894	2099	2116	2133	rBV	146290	258995	62.27%	7.887%
14	8.177	2192	2204	2217	rBV	27141	45998	11.06%	1.401%
15	8.550	2307	2320	2331	rBV	29656	49888	11.99%	1.519%
16	8.633	2334	2346	2379	rBV3	196963	415934	100.00%	12.667%
17	9.415	2577	2589	2605	rBV	194878	325644	78.29%	9.917%
18	10.752	2994	3005	3016	rBV	70483	113497	27.29%	3.456%
19	11.807	3318	3333	3352	rBV	186148	303666	73.01%	9.248%
20	12.189	3440	3452	3464	rBV	145742	236647	56.90%	7.207%
21	14.549	4177	4186	4189	rBV6	3443	4728	1.14%	0.144%




Sum of corrected areas: 3283718

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
Data File : VU053047.D
Acq On : 10 Feb 2023 18:50
Operator : JC/MD
Sample : 01512-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

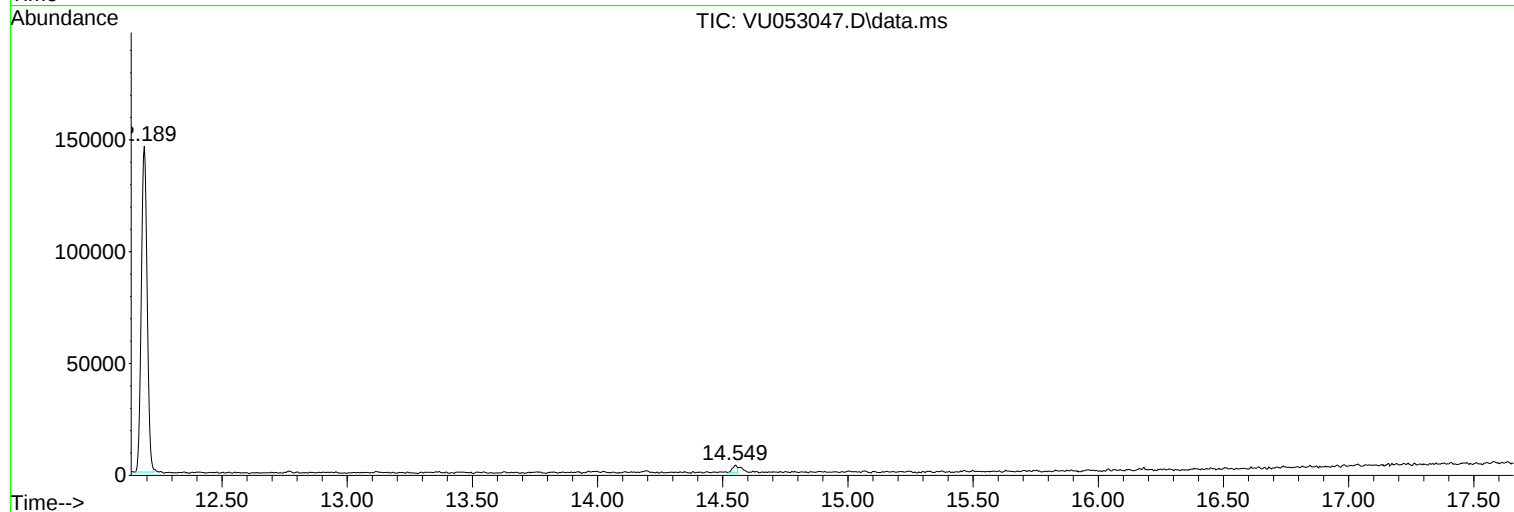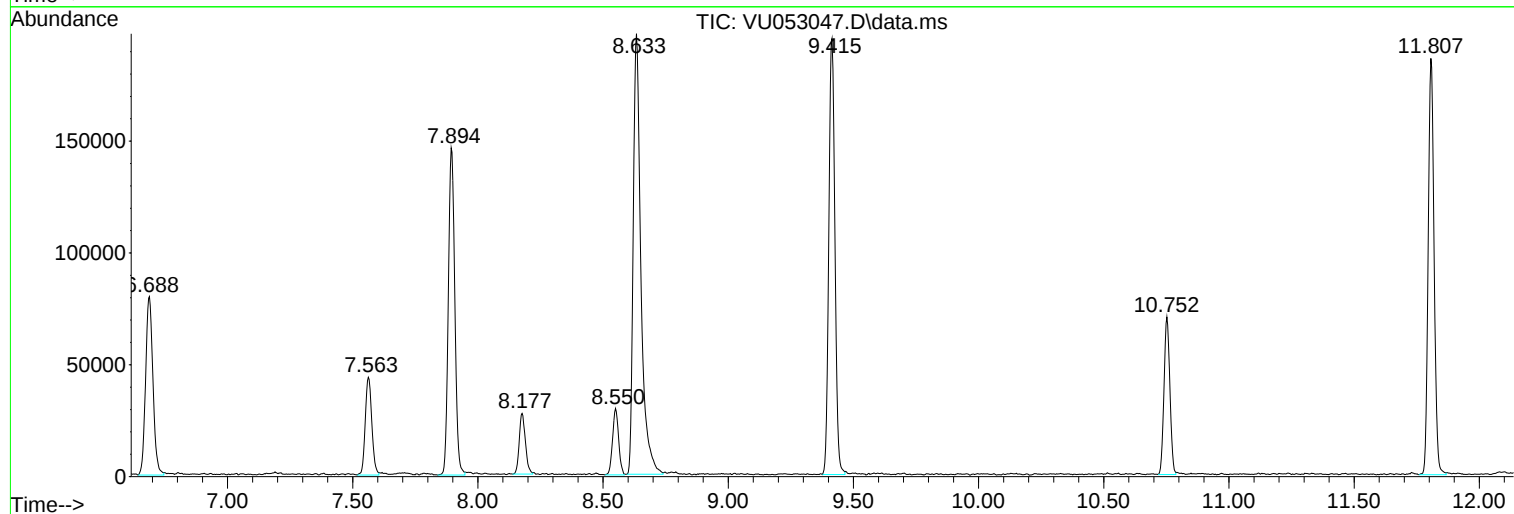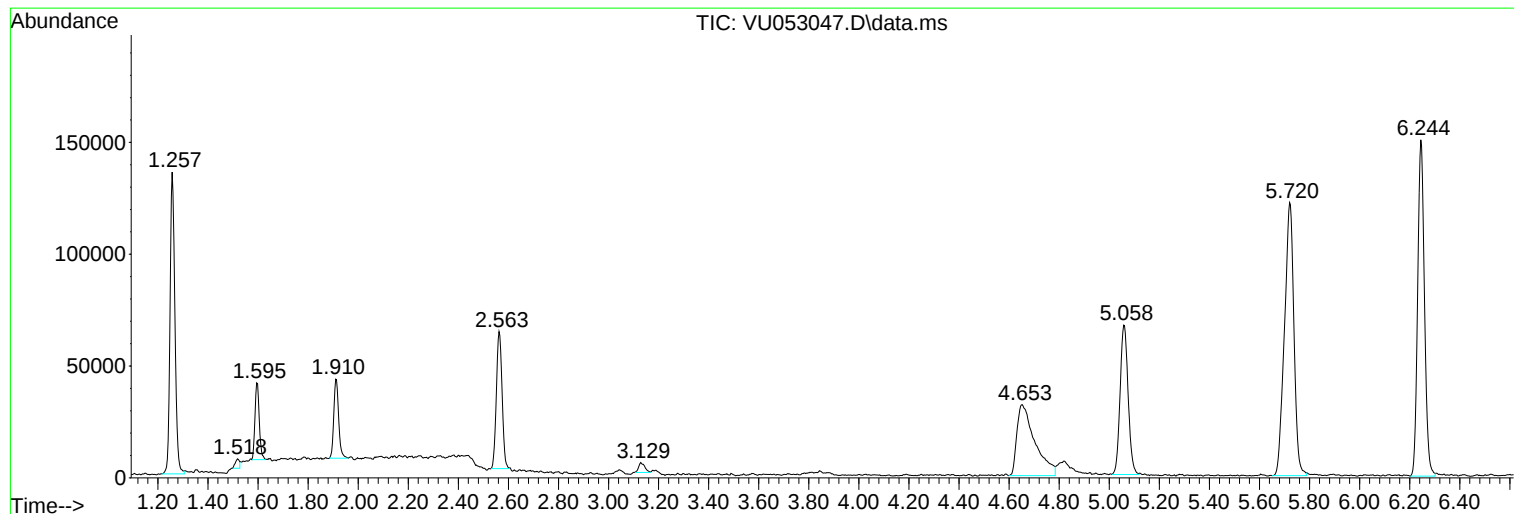

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
Data File : VU053047.D
Acq On : 10 Feb 2023 18:50
Operator : JC/MD
Sample : 01512-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
Data File : VU053047.D
Acq On : 10 Feb 2023 18:50
Operator : JC/MD
Sample : 01512-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc