


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021023\
Data File : VU053028.D
Acq On : 10 Feb 2023 09:18
Operator : JC/MD
Sample : BFB195
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB195

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sun Feb 12 22:49:21 2023

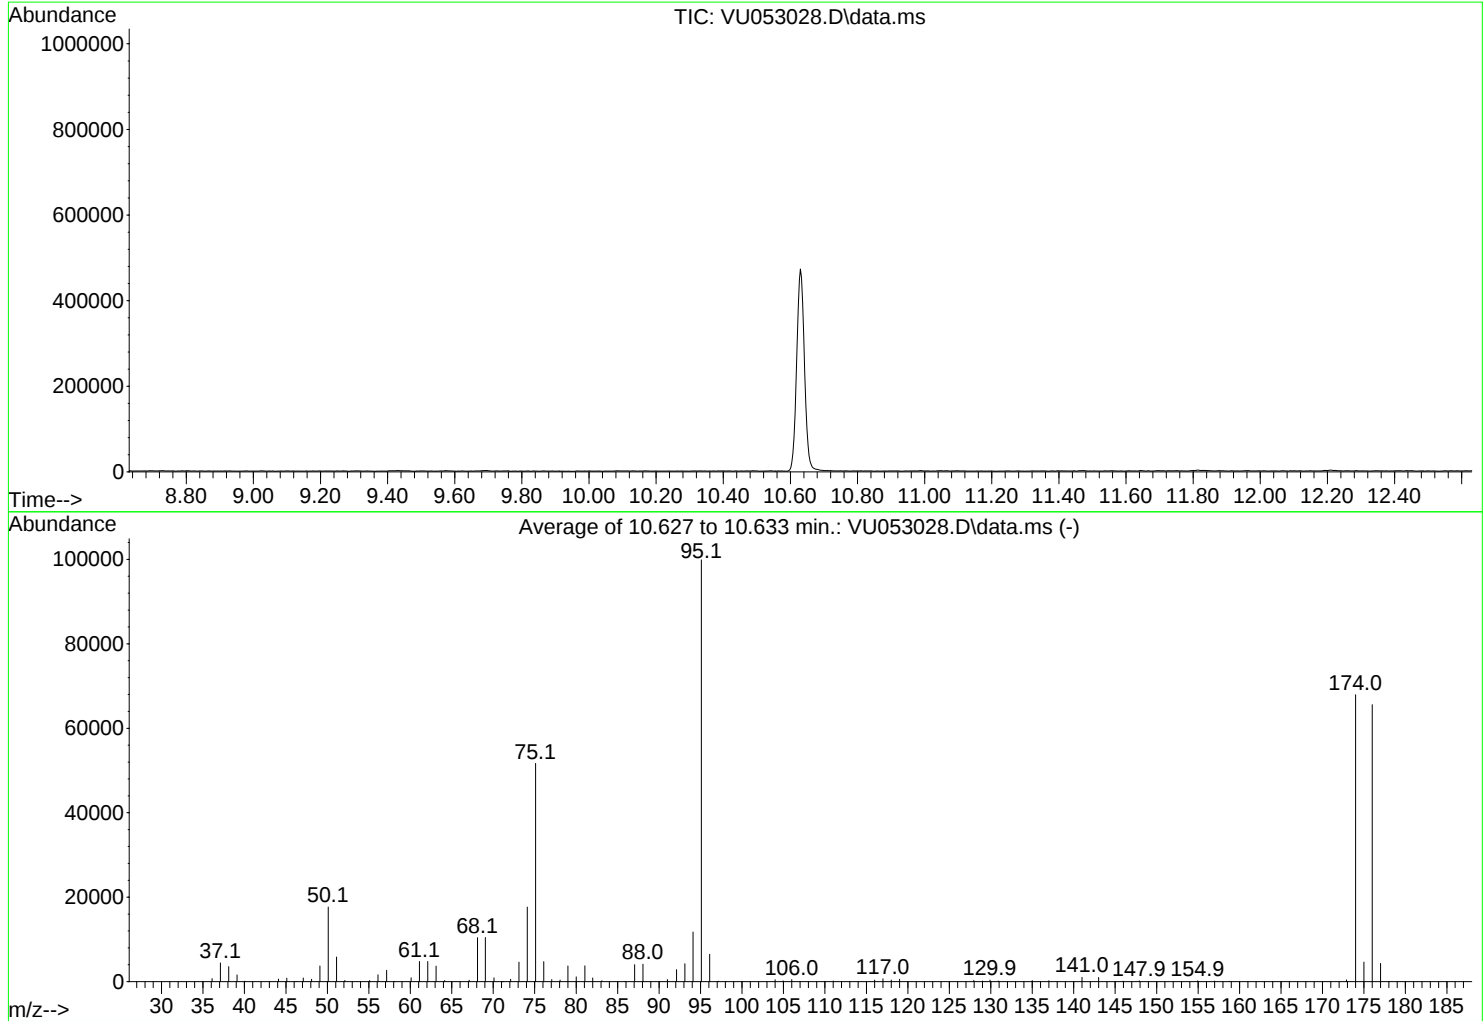

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2952

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	17640	PASS
75	95	30	80	51.7	51669	PASS
95	95	100	100	100.0	99888	PASS
96	95	5	9	6.5	6493	PASS
173	174	0.00	2	0.6	408	PASS
174	95	50	120	68.0	67952	PASS
175	174	5	9	6.8	4643	PASS
176	174	95	101	96.6	65608	PASS
177	176	5	9	6.6	4332	PASS

m/z	Abundance
41.10	214.0
43.10	282.0
44.10	376.0
55.10	277.0
57.20	230.0
58.20	107.0
68.10	111.0
69.00	121.0
71.10	194.0
97.20	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB195

m/z	Abundance
36.10	757.0
37.10	4334.0
38.10	3451.0
39.10	1610.0
40.10	121.0
41.10	197.0
43.10	338.0
44.10	984.0
45.10	829.0
46.20	124.0
47.10	867.0
48.10	548.0
49.10	3510.0
50.10	17472.0
51.10	5788.0
52.10	312.0
55.10	527.0
56.10	1676.0
57.10	2863.0
58.10	215.0
60.10	975.0
61.10	4490.0
62.10	4720.0
63.10	3661.0
64.10	275.0
67.10	337.0
68.10	10190.0
69.10	10373.0
70.10	909.0
71.10	192.0
72.10	561.0
73.10	4608.0
74.10	17304.0
75.10	51400.0
76.10	4739.0
77.00	516.0
78.10	400.0
79.00	3651.0
80.00	1039.0
81.10	3780.0
82.00	817.0
83.10	211.0
85.90	121.0
87.10	4059.0
88.10	4111.0
91.00	471.0
92.10	2782.0
93.10	4279.0
94.10	11482.0
95.10	98600.0
96.10	6442.0
97.20	246.0
98.10	113.0
104.00	464.0
105.00	165.0
106.00	453.0
107.00	108.0
110.00	115.0
111.00	167.0
113.00	127.0
115.00	112.0
116.00	374.0
117.00	686.0
118.00	373.0
119.00	592.0
127.90	334.0
129.00	168.0
129.90	358.0
130.90	184.0
135.00	244.0
137.00	219.0
141.00	899.0
143.00	1032.0
146.00	103.0
147.90	154.0
154.90	187.0
157.00	115.0
158.80	128.0
172.90	385.0
174.00	65488.0
175.00	4413.0
176.00	62672.0
177.00	4270.0
178.00	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB195

m/z	Abundance
36.10	755.0
37.10	4582.0
38.10	3662.0
39.10	1669.0
40.00	116.0
41.10	158.0
43.10	344.0
44.10	1025.0
45.10	823.0
47.10	854.0
48.10	610.0
49.10	3788.0
50.10	18224.0
51.10	6067.0
52.10	311.0
55.10	568.0
56.10	1650.0
57.10	2987.0
58.00	205.0
60.10	946.0
61.10	4916.0
62.10	4911.0
63.10	3812.0
64.20	273.0
67.10	345.0
68.10	10847.0
69.10	10952.0
70.10	942.0
71.10	211.0
72.10	580.0
73.10	4830.0
74.10	18392.0
75.10	53248.0
76.10	4912.0
77.00	463.0
78.00	390.0
79.00	3814.0
80.00	1215.0
81.00	3881.0
82.00	897.0
83.10	236.0
85.90	103.0
87.10	4140.0
88.10	4243.0
91.00	524.0
92.10	2950.0
93.10	4388.0
94.10	12193.0
95.10	103376.0
96.10	6632.0
97.20	272.0
104.00	466.0
104.90	177.0
106.00	489.0
107.00	100.0
110.00	111.0
111.00	156.0
112.90	102.0
115.00	111.0
116.00	416.0
117.00	722.0
118.00	374.0
119.00	601.0
127.90	329.0
129.00	176.0
129.90	390.0
130.90	164.0
135.00	277.0
137.00	241.0
141.00	1067.0
143.00	1007.0
145.90	114.0
147.90	175.0
155.00	202.0
156.90	146.0
158.80	121.0
172.90	419.0
174.00	70088.0
175.00	4803.0
176.00	67624.0
177.00	4463.0
178.00	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB195

m/z	Abundance
36.10	715.0
37.10	4336.0
38.10	3571.0
39.10	1508.0
40.00	110.0
41.10	165.0
43.10	331.0
44.10	993.0
45.10	798.0
47.10	886.0
48.10	577.0
49.10	3894.0
50.10	17224.0
51.10	5694.0
52.10	327.0
55.10	545.0
56.10	1523.0
57.20	2873.0
58.10	184.0
60.10	861.0
61.10	4912.0
62.10	4675.0
63.10	3522.0
64.10	259.0
67.10	314.0
68.10	10542.0
69.10	10430.0
70.10	860.0
71.10	233.0
72.10	561.0
73.10	4489.0
74.10	17264.0
75.10	50360.0
76.10	4606.0
77.10	448.0
78.00	382.0
79.00	3627.0
80.00	1201.0
81.00	3647.0
82.00	907.0
83.10	258.0
87.00	3911.0
88.00	4054.0
91.00	501.0
92.10	2772.0
93.10	4018.0
94.10	11572.0
95.10	97688.0
96.10	6404.0
97.10	295.0
104.00	412.0
104.90	175.0
106.00	492.0
111.00	113.0
116.00	373.0
117.00	676.0
118.00	373.0
119.00	528.0
128.00	299.0
129.00	158.0
129.90	384.0
130.90	124.0
135.00	259.0
137.00	200.0
141.00	1132.0
143.00	924.0
145.90	136.0
147.90	195.0
153.00	105.0
155.00	207.0
156.90	174.0
172.90	419.0
174.00	68280.0
175.00	4713.0
176.00	66528.0
177.00	4263.0

Instrument :
MSVOA_U
ClientSampleId :
BFB195