

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021119\
 Data File : VU029398.D
 Acq On : 11 Feb 2019 15:34
 Operator : JC/SP
 Sample : K1387-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JJ7

Quant Time: Feb 12 02:07:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Feb 12 01:17:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	241600	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	223778	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	119531	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	75733	4.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.60%
7) Chloroethane-d5	1.68	69	61704	4.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.00%
11) 1,1-Dichloroethene-d2	2.27	63	118502	3.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.20%
20) 2-Butanone-d5	4.19	46	146327	45.56	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.12%
24) Chloroform-d	4.65	84	119503	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	5.31	65	60228	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
32) Benzene-d6	5.34	84	249625	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
36) 1,2-Dichloropropane-d6	6.33	67	72450	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.60%
41) Toluene-d8	7.56	98	243714	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.60%
43) trans-1,3-Dichloropropene-	7.85	79	33147	4.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.40%
46) 2-Hexanone-d5	8.31	63	146624	45.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.40%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	59440	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	99797	4.57	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.40%


Target Compounds					Ovalue
13) Acetone	2.32	43	4370	1.700 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU021119\
Data File : VU029398.D
Acq On : 11 Feb 2019 15:34
Operator : JC/SP
Sample : K1387-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JJ7

Quant Time: Feb 12 02:07:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Feb 12 01:17:05 2019
Response via : Initial Calibration

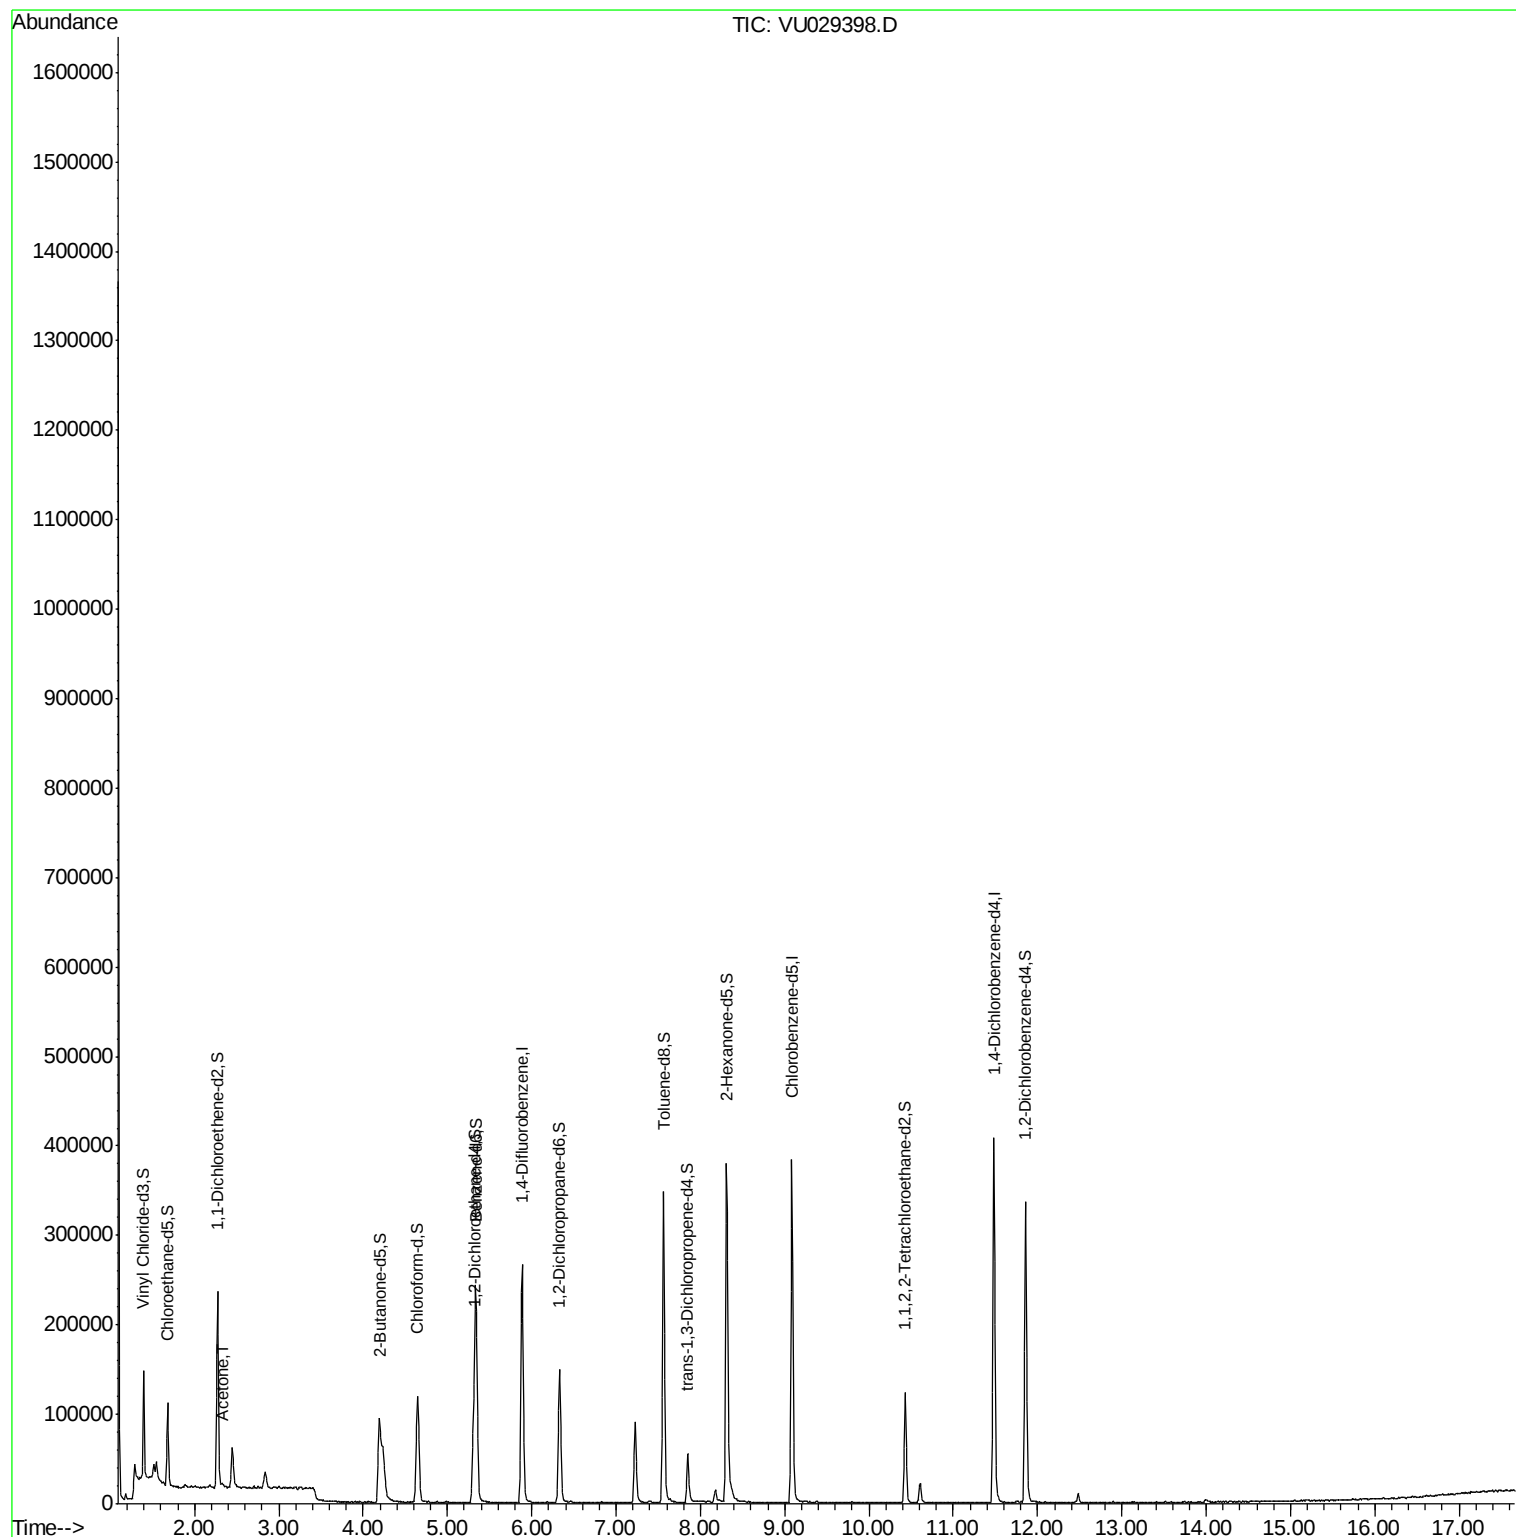

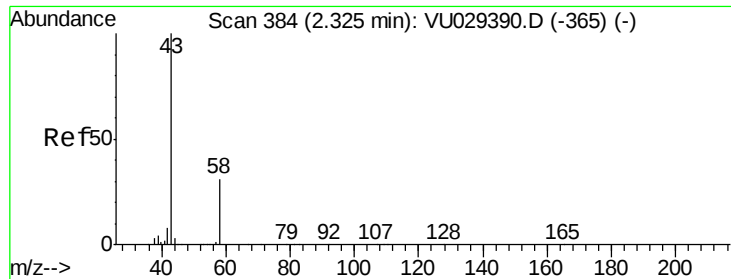

#13

Acetone

Concen: 1.700 ug/L

RT: 2.32 min Scan# 384

Delta R.T. 0.00 min

Lab File: VU029398.D

Acq: 11 Feb 2019 15:34

Instrument :

MSVOA_U

ClientSampleId :

C0JJ7

Tot Ion: 43 Resp: 4370

Ion Ratio Lower Upper

43 100

58 37.8 0.0 64.2

