


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021119\
 Data File : VU029387.D
 Acq On : 11 Feb 2019 09:41
 Operator : JC/SP
 Sample : BFB44
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Feb 12 01:17:05 2019

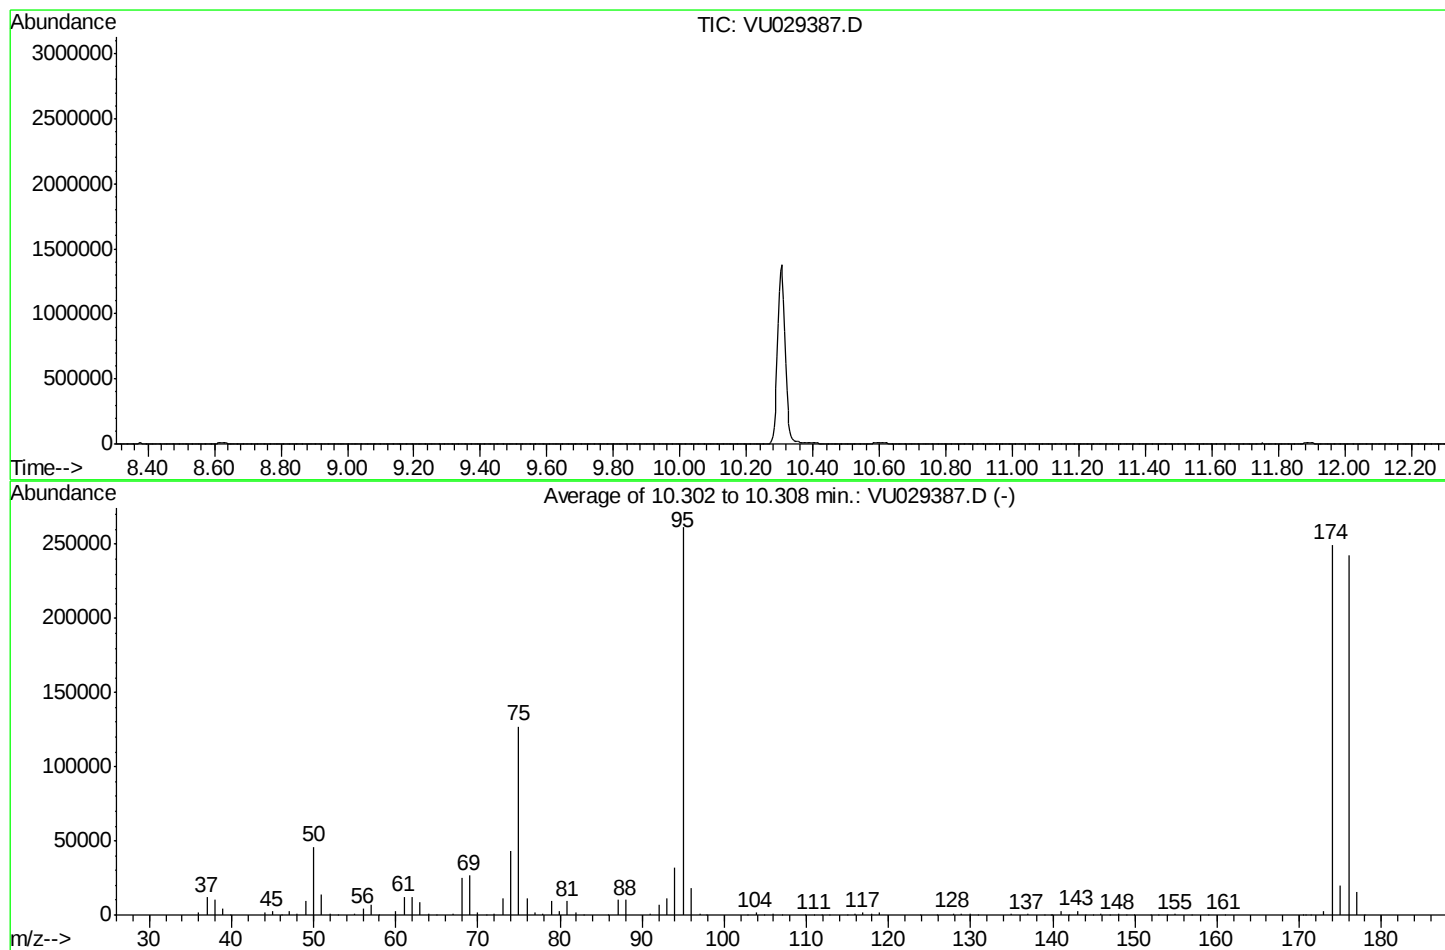

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	45944	PASS
75	95	30	80	48.6	126973	PASS
95	95	100	100	100.0	261461	PASS
96	95	5	9	6.8	17853	PASS
173	174	0.00	2	1.0	2447	PASS
174	95	50	120	95.6	249834	PASS
175	174	5	9	7.9	19621	PASS
176	174	95	101	97.3	242986	PASS
177	176	5	9	6.4	15479	PASS

Scan 2851 (10.257 min): VU029387.D
BFB44

m/z	Abundance
39.10	136.0
39.90	168.0
41.00	245.0
41.90	114.0
43.10	350.0
44.00	582.0
55.00	208.0
56.00	106.0
206.90	196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	2039.0
37.00	12141.0
38.00	10772.0
39.00	4299.0
39.90	338.0
41.00	152.0
43.00	250.0
44.00	2126.0
45.00	2389.0
46.10	224.0
47.10	2289.0
48.00	1342.0
49.00	10067.0
50.00	46776.0
51.00	14533.0
52.00	686.0
55.00	827.0
56.00	4291.0
57.00	7123.0
58.00	314.0
60.00	2170.0
61.00	12482.0
62.00	12027.0
63.00	9099.0
64.00	757.0
65.00	158.0
67.00	745.0
68.00	25312.0
69.00	26608.0
70.00	2138.0
71.10	152.0
72.00	1355.0
73.00	11472.0
74.00	43264.0
75.00	128024.0
76.00	10823.0
76.90	1332.0
78.00	975.0
78.90	9128.0
79.90	2603.0
80.90	9240.0
82.00	2067.0
82.90	360.0
85.80	299.0
87.00	10810.0
88.00	10420.0
91.00	1015.0
92.00	7374.0
93.00	11117.0
94.00	32160.0
95.00	262400.0
96.00	18048.0
97.00	490.0
97.90	116.0
102.80	185.0
103.90	1409.0
104.80	402.0
105.90	1352.0
107.00	256.0
109.90	192.0
111.00	253.0
111.80	188.0
112.90	270.0
114.90	324.0
115.90	1088.0
116.90	1704.0
117.90	1049.0
118.90	1474.0
123.90	136.0
125.90	106.0
127.80	1033.0
128.90	469.0
129.90	1004.0
130.90	331.0
134.90	467.0
136.90	589.0
138.90	130.0
139.90	205.0
141.00	2541.0
141.90	322.0
143.00	2811.0
144.00	160.0
144.90	270.0
145.90	506.0
146.90	140.0
148.00	661.0
148.90	191.0
149.80	213.0
152.00	142.0
152.90	183.0
153.80	134.0
154.90	573.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

157.00	421.0
158.90	331.0
160.90	317.0
170.40	140.0
170.80	122.0
171.30	180.0
173.00	2328.0
174.00	242752.0
175.00	19688.0
176.00	236032.0
177.00	15681.0
177.90	329.0
207.10	175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	2229.0
37.00	12163.0
38.00	11036.0
39.00	4404.0
39.90	328.0
41.10	183.0
43.00	261.0
44.00	2090.0
45.00	2339.0
46.10	215.0
47.10	2411.0
48.00	1373.0
49.00	10085.0
50.00	47376.0
51.00	14628.0
52.00	611.0
53.00	108.0
55.00	809.0
56.00	4294.0
57.00	7446.0
58.00	312.0
60.00	2351.0
61.00	12839.0
62.00	12310.0
63.00	9237.0
64.00	732.0
65.00	149.0
67.00	724.0
68.00	25792.0
69.00	27376.0
70.00	2107.0
71.10	134.0
72.00	1296.0
73.00	11541.0
74.00	44616.0
75.00	131136.0
76.00	11417.0
77.00	1393.0
77.90	969.0
78.90	9583.0
79.90	2614.0
80.90	9626.0
82.00	2189.0
82.90	392.0
85.80	282.0
87.00	10312.0
88.00	10700.0
90.90	1039.0
92.00	7454.0
93.00	11198.0
94.00	32976.0
95.00	269696.0
96.00	18368.0
97.00	539.0
102.90	182.0
103.90	1403.0
104.90	412.0
105.90	1277.0
106.90	271.0
109.90	171.0
110.90	292.0
111.80	181.0
112.90	264.0
114.90	283.0
115.90	1134.0
116.90	1668.0
117.90	1051.0
118.90	1537.0
123.80	151.0
125.90	109.0
127.90	1122.0
128.90	546.0
129.90	1121.0
130.90	319.0
134.90	518.0
136.90	640.0
138.90	122.0
140.00	198.0
141.00	2874.0
142.00	284.0
142.90	3026.0
143.90	153.0
145.00	253.0
145.90	536.0
146.90	151.0
148.00	752.0
148.90	189.0
149.90	189.0
152.00	152.0
152.90	235.0
153.80	158.0
154.90	636.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

156.90	406.0
158.90	340.0
160.90	362.0
170.40	163.0
173.00	2525.0
174.00	258176.0
175.00	20296.0
176.00	250688.0
177.00	15966.0
177.90	365.0
206.90	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	2081.0
37.00	10949.0
38.00	10122.0
39.00	3948.0
39.90	300.0
41.10	218.0
43.10	287.0
44.00	1934.0
45.00	2074.0
46.10	165.0
47.00	2181.0
48.00	1253.0
49.00	9205.0
50.00	43680.0
51.00	13204.0
52.00	552.0
53.00	101.0
55.00	755.0
56.00	3715.0
57.00	6923.0
57.90	285.0
60.00	2247.0
61.00	11695.0
62.00	11180.0
63.00	8700.0
64.00	690.0
67.00	675.0
68.00	23984.0
69.00	25376.0
70.00	1948.0
72.00	1147.0
73.00	10710.0
74.00	41856.0
75.00	121760.0
76.00	10736.0
77.00	1287.0
77.90	914.0
78.90	8872.0
79.90	2346.0
80.90	8991.0
81.90	2153.0
82.90	345.0
85.90	234.0
87.00	9113.0
88.00	9624.0
90.90	1031.0
92.00	6863.0
93.00	10306.0
94.00	30464.0
95.00	252288.0
96.00	17144.0
97.00	545.0
102.90	153.0
103.90	1238.0
104.90	389.0
105.90	1141.0
106.90	308.0
109.90	135.0
110.90	342.0
111.90	165.0
112.80	244.0
114.90	236.0
115.80	1143.0
116.90	1505.0
117.90	978.0
118.90	1380.0
123.80	173.0
125.90	125.0
127.90	1085.0
128.90	536.0
129.90	1099.0
130.80	297.0
134.90	541.0
136.90	613.0
139.70	163.0
141.00	2897.0
142.00	258.0
142.90	2933.0
143.90	123.0
144.90	177.0
145.90	504.0
146.90	165.0
148.00	740.0
148.90	196.0
149.90	184.0
151.90	157.0
152.90	259.0
153.90	190.0
154.90	650.0
156.80	420.0
158.90	304.0
160.90	365.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

170.50	123.0
173.00	2490.0
174.00	248576.0
175.00	18880.0
176.00	242240.0
177.00	14790.0
177.90	376.0
206.90	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44