


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021120\
 Data File : VU036714.D
 Acq On : 11 Feb 2020 09:15
 Operator : JC/MD
 Sample : BFB51
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB104

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis
 Last Update : Wed Feb 12 02:32:22 2020

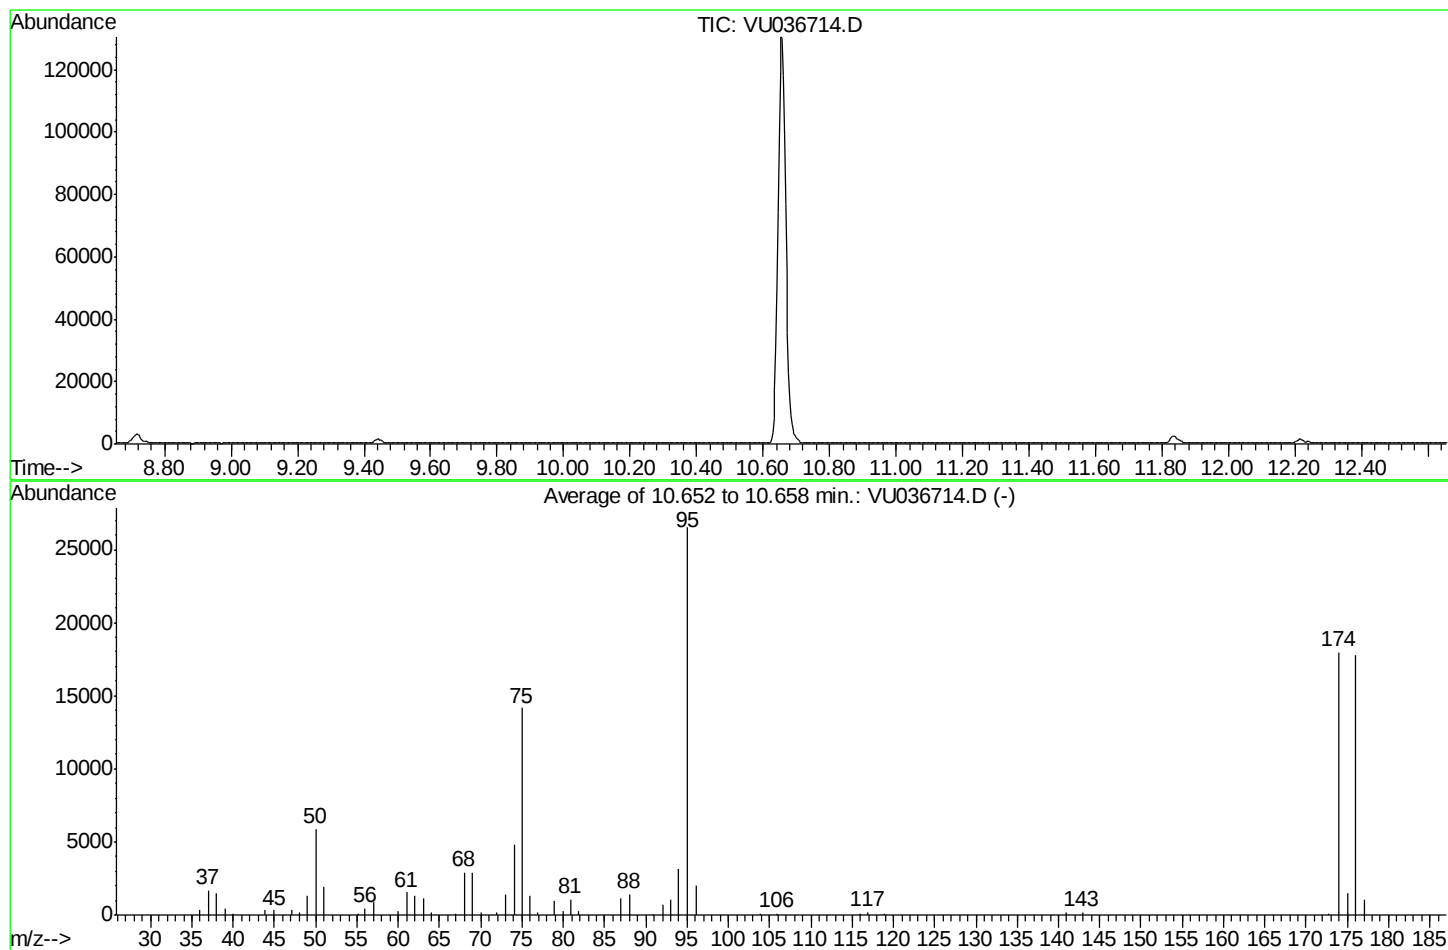

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	5910	PASS
75	95	30	80	53.4	14163	PASS
95	95	100	100	100.0	26520	PASS
96	95	5	9	7.6	2004	PASS
173	174	0.00	2	0.4	78	PASS
174	95	50	120	67.8	17978	PASS
175	174	5	9	8.5	1533	PASS
176	174	95	101	98.7	17738	PASS
177	176	5	9	5.9	1047	PASS

m/z	Abundance
35.90	381.0
37.00	1576.0
38.00	1441.0
39.00	468.0
40.00	115.0
43.90	522.0
45.00	336.0
47.10	316.0
48.10	174.0
49.00	1224.0
50.00	5556.0
51.00	1839.0
55.10	106.0
56.00	439.0
57.00	897.0
60.00	291.0
61.00	1535.0
62.00	1268.0
63.00	1126.0
63.90	159.0
66.90	102.0
68.00	2777.0
69.00	2810.0
70.00	146.0
71.90	200.0
73.10	1358.0
74.10	4460.0
75.00	13481.0
76.00	1230.0
76.90	183.0
78.90	879.0
79.90	317.0
80.90	992.0
81.90	272.0
87.00	1135.0
88.00	1330.0
92.00	658.0
93.00	1050.0
94.00	2967.0
95.10	25184.0
96.00	2050.0
105.90	102.0
116.90	184.0
118.90	125.0
141.00	186.0
142.90	200.0
174.00	16576.0
175.10	1453.0
176.00	16416.0
177.00	1044.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
44.00	261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	308.0
37.00	1720.0
38.00	1476.0
39.00	431.0
39.90	101.0
43.90	639.0
45.00	350.0
47.00	302.0
47.90	189.0
49.00	1315.0
50.00	6011.0
51.00	1891.0
55.10	118.0
56.00	488.0
57.00	853.0
60.00	295.0
61.00	1498.0
62.00	1364.0
63.00	1164.0
64.00	159.0
67.00	121.0
68.00	2995.0
69.00	2931.0
70.00	204.0
71.90	163.0
73.00	1301.0
74.10	4971.0
75.00	14414.0
76.00	1365.0
77.00	212.0
78.90	952.0
79.90	299.0
80.90	1096.0
81.90	256.0
86.90	1117.0
88.00	1479.0
90.90	114.0
92.00	718.0
93.00	1069.0
94.00	3223.0
95.00	27104.0
96.10	1924.0
103.90	104.0
105.90	127.0
115.90	104.0
116.90	178.0
118.90	109.0
141.00	176.0
143.00	198.0
172.80	234.0
174.00	18848.0
175.10	1576.0
176.00	18512.0
177.00	1015.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	364.0
37.00	1702.0
38.00	1529.0
39.00	468.0
39.90	106.0
43.90	571.0
45.00	366.0
47.10	320.0
48.00	185.0
49.00	1297.0
50.00	6165.0
51.00	2004.0
55.10	116.0
56.00	485.0
57.00	889.0
60.00	312.0
61.00	1621.0
62.00	1369.0
63.00	1194.0
64.00	158.0
66.90	135.0
68.00	3035.0
69.00	2977.0
70.00	164.0
71.90	196.0
73.10	1439.0
74.10	4962.0
75.00	14596.0
76.00	1373.0
76.90	202.0
78.90	947.0
79.90	302.0
80.90	1073.0
81.90	262.0
86.90	1147.0
88.00	1515.0
92.00	718.0
93.00	1085.0
94.00	3257.0
95.10	27272.0
96.00	2040.0
103.90	111.0
105.90	123.0
115.90	113.0
116.90	188.0
118.90	133.0
141.00	190.0
142.90	201.0
174.00	18512.0
175.10	1571.0
176.00	18288.0
177.00	1084.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104