


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021123\
Data File : VU053052.D
Acq On : 11 Feb 2023 16:26
Operator : JC/MD
Sample : BFB196
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB196

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sun Feb 12 22:49:21 2023

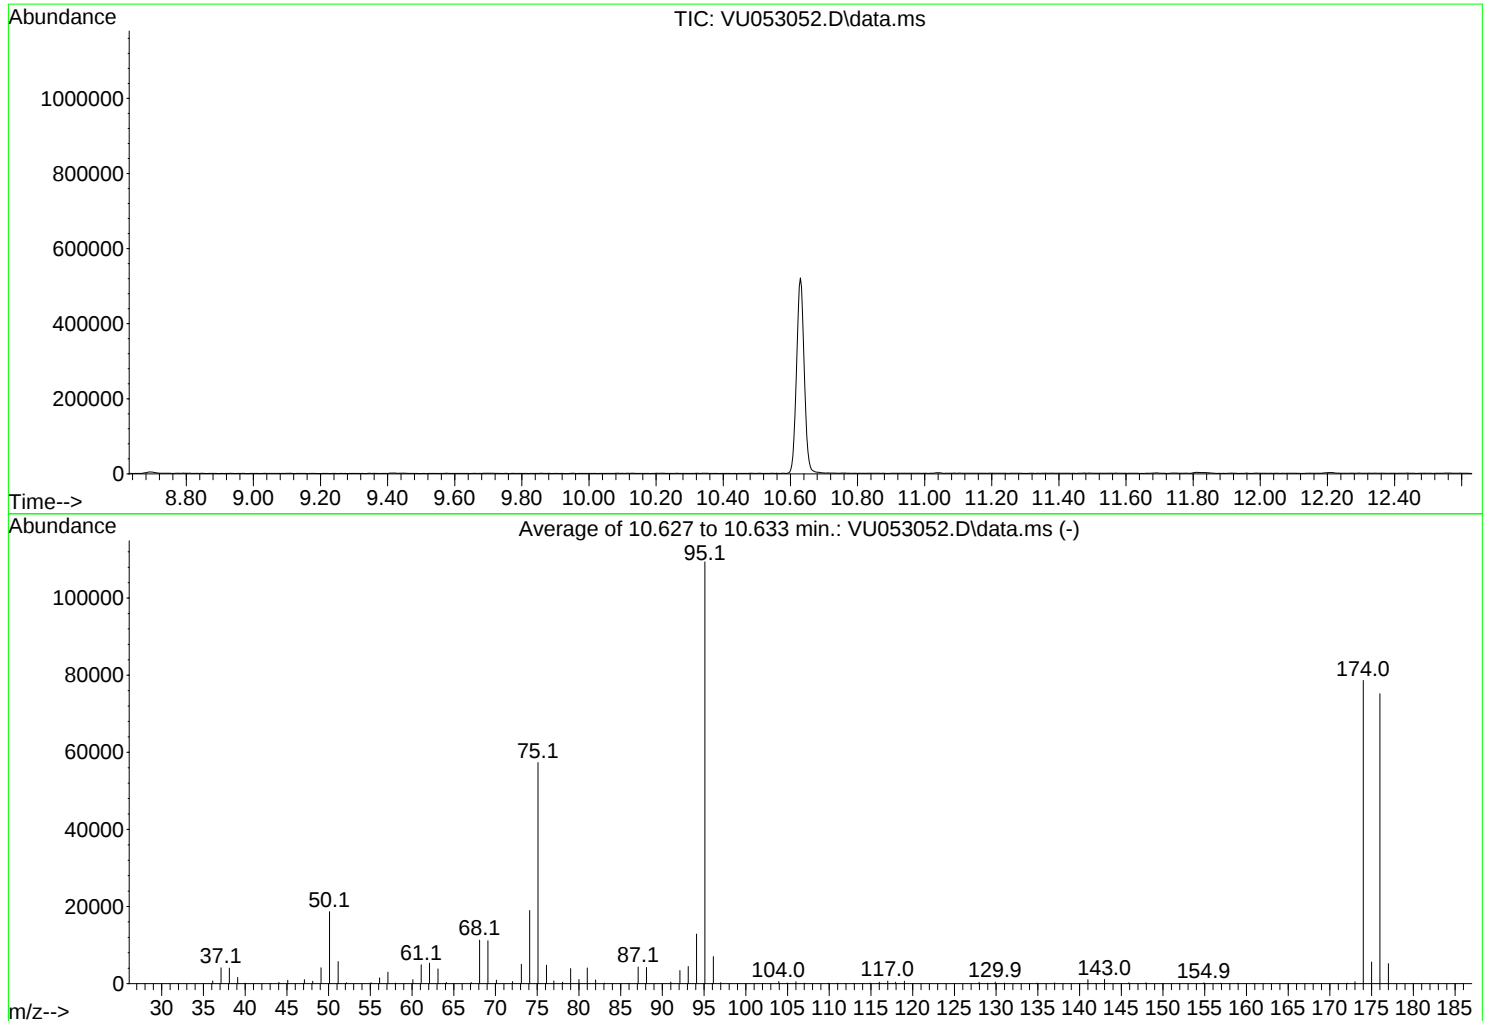

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2951

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	18693	PASS
75	95	30	80	52.4	57357	PASS
95	95	100	100	100.0	109405	PASS
96	95	5	9	6.4	7035	PASS
173	174	0.00	2	0.6	486	PASS
174	95	50	120	71.9	78632	PASS
175	174	5	9	7.1	5609	PASS
176	174	95	101	95.6	75181	PASS
177	176	5	9	6.9	5205	PASS

m/z	Abundance
36.10	137.0
41.10	247.0
43.10	213.0
44.00	392.0
55.10	213.0
56.20	118.0
57.10	172.0
71.10	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB196

m/z	Abundance
36.10	847.0
37.10	4191.0
38.10	3917.0
39.10	1613.0
40.00	129.0
41.10	139.0
43.10	304.0
44.10	704.0
45.10	925.0
47.10	939.0
48.10	618.0
49.10	4169.0
50.10	18656.0
51.20	5750.0
52.20	290.0
55.10	452.0
56.10	1639.0
57.10	3239.0
58.10	175.0
60.10	1073.0
61.10	4864.0
62.10	5390.0
63.10	3728.0
64.10	359.0
67.10	318.0
68.10	11388.0
69.10	11310.0
70.10	916.0
71.10	167.0
72.00	523.0
73.10	5144.0
74.10	18712.0
75.10	57144.0
76.10	4868.0
77.00	741.0
78.00	378.0
79.00	3929.0
80.00	1092.0
81.00	4085.0
82.00	887.0
83.00	174.0
85.90	162.0
87.10	4411.0
88.10	4153.0
91.00	401.0
92.10	3329.0
93.10	4407.0
94.10	12705.0
95.10	108288.0
96.10	7267.0
97.00	209.0
103.90	554.0
104.90	160.0
106.00	496.0
107.10	112.0
109.90	130.0
110.90	110.0
111.90	125.0
112.90	131.0
114.90	120.0
116.00	398.0
117.00	597.0
117.90	410.0
119.00	602.0
127.90	361.0
129.00	138.0
129.90	474.0
131.00	176.0
134.90	153.0
137.00	193.0
141.00	1075.0
141.90	123.0
143.00	1050.0
145.90	219.0
148.00	255.0
154.90	269.0
156.80	107.0
159.00	121.0
160.90	111.0
172.20	123.0
173.00	434.0
174.00	75648.0
175.00	5422.0
176.00	72176.0
177.00	5092.0

Instrument :
MSVOA_U
ClientSampleId :
BFB196

m/z	Abundance
36.10	877.0
37.10	4235.0
38.10	4172.0
39.10	1658.0
40.00	132.0
41.10	147.0
43.10	293.0
44.10	710.0
45.10	908.0
47.10	1045.0
48.10	600.0
49.10	4262.0
50.10	19248.0
51.10	5834.0
52.20	282.0
55.10	461.0
56.10	1620.0
57.10	3267.0
58.00	169.0
60.10	1070.0
61.10	5063.0
62.10	5504.0
63.10	3916.0
64.10	341.0
67.10	312.0
68.10	11715.0
69.10	11343.0
70.10	941.0
71.10	179.0
72.00	535.0
73.10	5203.0
74.10	19528.0
75.10	59536.0
76.10	4841.0
77.00	718.0
78.10	398.0
79.00	4035.0
80.00	1127.0
81.00	4209.0
82.00	970.0
83.00	181.0
85.90	147.0
87.10	4414.0
88.10	4293.0
91.00	451.0
92.10	3514.0
93.10	4550.0
94.10	13315.0
95.10	112856.0
96.10	7201.0
97.00	249.0
103.90	562.0
104.90	167.0
106.00	505.0
107.00	126.0
109.90	135.0
110.90	115.0
113.00	114.0
114.90	160.0
116.00	403.0
117.00	681.0
117.90	388.0
119.00	663.0
127.90	382.0
129.00	135.0
129.90	435.0
131.00	163.0
134.90	164.0
137.00	205.0
141.00	1062.0
141.90	107.0
143.00	1145.0
145.90	256.0
148.00	260.0
154.90	261.0
156.90	101.0
159.00	136.0
160.90	106.0
172.10	111.0
173.00	503.0
174.00	81256.0
175.00	5781.0
176.00	77576.0
177.00	5372.0

Instrument :
MSVOA_U
ClientSampleId :
BFB196

m/z	Abundance
36.10	854.0
37.10	3935.0
38.10	3964.0
39.10	1543.0
40.00	111.0
41.10	157.0
43.10	266.0
44.10	725.0
45.10	794.0
47.10	1134.0
48.10	601.0
49.10	3938.0
50.10	18176.0
51.10	5559.0
52.10	239.0
55.10	440.0
56.10	1527.0
57.10	3017.0
58.00	149.0
60.10	980.0
61.10	4761.0
62.10	5050.0
63.10	3783.0
64.10	326.0
67.10	300.0
68.10	10759.0
69.10	10704.0
70.10	884.0
71.00	188.0
72.10	569.0
73.10	4748.0
74.10	18696.0
75.10	55392.0
76.10	4577.0
77.00	641.0
78.10	354.0
79.00	3761.0
80.00	1080.0
81.00	3943.0
82.00	964.0
83.10	163.0
87.10	4148.0
88.10	4087.0
91.00	451.0
92.10	3344.0
93.10	4386.0
94.10	12552.0
95.10	107072.0
96.10	6637.0
97.00	269.0
104.00	506.0
105.00	139.0
106.00	473.0
107.00	148.0
109.90	101.0
111.00	135.0
114.90	186.0
116.00	366.0
117.00	724.0
118.00	378.0
119.00	623.0
128.00	357.0
129.00	150.0
129.90	332.0
131.00	147.0
134.90	161.0
137.00	186.0
141.00	990.0
143.00	1147.0
145.90	247.0
147.90	242.0
150.00	103.0
154.90	239.0
156.90	129.0
159.00	115.0
172.00	119.0
173.00	522.0
174.00	78992.0
175.00	5625.0
176.00	75792.0
177.00	5150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB196