

Data File : VU029431.D
Acq On : 12 Feb 2019 19:42
Operator : JC/SP
Sample : K1436-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESXB2

Quant Time: Feb 13 03:31:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Feb 13 03:26:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	202607	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	191584	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	103834	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	63821	4.69	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.80%
7) Chloroethane-d5	1.68	69	59947	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.80%
11) 1,1-Dichloroethene-d2	2.27	63	106291	3.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.80%
20) 2-Butanone-d5	4.21	46	138286	48.86	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.72%
24) Chloroform-d	4.65	84	85455	3.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.00%
26) 1,2-Dichloroethane-d4	5.31	65	54503	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
32) Benzene-d6	5.34	84	230102	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.33	67	66068	4.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.00%
41) Toluene-d8	7.56	98	216319	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
43) trans-1,3-Dichloropropene-	7.85	79	25016	4.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.20%
46) 2-Hexanone-d5	8.31	63	147356	52.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.26%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	56786	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	96284	5.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.60%

Target Compounds

					Qvalue	
10) 1,1,2-Trichloro-1,2,2-trif	2.27	101	994	0.056	ug/L #	17
12) 1,1-Dichloroethene	2.27	96	1365	0.082	ug/L #	1
13) Acetone	2.35	43	47920	18.637	ug/L	97
15) Methyl Acetate	2.35	43	43501	6.604	ug/L #	47
21) 2-Butanone	4.31	43	7292	2.295	ug/L	77
25) Chloroform	4.67	83	20295	0.757	ug/L	94
33) Benzene	5.39	78	55788	0.989	ug/L	100
37) 1,2-Dichloropropane	6.33	63	7607	0.539	ug/L #	87
39) cis-1,3-Dichloropropene	7.22	75	1677	0.075	ug/L	83
42) Toluene	7.64	91	55071	0.870	ug/L	99
48) 2-Hexanone	8.37	43	4952	0.835	ug/L #	86
52) Ethylbenzene	9.25	91	4219	0.059	ug/L	89
53) m,p-xylene	9.38	106	4937	0.173	ug/L	98
54) o-xylene	9.78	106	3039	0.108	ug/L	87
59) 1,2,3-Trichloropropane	11.48	75	10146	1.120	ug/L	88
69) Naphthalene	13.75	128	3936	0.089	ug/L #	91

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU021219\
Quantitation Report (Not Reviewed)

Data File : VU029431.D
Acq On : 12 Feb 2019 19:42
Operator : JC/SP
Sample : K1436-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESXB2

Quant Time: Feb 13 03:31:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Feb 13 03:26:10 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU029431.D
Acq On : 12 Feb 2019 19:42
Operator : JC/SP
Sample : K1436-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESXB2

Quant Time: Feb 13 03:31:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Feb 13 03:26:10 2019
Response via : Initial Calibration

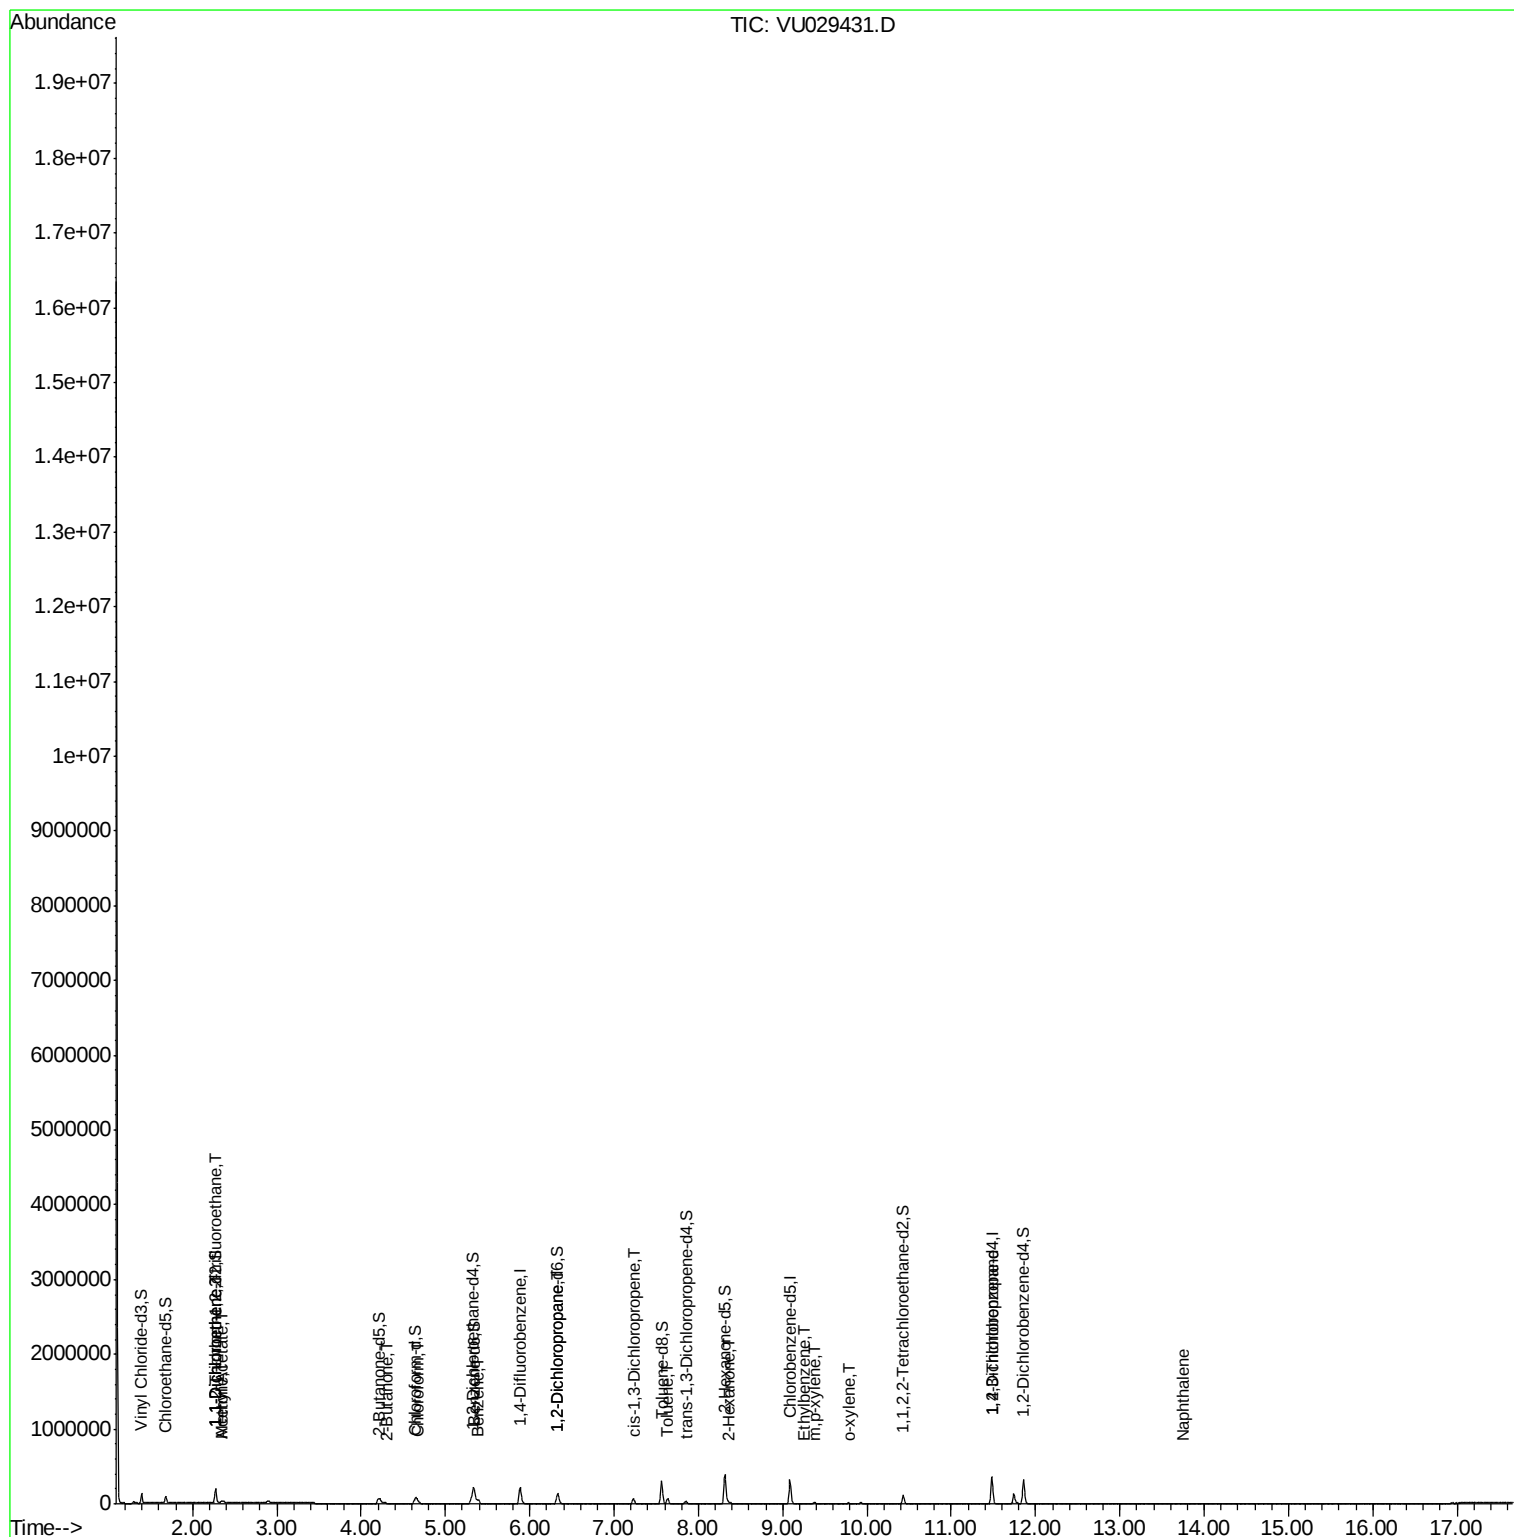

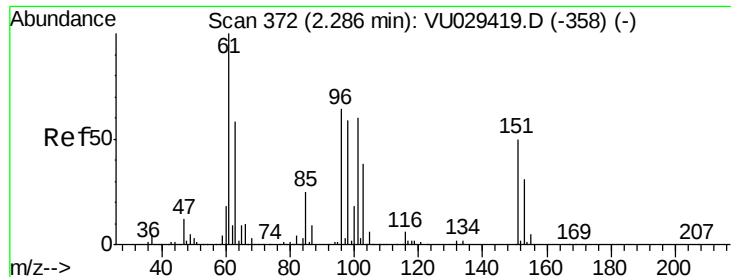

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.056 ug/L

RT: 2.27 min Scan# 368

Delta R.T. -0.01 min

Lab File: VU029431.D

Acq: 12 Feb 2019 19:42

Instrument :

MSVOA_U

ClientSampleId :

ESXB2


Tgt Ion: 101 Resp: 994

Ion Ratio Lower Upper

101 100

85 2.0 35.1 52.7#




151 0.0 67.0 100.6#

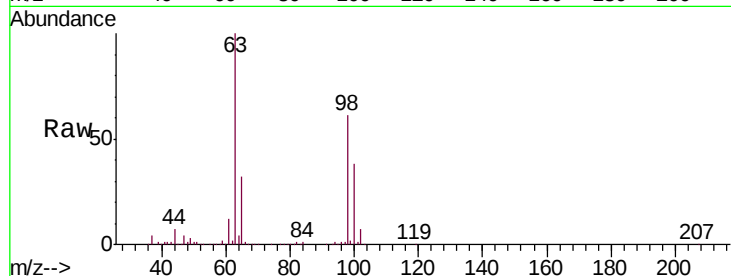

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VU0

Ion 151.00 (150.70 to 151.70): V

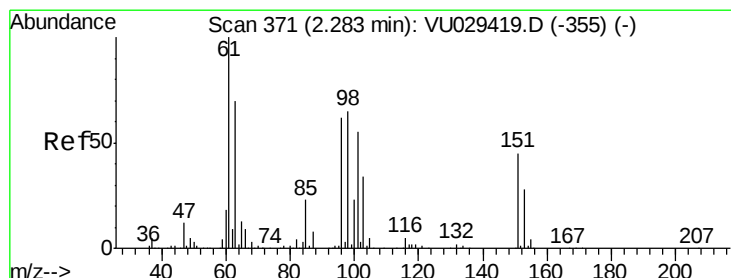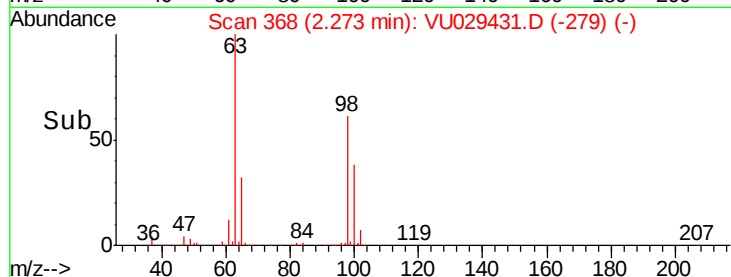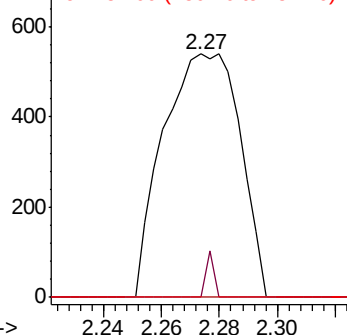

#12

1,1-Dichloroethene

Concen: 0.082 ug/L

RT: 2.27 min Scan# 368

Delta R.T. -0.01 min

Lab File: VU029431.D

Acq: 12 Feb 2019 19:42


Tgt Ion: 96 Resp: 1365

Ion Ratio Lower Upper

96 100

61 1083.6 115.1 213.7#



63 8925.1 83.5 155.1#

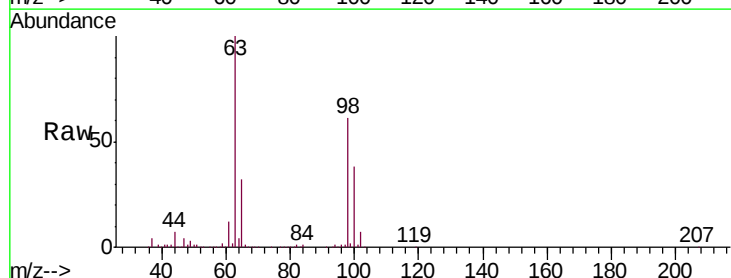


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 63.00 (62.70 to 63.70): VU0

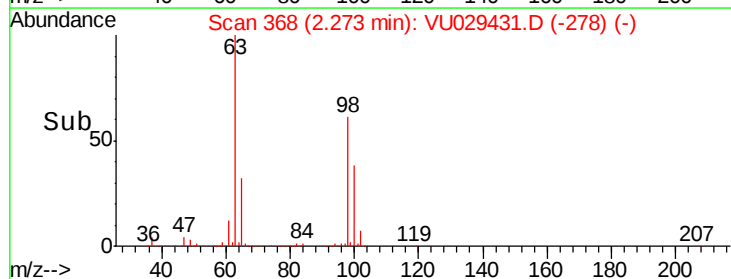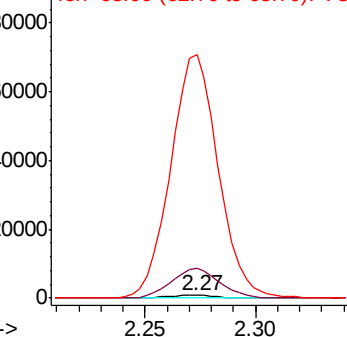

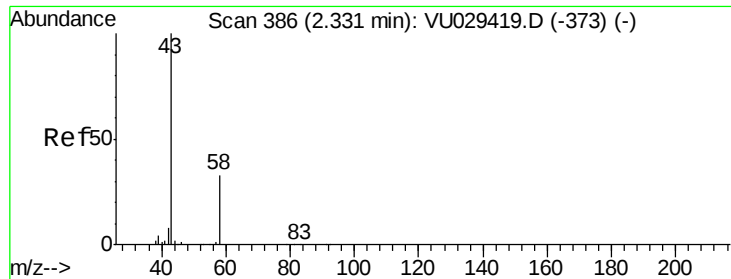

#13

Acetone

Concen: 18.637 ug/L

RT: 2.35 min Scan# 391

Delta R.T. 0.02 min

Lab File: VU029431.D

Acq: 12 Feb 2019 19:42

Instrument :

MSVOA_U

ClientSampleId :





ESXB2

Tgt Ion: 43 Resp: 47920

Ion Ratio Lower Upper

43 100

58 34.2 0.0 65.0

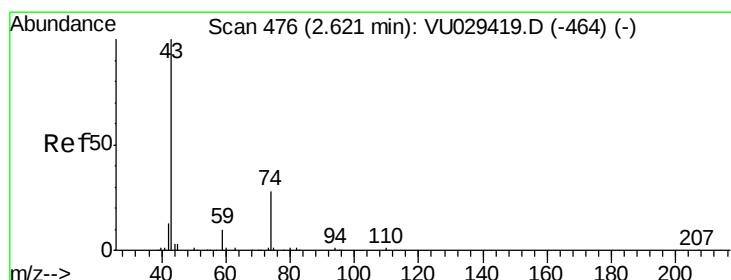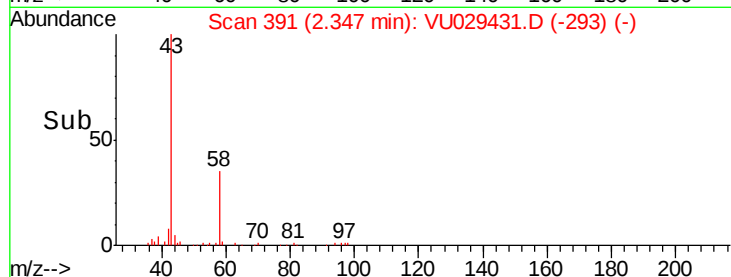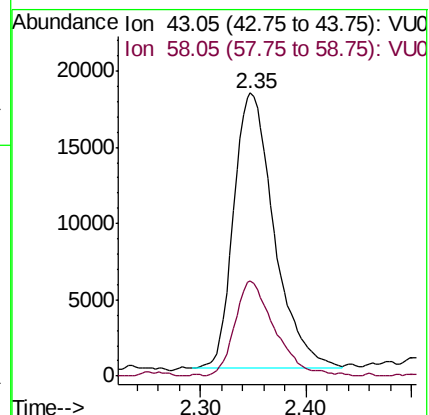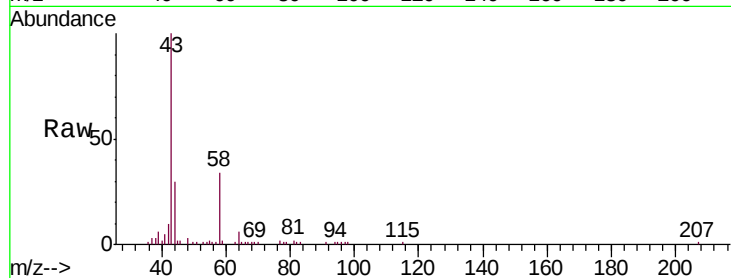

#15

Methyl Acetate

Concen: 6.604 ug/L

RT: 2.35 min Scan# 391

Delta R.T. -0.27 min

Lab File: VU029431.D




Acq: 12 Feb 2019 19:42


Tgt Ion: 43 Resp: 43501

Ion Ratio Lower Upper

43 100

74 0.0 22.3 33.5#

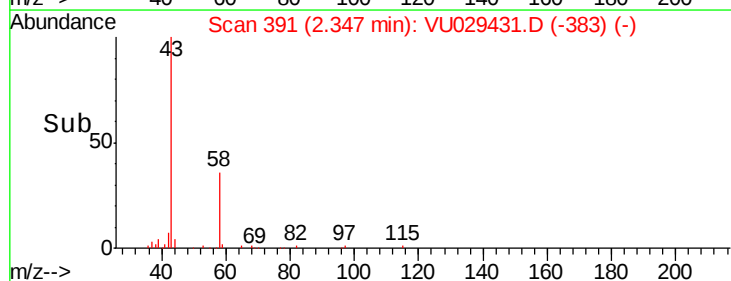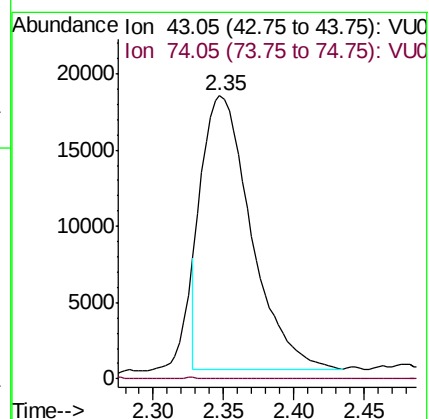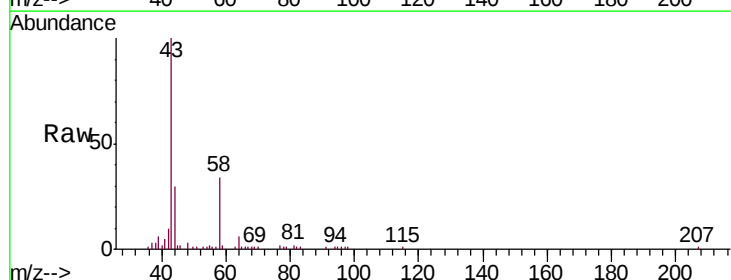

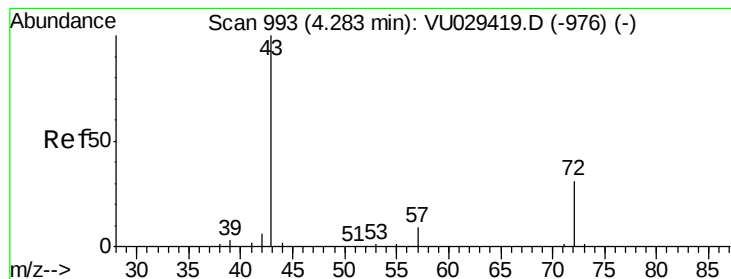

#21

2-Butanone

Concen: 2.295 ug/L

RT: 4.31 min Scan# 1001

Delta R.T. 0.03 min

Lab File: VU029431.D

Acq: 12 Feb 2019 19:42

Instrument :

MSVOA_U

ClientSampled :





ESXB2

Tgt Ion: 43 Resp: 7292

Ion Ratio Lower Upper

43 100

72 17.3 14.7 44.1

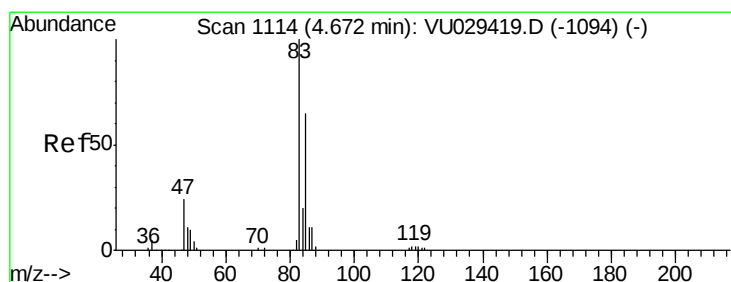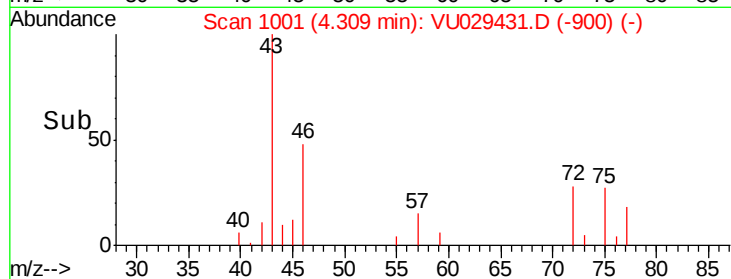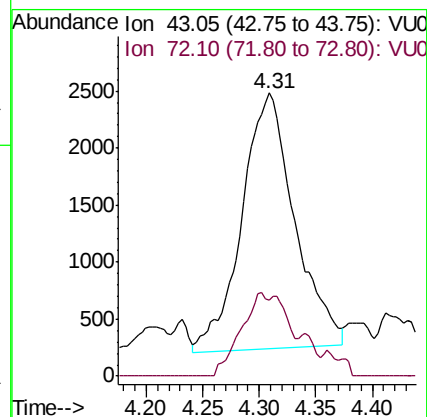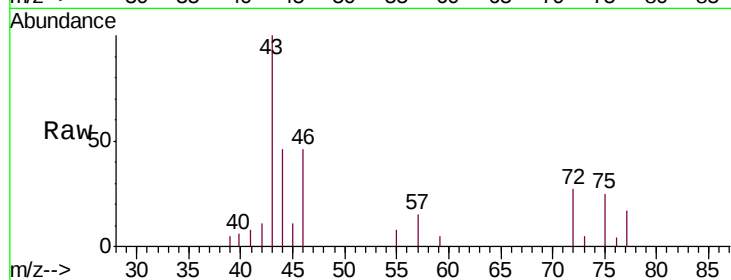

#25

Chloroform

Concen: 0.757 ug/L

RT: 4.67 min Scan# 1114

Delta R.T. 0.00 min

Lab File: VU029431.D




Acq: 12 Feb 2019 19:42


Tgt Ion: 83 Resp: 20295

Ion Ratio Lower Upper

83 100

85 63.8 47.8 88.8

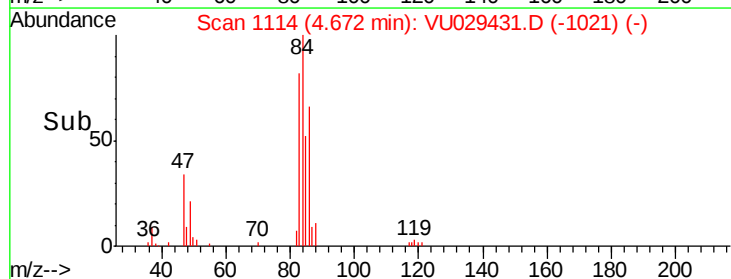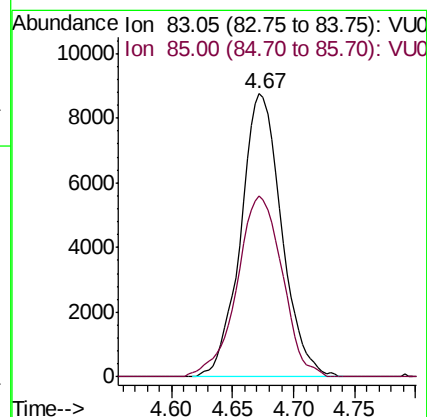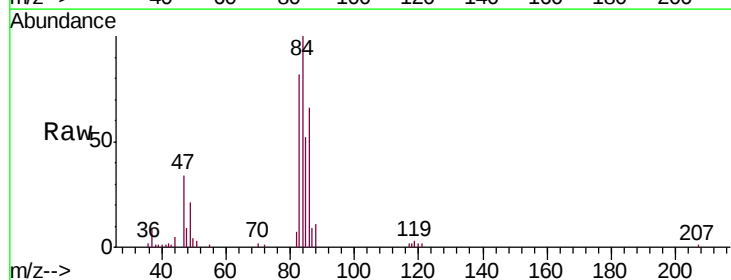

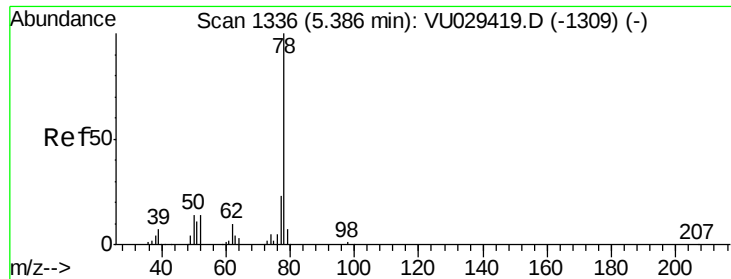

#33

Benzene

Concen: 0.989 ug/L

RT: 5.39 min Scan# 1336

Delta R.T. 0.00 min

Lab File: VU029431.D

Acq: 12 Feb 2019 19:42


Instrument :

MSVOA_U




ClientSampleId :

ESXB2

Tgt Ion: 78 Resp: 55788

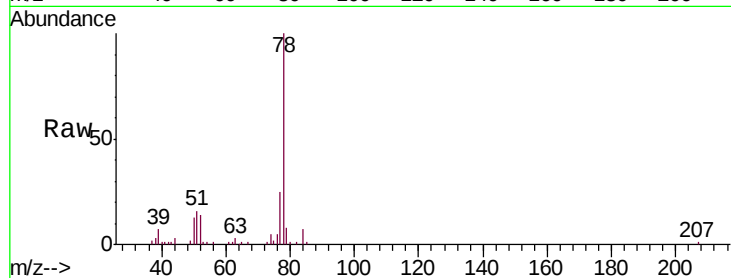

Abundance Ion 78.10 (77.80 to 78.80): VU0

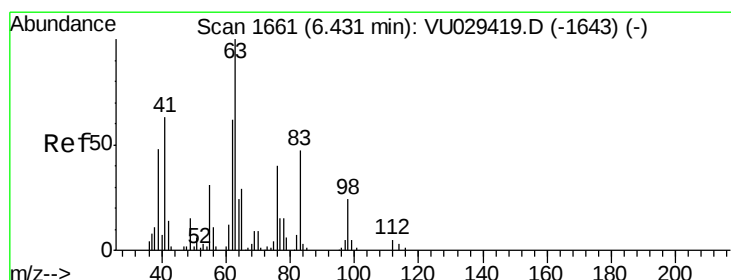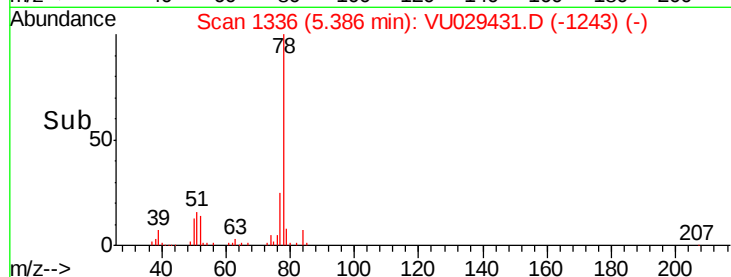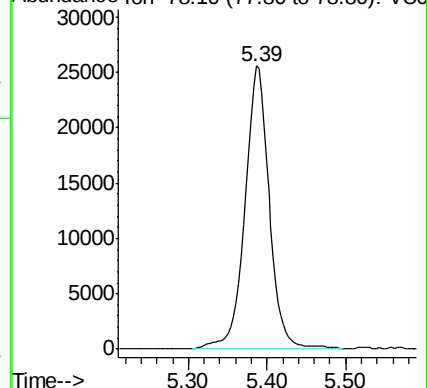

#37

1,2-Dichloropropane

Concen: 0.539 ug/L

RT: 6.33 min Scan# 1630

Delta R.T. -0.10 min

Lab File: VU029431.D


Acq: 12 Feb 2019 19:42

Tgt Ion: 63 Resp: 7607



Ion Ratio Lower Upper


63 100

112 0.0 3.5 5.3#

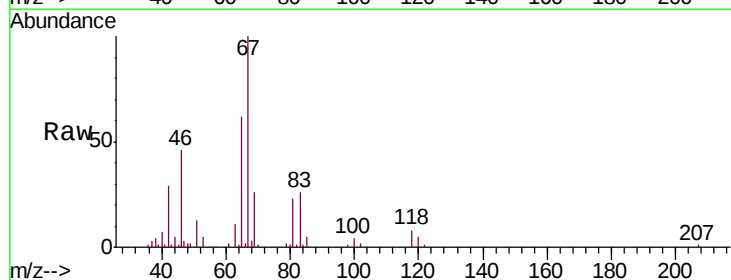

Abundance Ion 63.10 (62.80 to 63.80): VU0



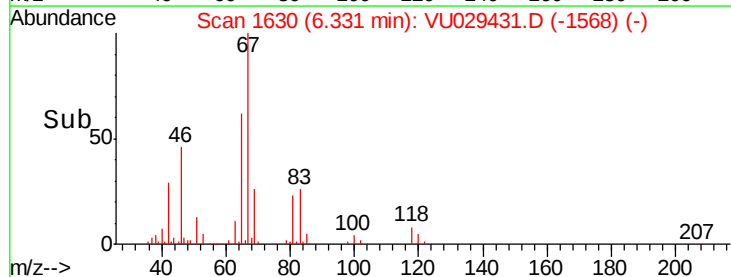
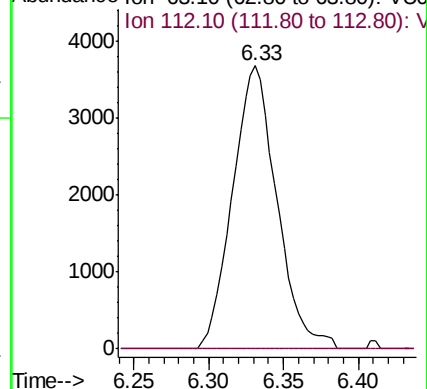


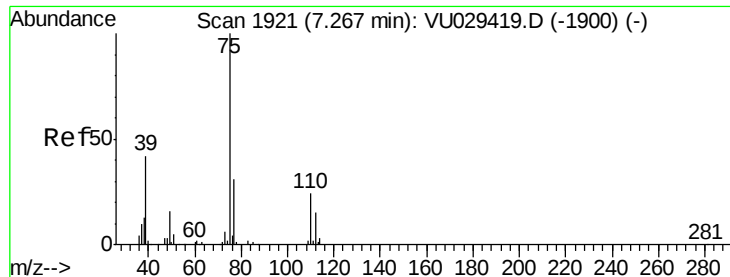

#39
 cis-1,3-Dichloropropene
 Concen: 0.075 ug/L
 RT: 7.22 min Scan# 1908
 Delta R.T. -0.04 min
 Lab File: VU029431.D
 Acq: 12 Feb 2019 19:42




Instrument :
 MSVOA_U
 ClientSampleId :
 ESXB2


Tgt Ion: 75 Resp: 1677
 Ion Ratio Lower Upper
 75 100
 77 41.3 22.3 41.3

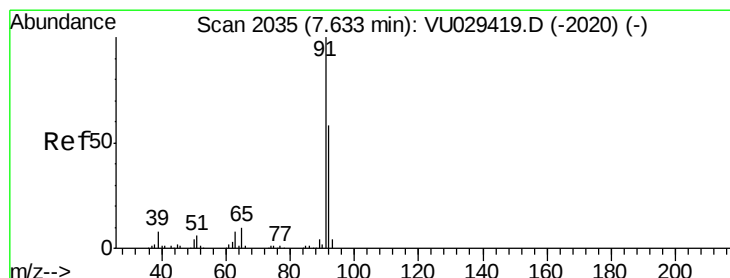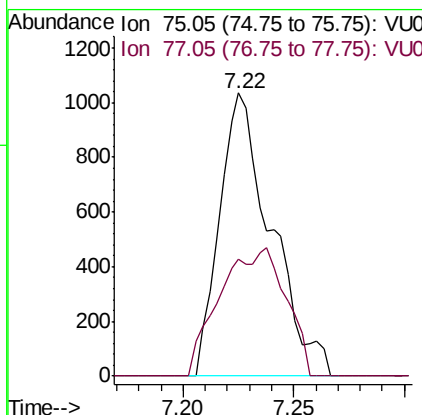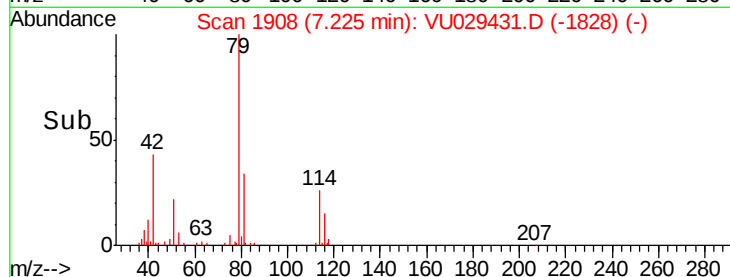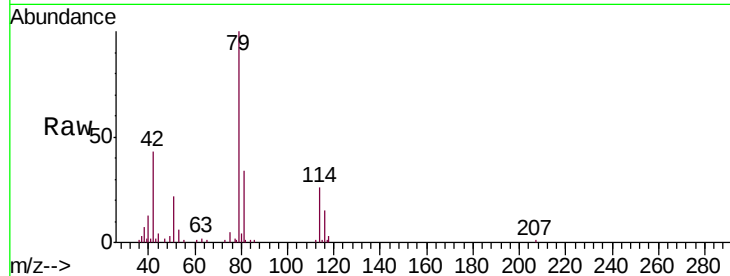

#42
 Toluene
 Concen: 0.870 ug/L
 RT: 7.64 min Scan# 2036
 Delta R.T. 0.00 min
 Lab File: VU029431.D
 Acq: 12 Feb 2019 19:42

Tgt Ion: 91 Resp: 55071
 Ion Ratio Lower Upper
 91 100
 92 57.6 39.8 73.8

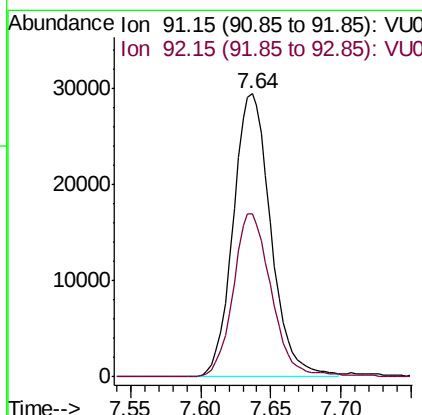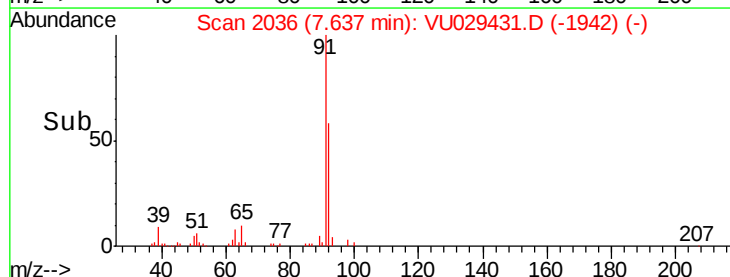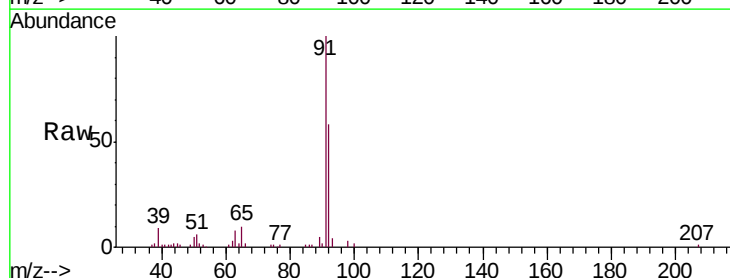


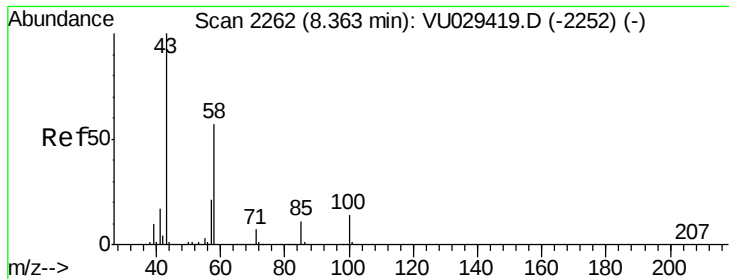




#48
2-Hexanone
Concen: 0.835 ug/L
RT: 8.37 min Scan# 2264
Delta R.T. 0.01 min
Lab File: VU029431.D
Acq: 12 Feb 2019 19:42

Instrument :
MSVOA_U
ClientSampleId :
ESXB2

Tgt Ion: 43 Resp: 4952
Ion Ratio Lower Upper
43 100
58 49.2 45.7 68.5
57 12.4 16.4 24.6#
100 5.9 11.1 16.7#

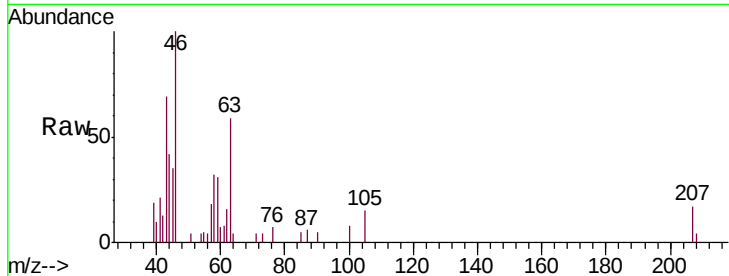


Abundance Ion 43.05 (42.75 to 43.75): VU0
Ion 58.05 (57.75 to 58.75): VU0
Ion 57.20 (56.90 to 57.90): VU0
Ion 100.15 (99.85 to 100.85): VU0

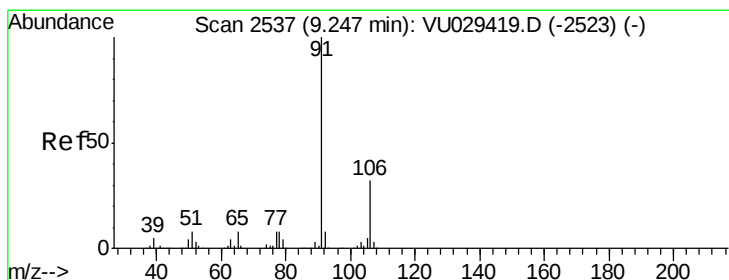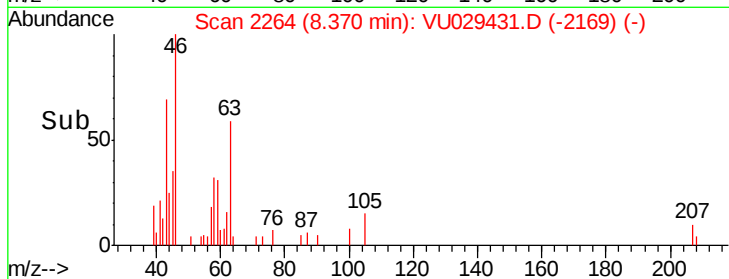
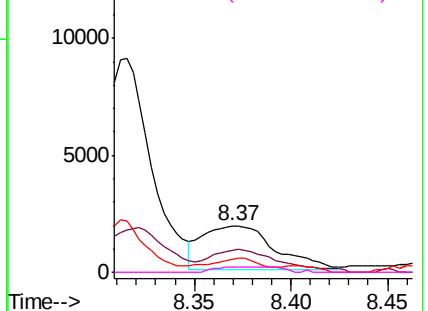



#52
Ethylbenzene
Concen: 0.059 ug/L
RT: 9.25 min Scan# 2538
Delta R.T. 0.00 min
Lab File: VU029431.D
Acq: 12 Feb 2019 19:42

Tgt Ion: 91 Resp: 4219
Ion Ratio Lower Upper
91 100
106 38.9 22.8 42.4

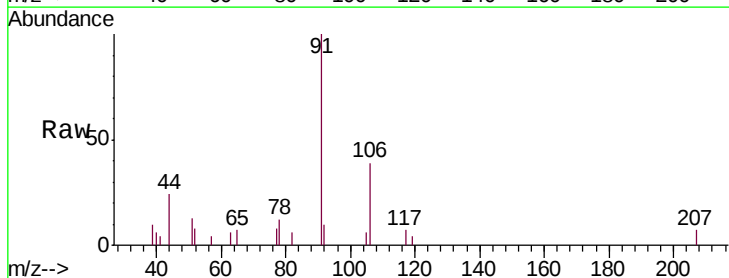

Abundance Ion 91.15 (90.85 to 91.85): VU0
Ion 106.15 (105.85 to 106.85): VU0

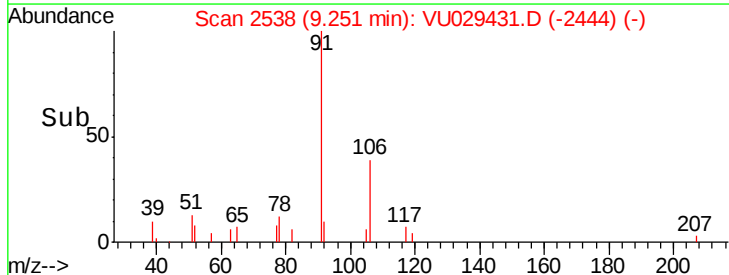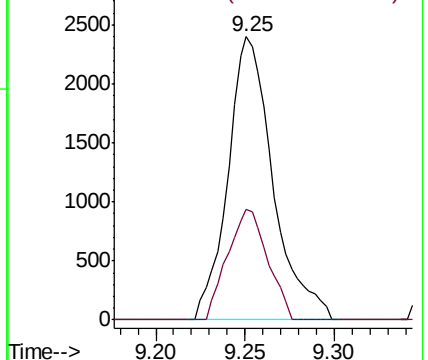

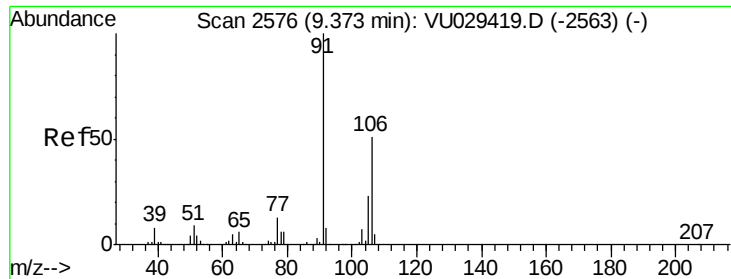

#53

m,p-xylene

Concen: 0.173 ug/L

RT: 9.38 min Scan# 2577

Delta R.T. 0.00 min

Lab File: VU029431.D

Acq: 12 Feb 2019 19:42

Instrument :

MSVOA_U

ClientSampleId :


ESXB2

Tgt Ion:106 Resp: 4937




Ion Ratio Lower Upper

106 100

91 196.9 135.7 251.9

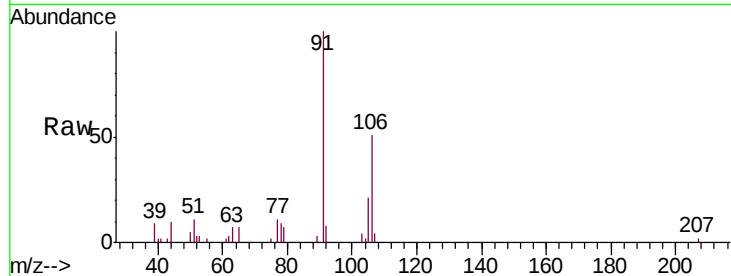

Abundance Ion 106.15 (105.85 to 106.85): V

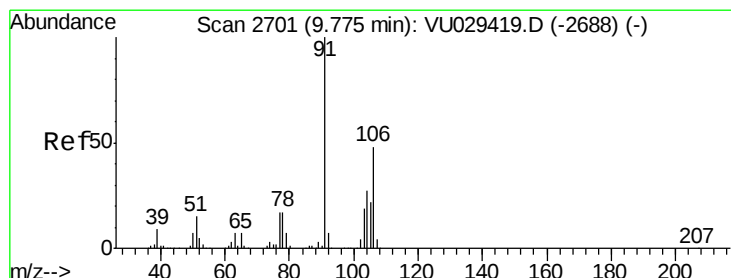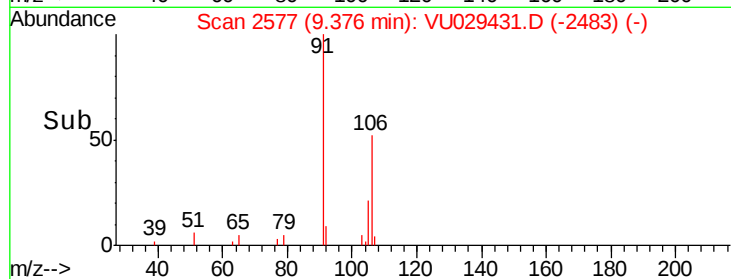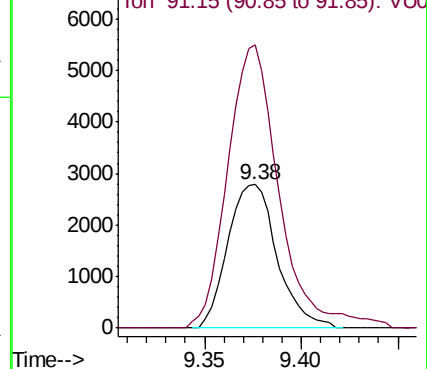

#54

o-xylene

Concen: 0.108 ug/L

RT: 9.78 min Scan# 2702

Delta R.T. 0.00 min

Lab File: VU029431.D


Acq: 12 Feb 2019 19:42

Tgt Ion:106 Resp: 3039



Ion Ratio Lower Upper


106 100

91 187.9 145.1 269.5

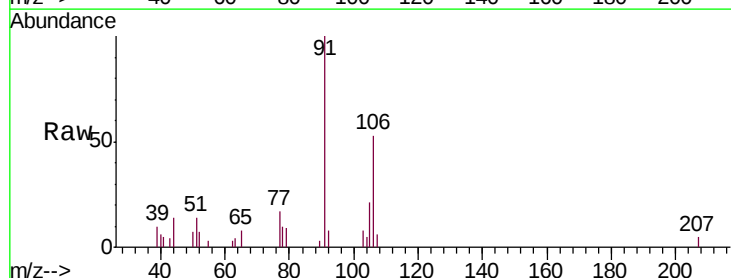

Abundance Ion 106.15 (105.85 to 106.85): V



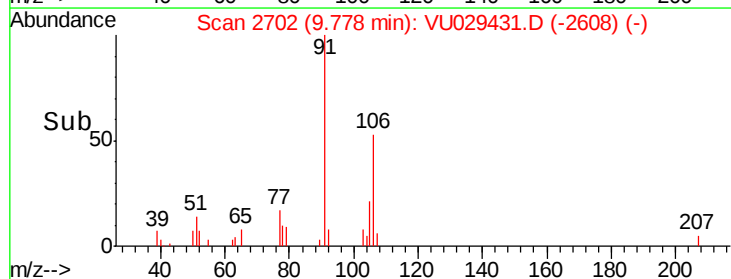
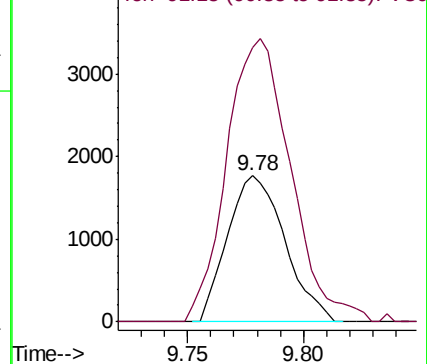


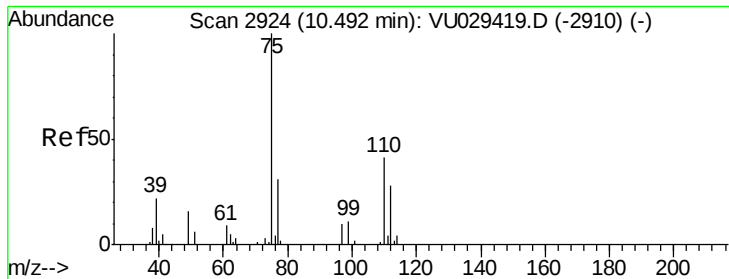

#59
 1,2,3-Trichloropropane
 Concen: 1.120 ug/L
 RT: 11.48 min Scan# 3232
 Delta R.T. 0.99 min
 Lab File: VU029431.D
 Acq: 12 Feb 2019 19:42

Instrument :
 MSVOA_U
 ClientSampleId :
 ESXB2

Tgt Ion: 75 Resp: 10146
 Ion Ratio Lower Upper
 75 100
 77 42.0 28.2 42.2

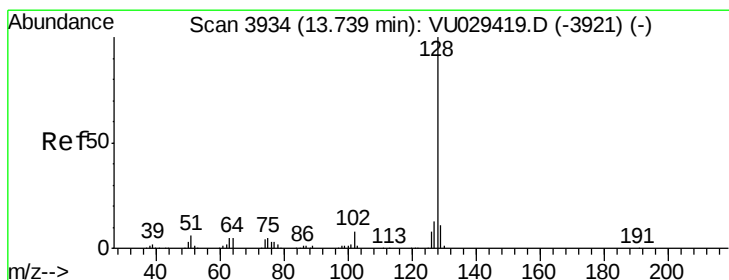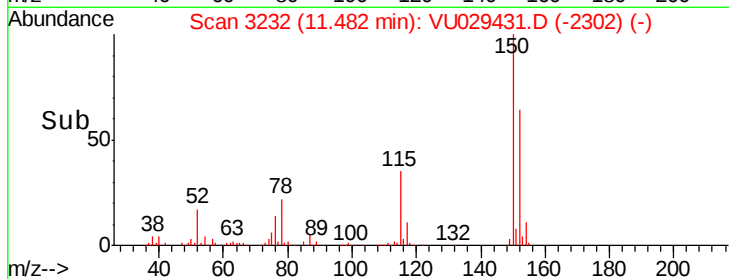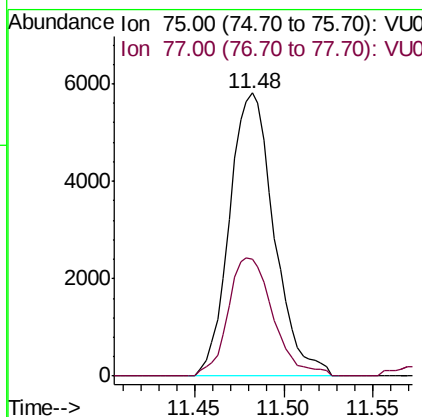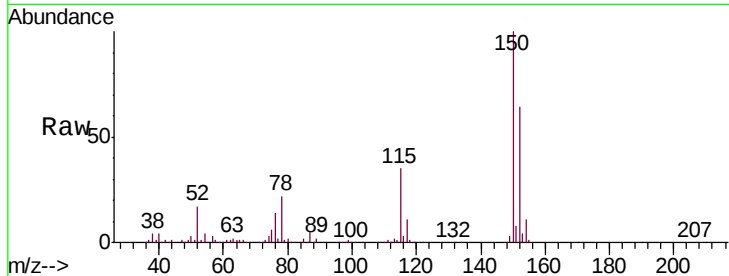

#69
 Naphthalene
 Concen: 0.089 ug/L
 RT: 13.75 min Scan# 3937
 Delta R.T. 0.01 min
 Lab File: VU029431.D
 Acq: 12 Feb 2019 19:42

Tgt Ion: 128 Resp: 3936
 Ion Ratio Lower Upper
 128 100
 129 8.8 8.7 13.1
 127 8.5 10.3 15.5#

