

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021219\
 Data File : VU029428.D
 Acq On : 12 Feb 2019 18:31
 Operator : JC/SP
 Sample : K1436-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESXA9

Quant Time: Feb 13 13:51:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Feb 13 03:26:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	207436	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	194879	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	102541	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	66076	4.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.80%
7) Chloroethane-d5	1.68	69	57356	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.20%
11) 1,1-Dichloroethene-d2	2.27	63	104696	3.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.20%
20) 2-Butanone-d5	4.19	46	138446	47.78	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.56%
24) Chloroform-d	4.65	84	105864	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.31	65	55915	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.34	84	228912	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.33	67	68217	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.56	98	222583	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
43) trans-1,3-Dichloropropene-	7.85	79	26307	4.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.00%
46) 2-Hexanone-d5	8.31	63	137422	48.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.52%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	55471	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	94435	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	4549	1.728 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU021219\
Data File : VU029428.D
Acq On : 12 Feb 2019 18:31
Operator : JC/SP
Sample : K1436-16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESXA9

Quant Time: Feb 13 13:51:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Feb 13 03:26:10 2019
Response via : Initial Calibration

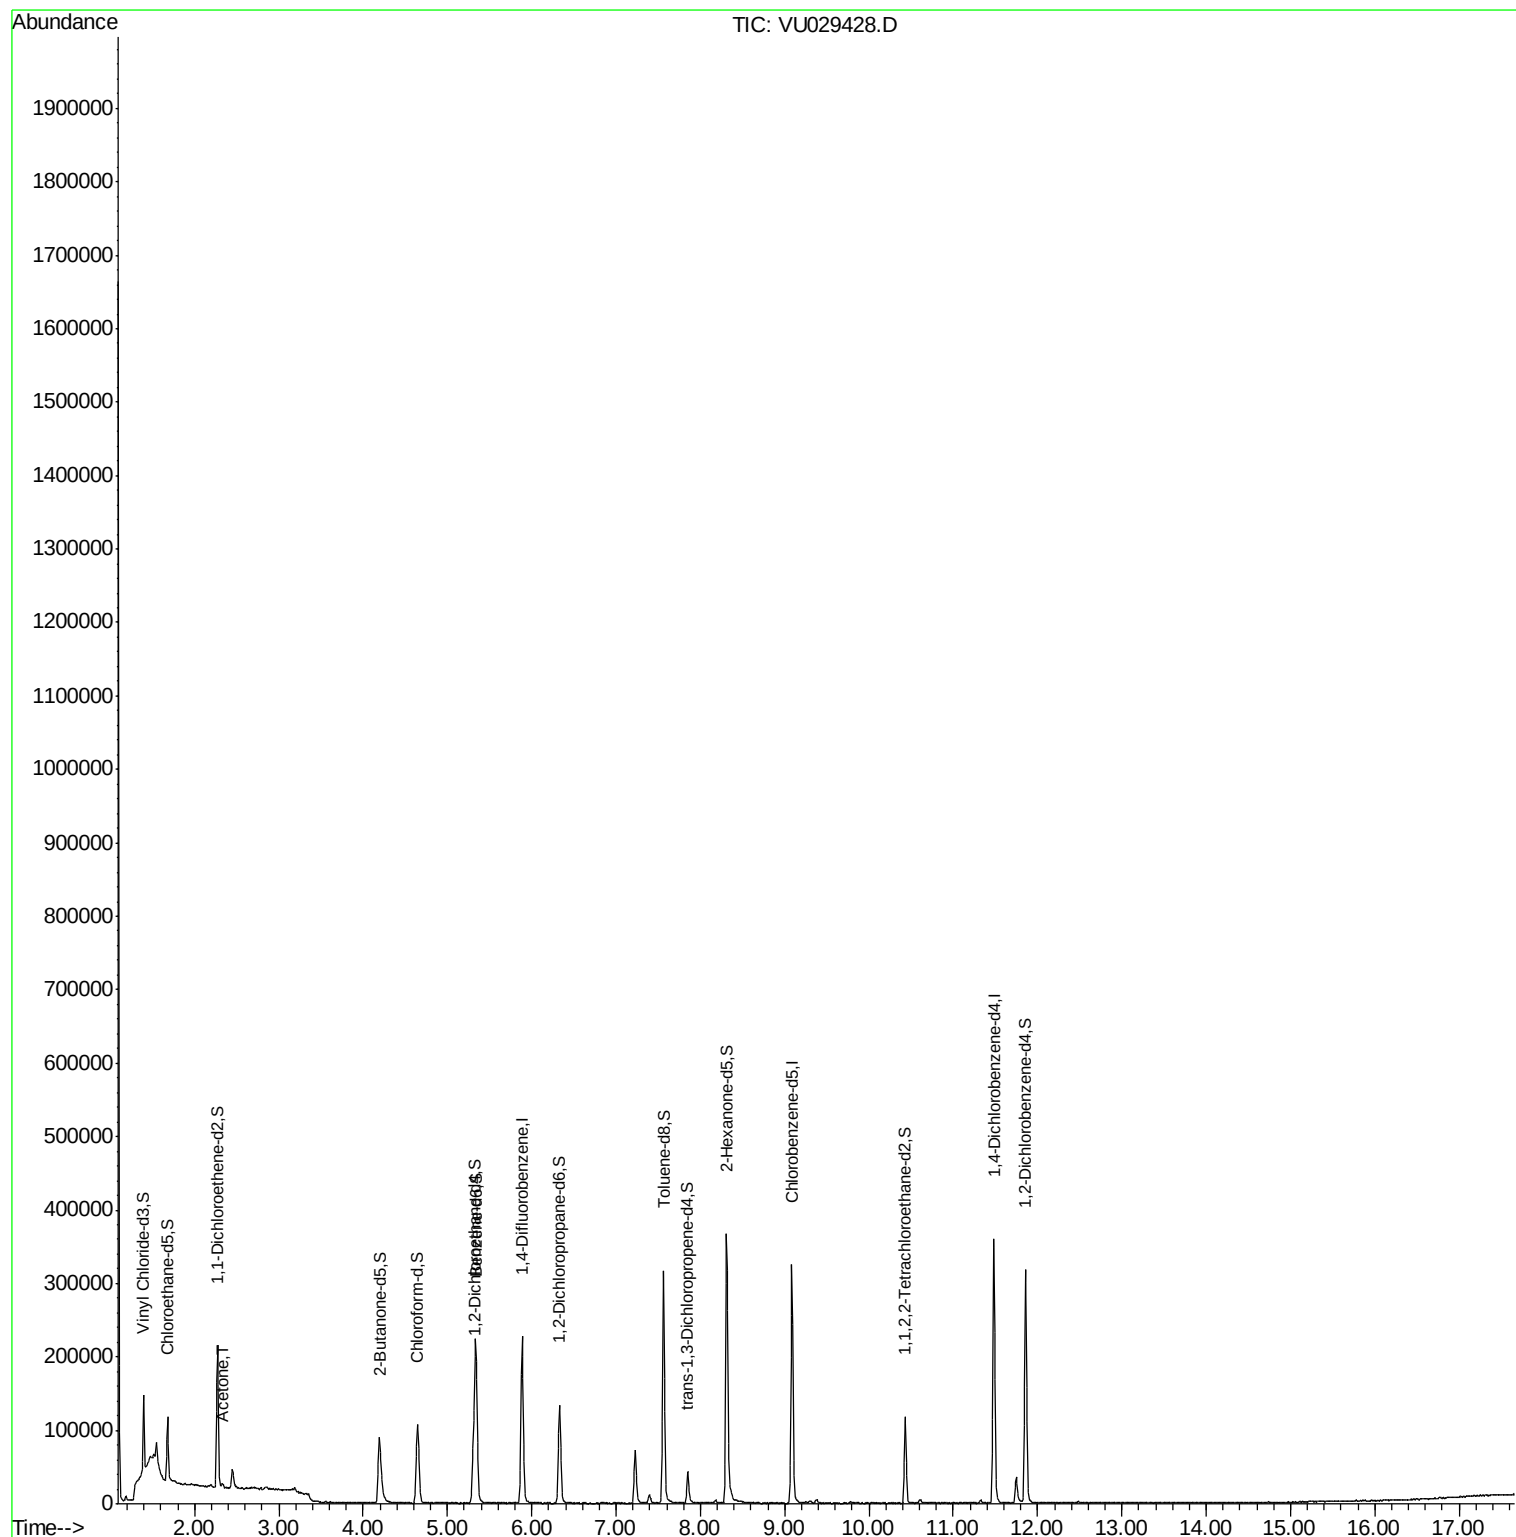

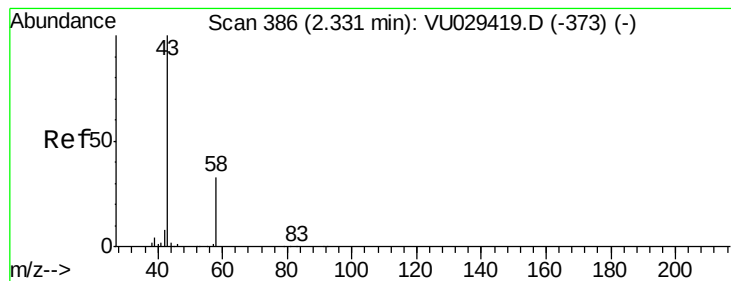

#13

Acetone

Concen: 1.728 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.01 min

Lab File: VU029428.D

Acq: 12 Feb 2019 18:31

Instrument :
MSVOA_U
ClientSampleId :
ESXA9

Tot Ion: 43 Resp: 4549

Ion Ratio Lower Upper

43 100

58 37.3 0.0 65.0

